

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022719\
 Data File : PP029180.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 27 Feb 2019 19:07
 Operator : EI\MA
 Sample : K1348-08
 Misc : hexane
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 OK-02-022519

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 28 03:36:59 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022119.M
 Quant Title : 8080.M
 QLast Update : Fri Feb 22 02:24:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.937	12.126	13138112	17693641	437.116	466.205
Target Compounds							
8) T	DICHLORPROP	0.000	13.561	0	585150	N.D.	17.308 #
12) T	2,4,5-T	0.000	15.846	0	2706503	N.D.	16.346 #
13) T	2,4-DB	16.244	0.000	10743005	0	562.393	N.D. #
15) T	Picloram	17.496	0.000	46991390	0	169.003	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022719\
Data File : PP029180.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 27 Feb 2019 19:07
Operator : EI\MA
Sample : K1348-08
Misc : hexane
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :
OK-02-022519

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 28 03:36:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022119.M
Quant Title : 8080.M
QLast Update : Fri Feb 22 02:24:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

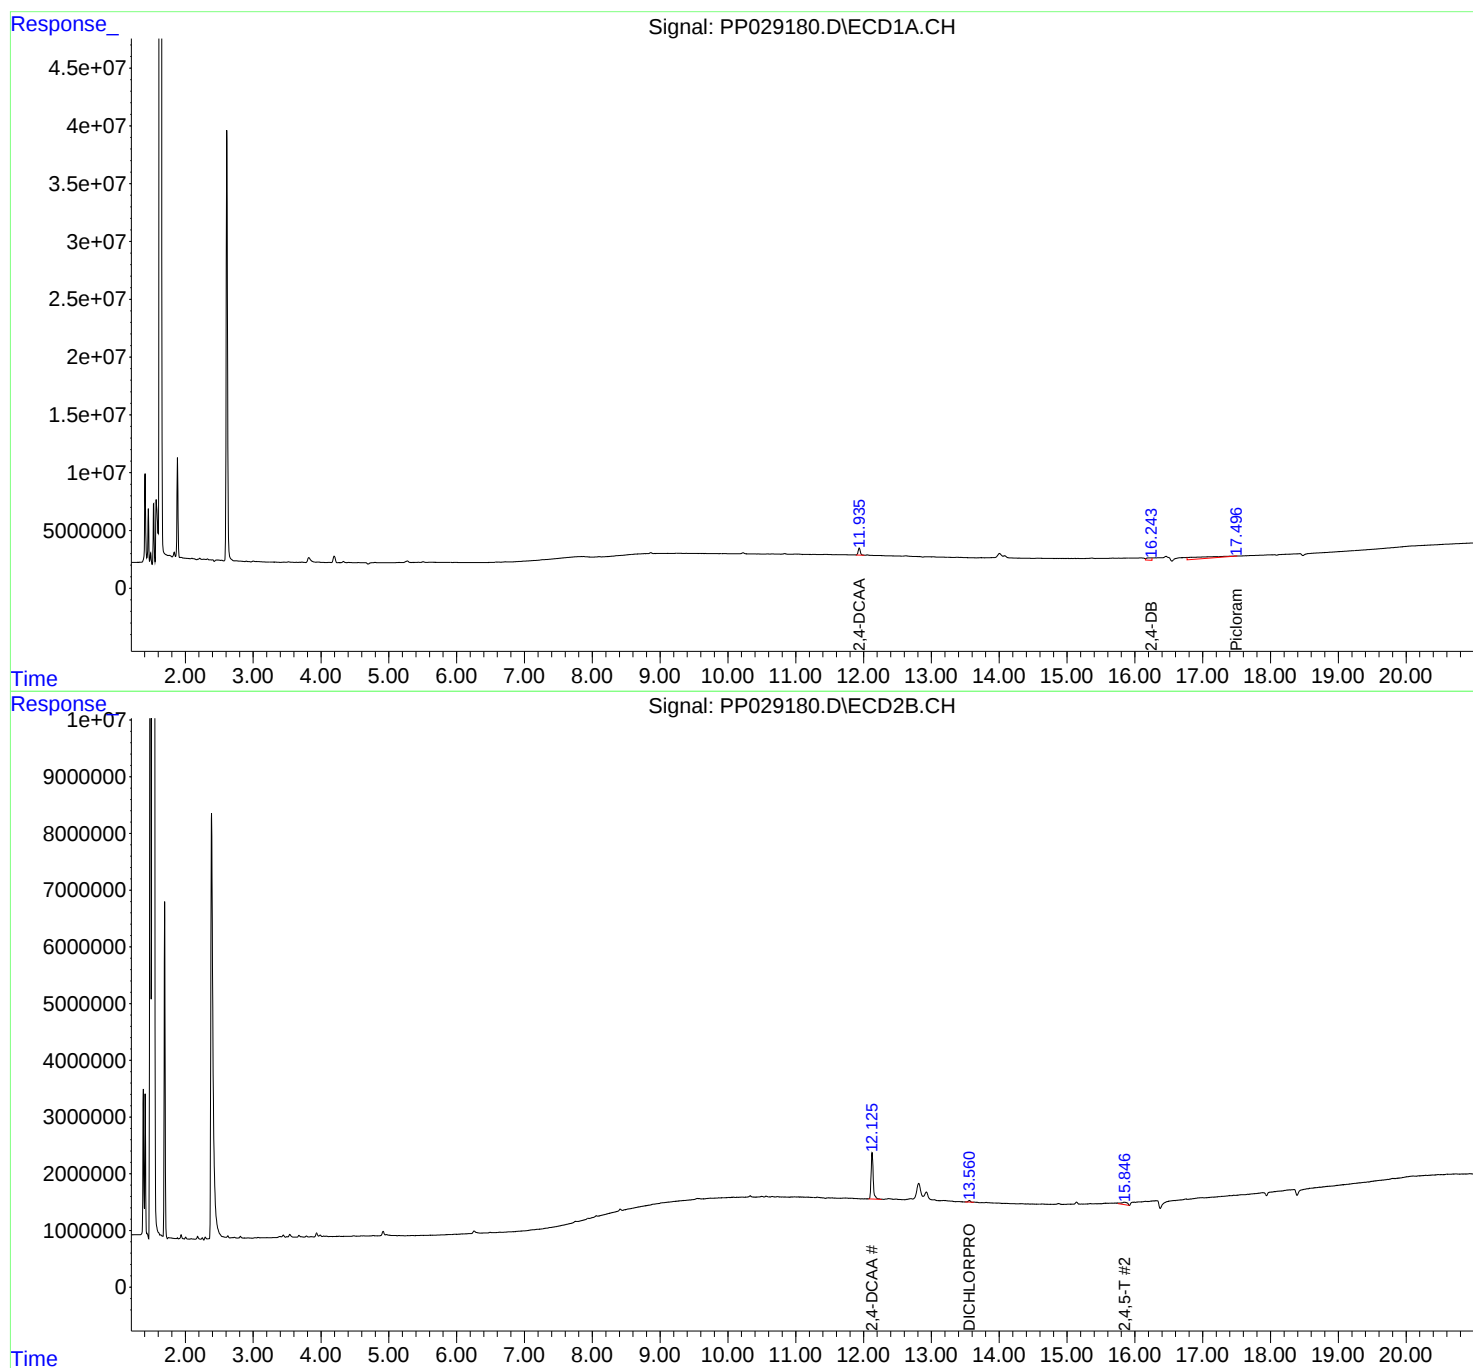


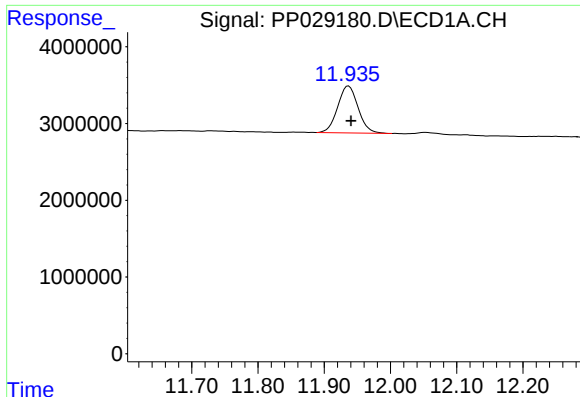

#4 2,4-DCAA


R.T.: 11.937 min
Delta R.T.: -0.004 min
Response: 13138112
Conc: 437.12 ng/ml

Instrument :
ECD_P
ClientSampleId :
OK-02-022519

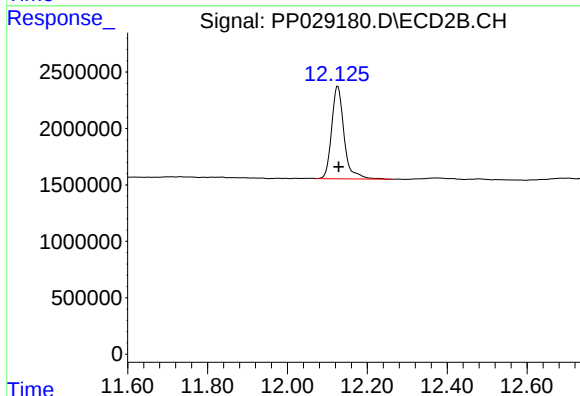


#4 2,4-DCAA

R.T.: 12.126 min
Delta R.T.: -0.002 min
Response: 17693641
Conc: 466.20 ng/ml

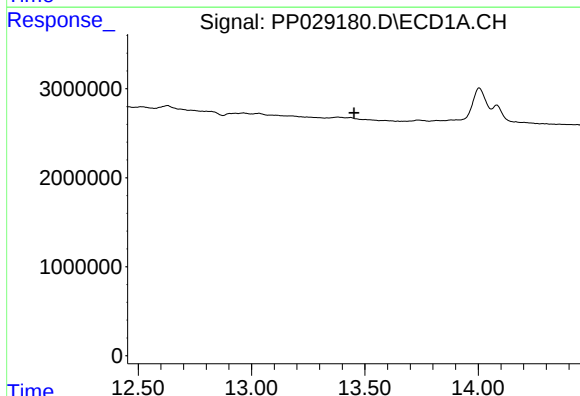


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 13.452 min
Response: 0
Conc: N.D.

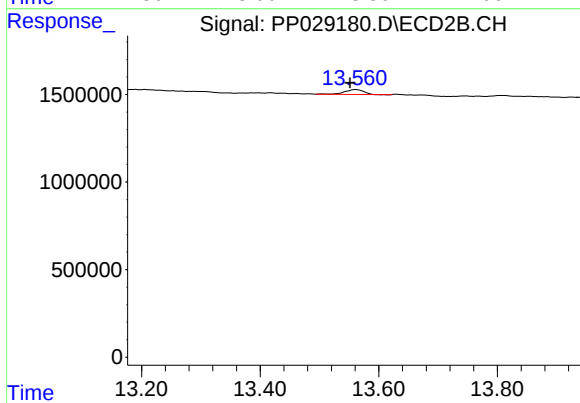

#8 DICHLORPROP


R.T.: 13.561 min
Delta R.T.: 0.010 min
Response: 585150
Conc: 17.31 ng/ml

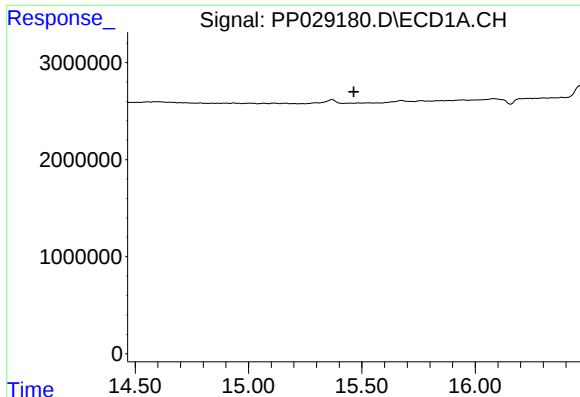

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 15.464 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
OK-02-022519

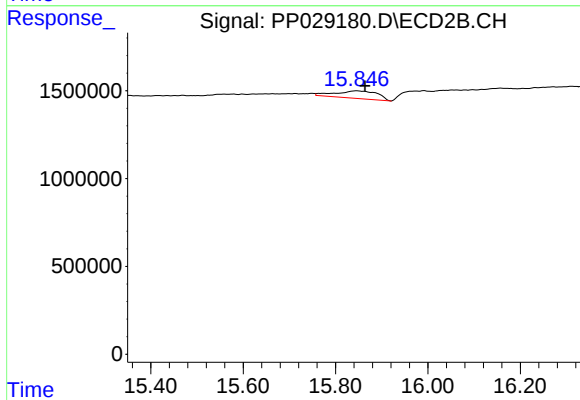


#12 2,4,5-T

R.T.: 15.846 min
Delta R.T.: -0.018 min
Response: 2706503
Conc: 16.35 ng/ml

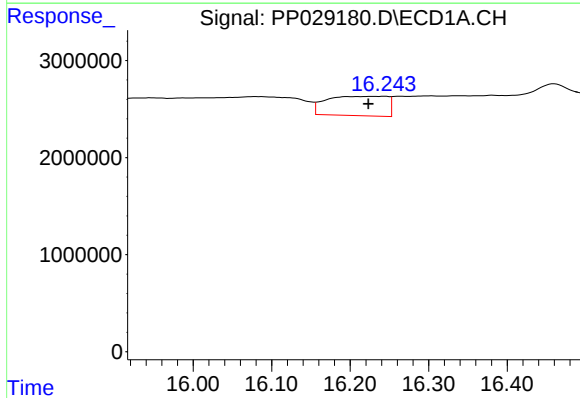


#13 2,4-DB

R.T.: 16.244 min
Delta R.T.: 0.021 min
Response: 10743005
Conc: 562.39 ng/ml

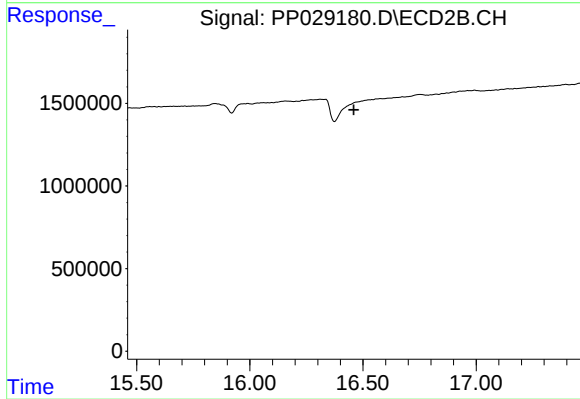

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 16.460 min
Response: 0
Conc: N.D.

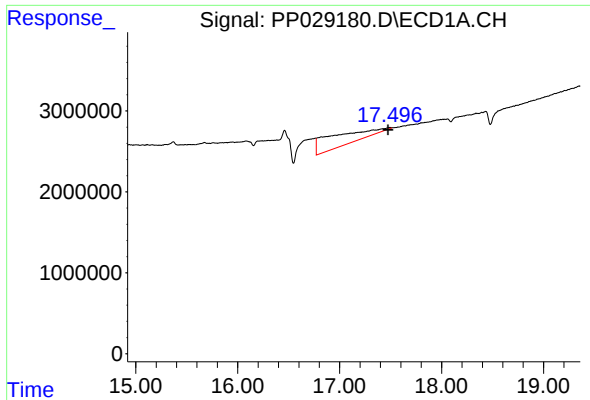

#15 Picloram

R.T.: 17.496 min
Delta R.T.: 0.020 min
Response: 46991390
Conc: 169.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
OK-02-022519

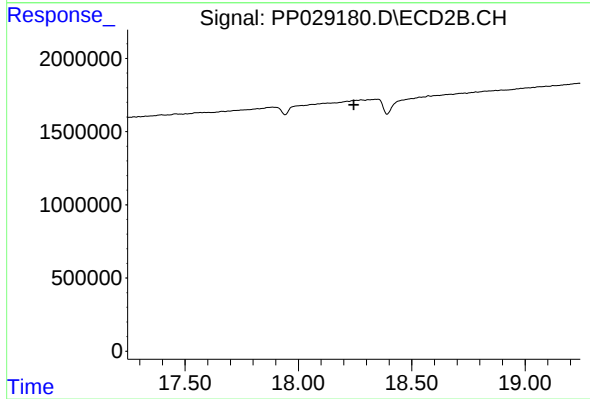

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 18.245 min
Response: 0
Conc: N.D.