

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022719\
 Data File : PP029194.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Feb 2019 1:04
 Operator : EI\MA
 Sample : K1610-10
 Misc : hexane
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 WV-E

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 28 03:39:26 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022119.M
 Quant Title : 8080.M
 QLast Update : Fri Feb 22 02:24:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.936	12.126	14940916	21038595	497.097	554.340
Target Compounds							
2) T	3,5-DICHL...	10.355	0.000	266339	0	4.318	N.D. #
5) T	DICAMBA	0.000	12.478	0	134897	N.D.	1.054 #
8) T	DICHLORPROP	0.000	13.558	0	292233	N.D.	8.644 #
10) T	Pentachlo...	14.213	14.643	4269166	3828511	6.551	7.439
12) T	2,4,5-T	0.000	15.846	0	8215890	N.D.	49.621 #
13) T	2,4-DB	16.270	0.000	6092702	0	318.951	N.D. #
14) T	DINOSEB	17.714	0.000	575803	0	3.954	N.D. #
15) T	Picloram	17.491	0.000	1737917	0	6.250	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022719\
Data File : PP029194.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Feb 2019 1:04
Operator : EI\MA
Sample : K1610-10
Misc : hexane
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :
WV-E

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 28 03:39:26 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022119.M
Quant Title : 8080.M
QLast Update : Fri Feb 22 02:24:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

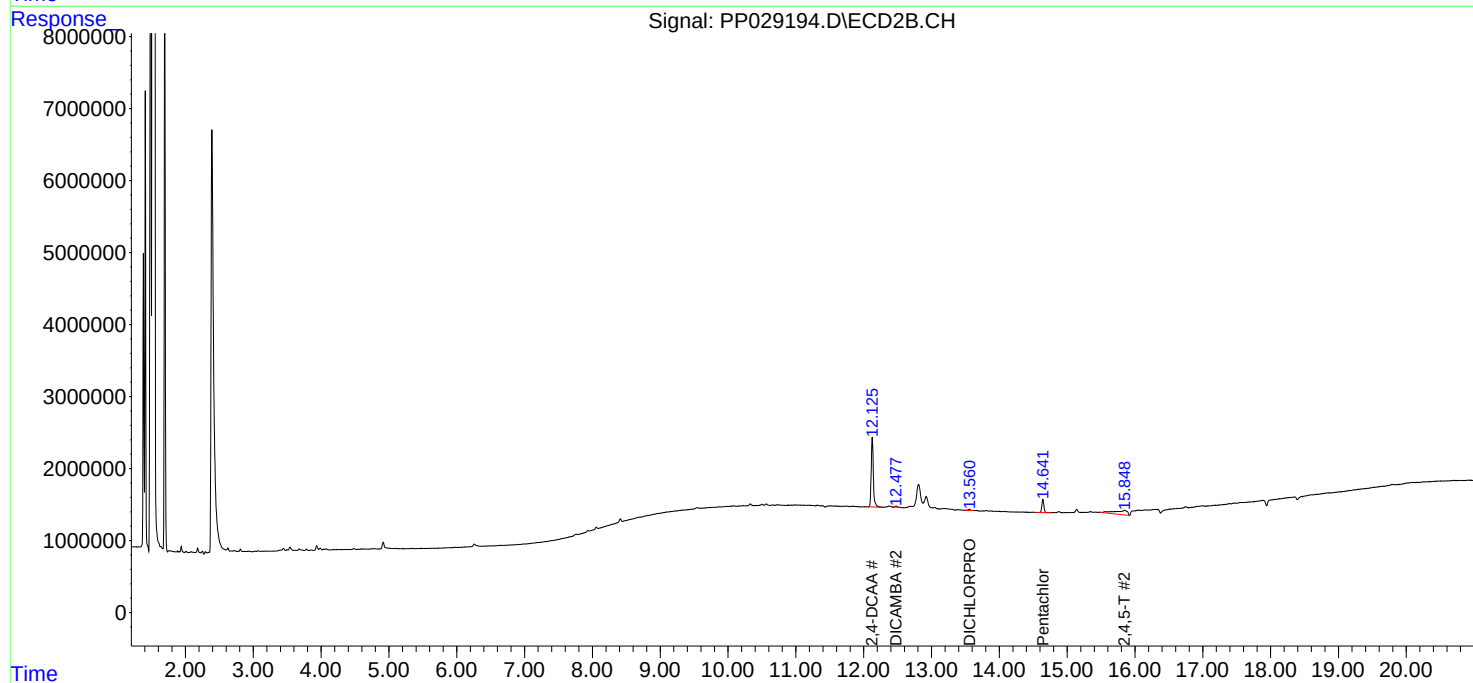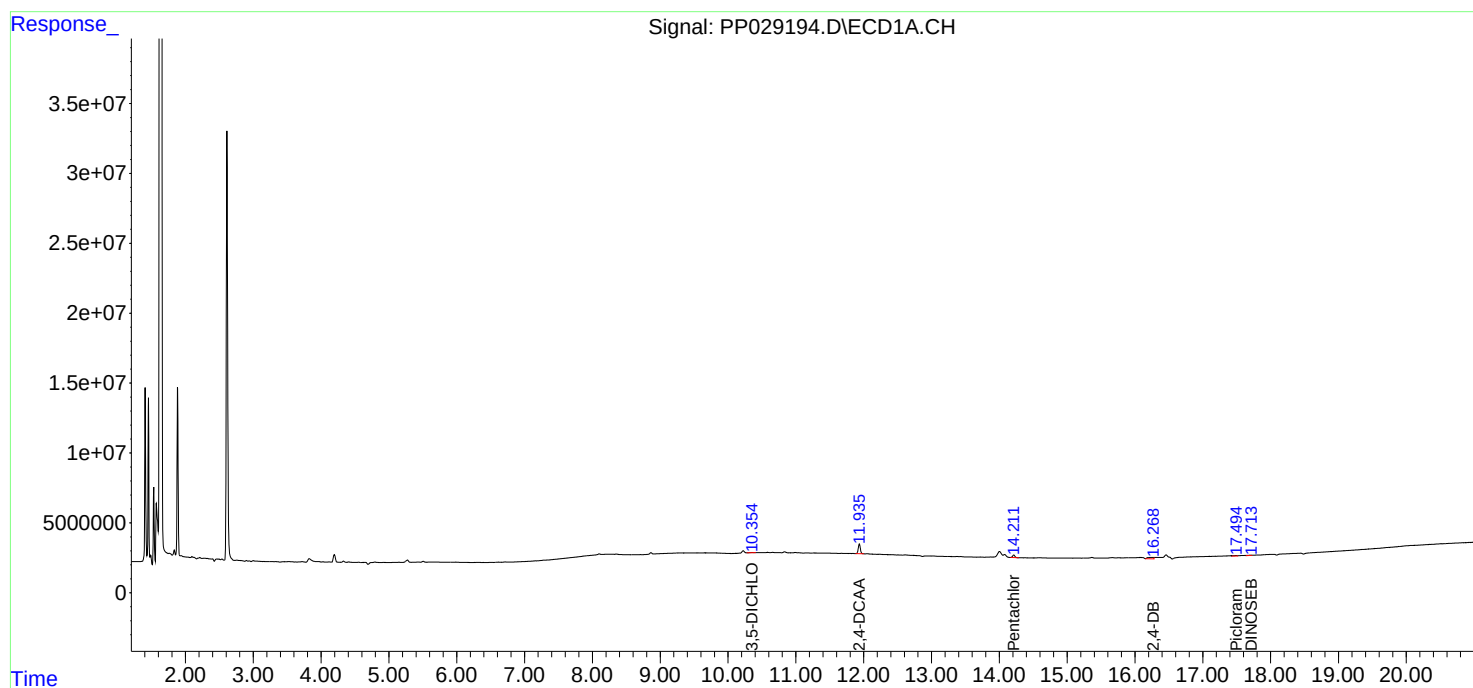


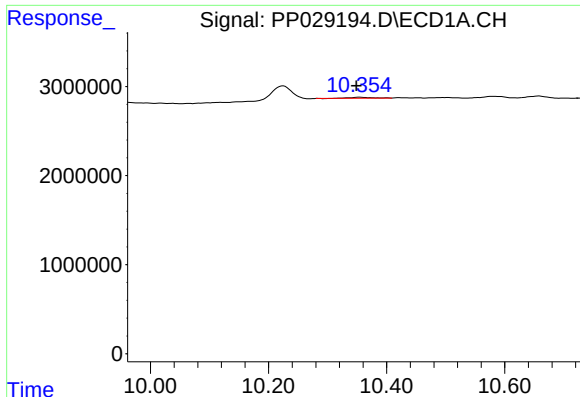

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 10.355 min
Delta R.T.: 0.006 min
Response: 266339
Conc: 4.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
WV-E

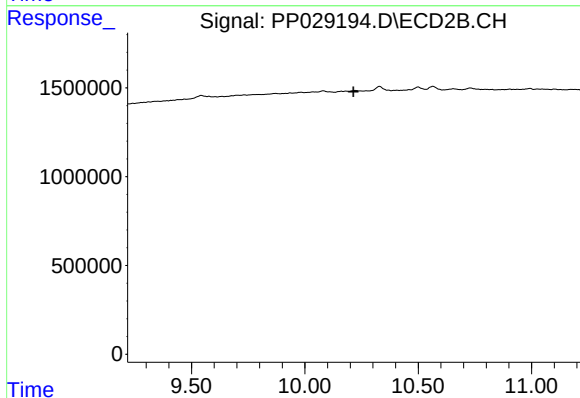


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T.: 10.215 min
Response: 0
Conc: N.D.

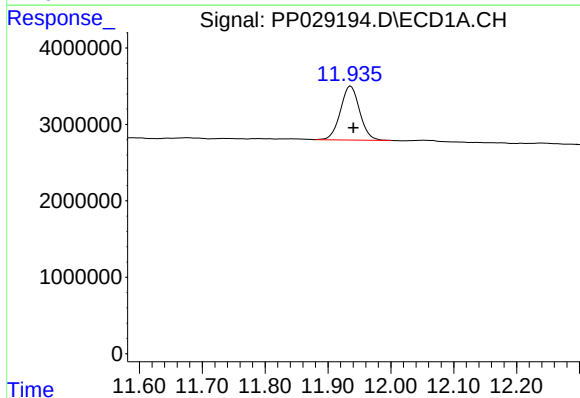


#4 2,4-DCAA

R.T.: 11.936 min
Delta R.T.: -0.004 min
Response: 14940916
Conc: 497.10 ng/ml

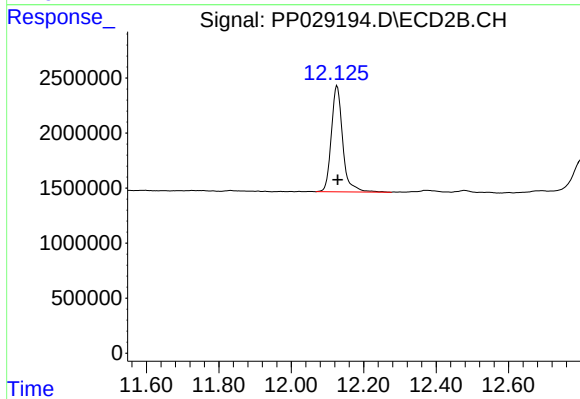

#4 2,4-DCAA


R.T.: 12.126 min
Delta R.T.: -0.002 min
Response: 21038595
Conc: 554.34 ng/ml

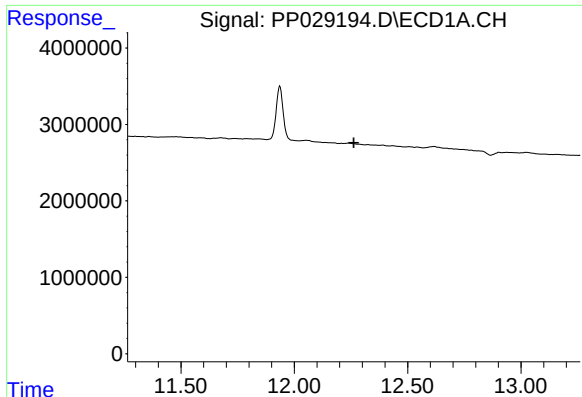

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 12.262 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
WV-E

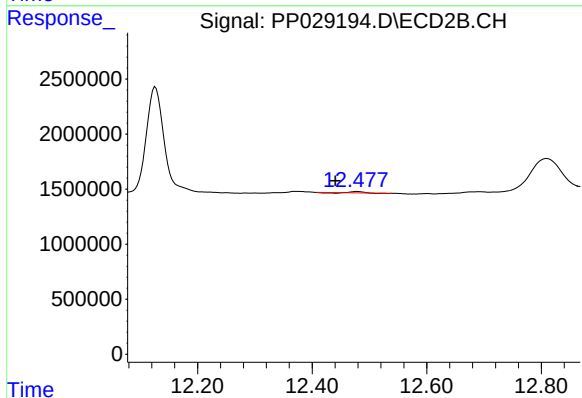


#5 DICAMBA

R.T.: 12.478 min
Delta R.T.: 0.037 min
Response: 134897
Conc: 1.05 ng/ml

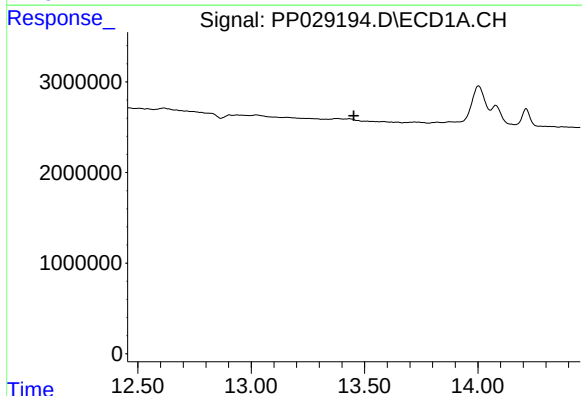


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 13.452 min
Response: 0
Conc: N.D.

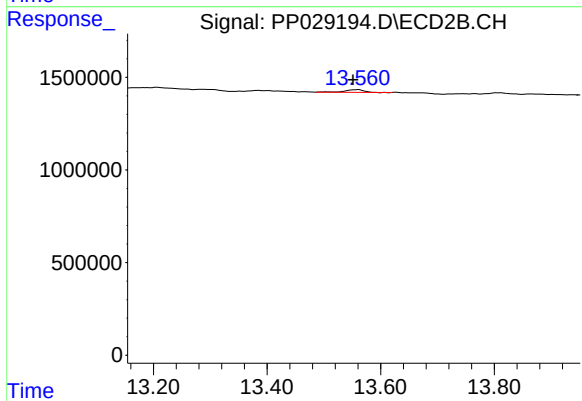

#8 DICHLORPROP


R.T.: 13.558 min
Delta R.T.: 0.007 min
Response: 292233
Conc: 8.64 ng/ml

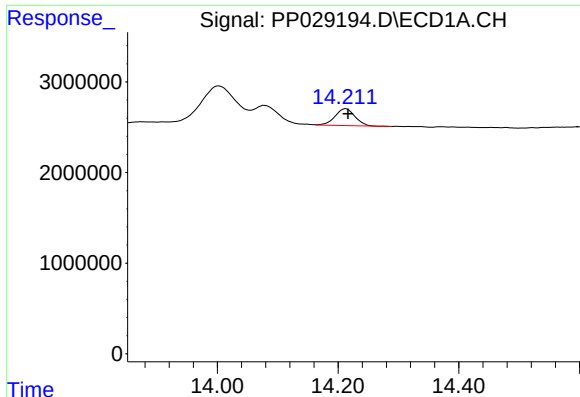

#10 Pentachlorophenol


R.T.: 14.213 min
Delta R.T.: -0.003 min
Response: 4269166
Conc: 6.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
WV-E

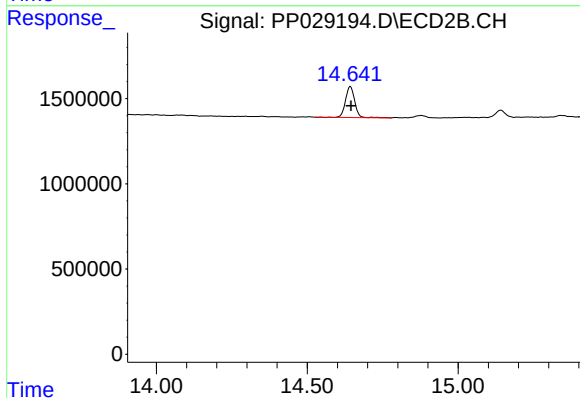


#10 Pentachlorophenol

R.T.: 14.643 min
Delta R.T.: -0.003 min
Response: 3828511
Conc: 7.44 ng/ml

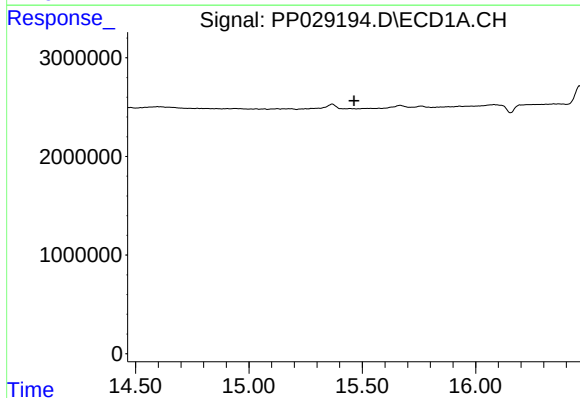


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 15.464 min
Response: 0
Conc: N.D.

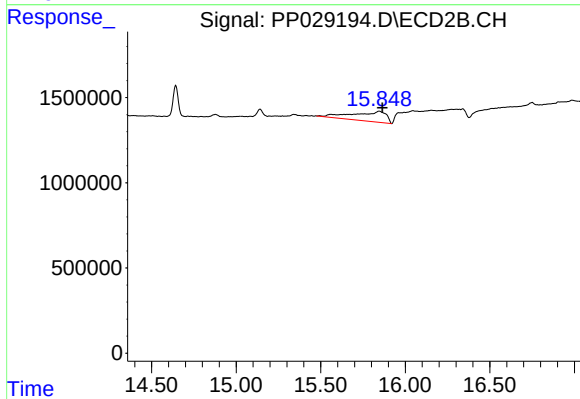

#12 2,4,5-T


R.T.: 15.846 min
Delta R.T.: -0.018 min
Response: 8215890
Conc: 49.62 ng/ml

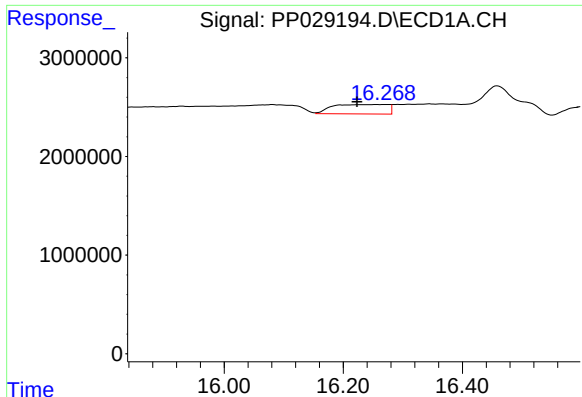

#13 2,4-DB


R.T.: 16.270 min
Delta R.T.: 0.047 min
Response: 6092702
Conc: 318.95 ng/ml

Instrument :
ECD_P
ClientSampleId :
WV-E

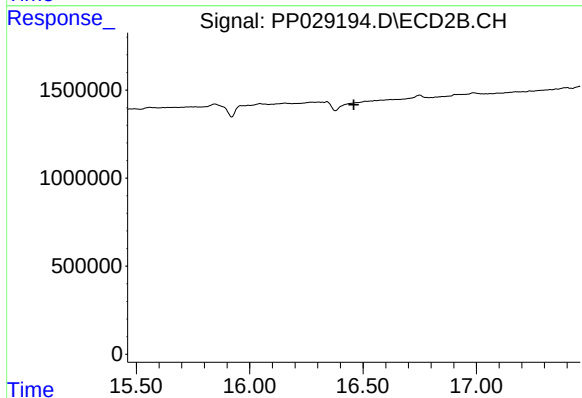


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 16.460 min
Response: 0
Conc: N.D.

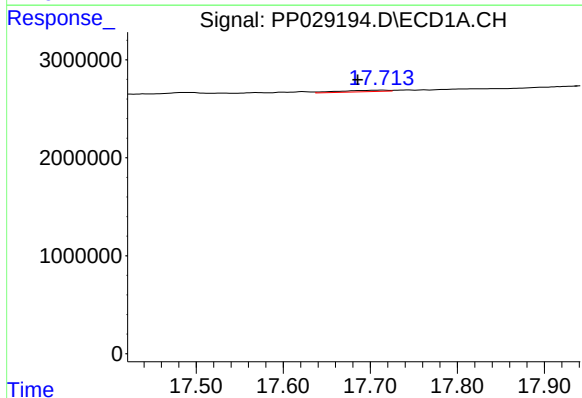


#14 DINOSEB

R.T.: 17.714 min
Delta R.T.: 0.028 min
Response: 575803
Conc: 3.95 ng/ml

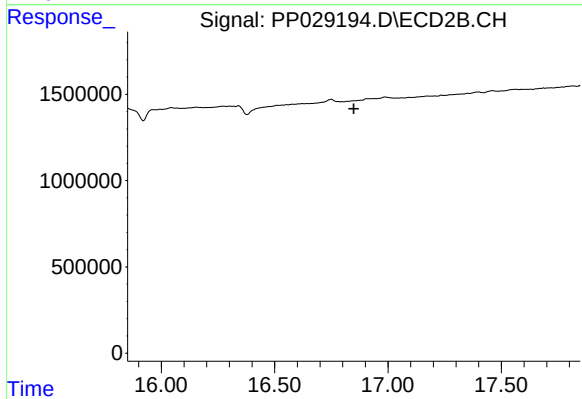

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 16.849 min
Response: 0
Conc: N.D.

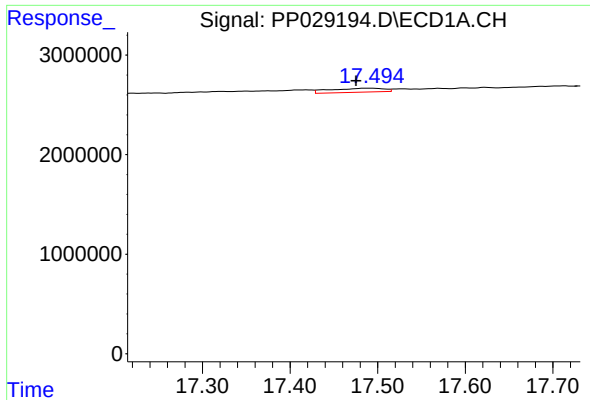

#15 Picloram

R.T.: 17.491 min
Delta R.T.: 0.015 min
Response: 1737917
Conc: 6.25 ng/ml

Instrument :
ECD_P
ClientSampleId :
WV-E

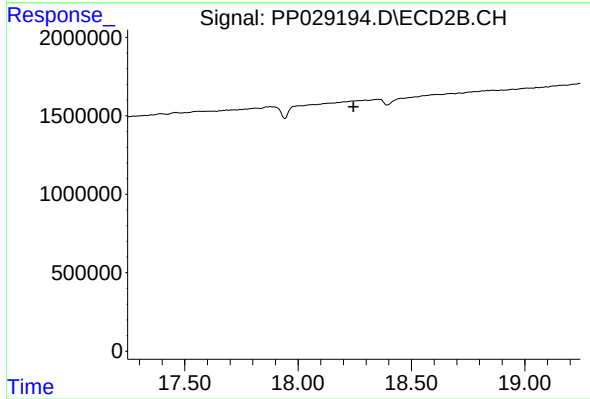

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 18.245 min
Response: 0
Conc: N.D.