

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022819\
 Data File : PP029198.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Feb 2019 10:26
 Operator : EI\MA
 Sample : HEXANE
 Misc : hexane
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 00:22:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022119.M
 Quant Title : 8080.M
 QLast Update : Fri Feb 22 02:24:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
5) T	DICAMBA	0.000	12.474	0	1740675	13.599 #
15) T	Picloram	0.000	18.242	0	4500286	19.999 #
16) T	DCPA	0.000	18.106	0	2539729	10.928 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022819\
Data File : PP029198.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Feb 2019 10:26
Operator : EI\MA
Sample : HEXANE
Misc : hexane
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 00:22:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022119.M
Quant Title : 8080.M
QLast Update : Fri Feb 22 02:24:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

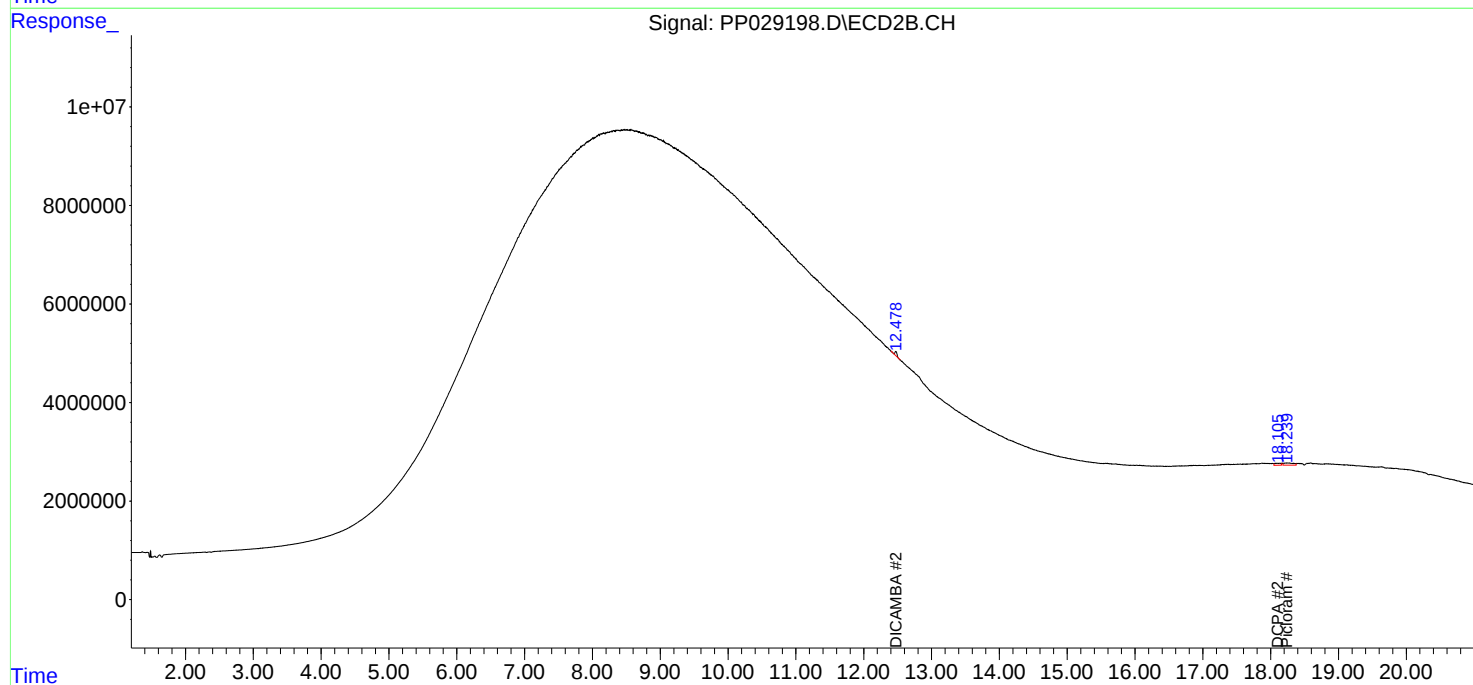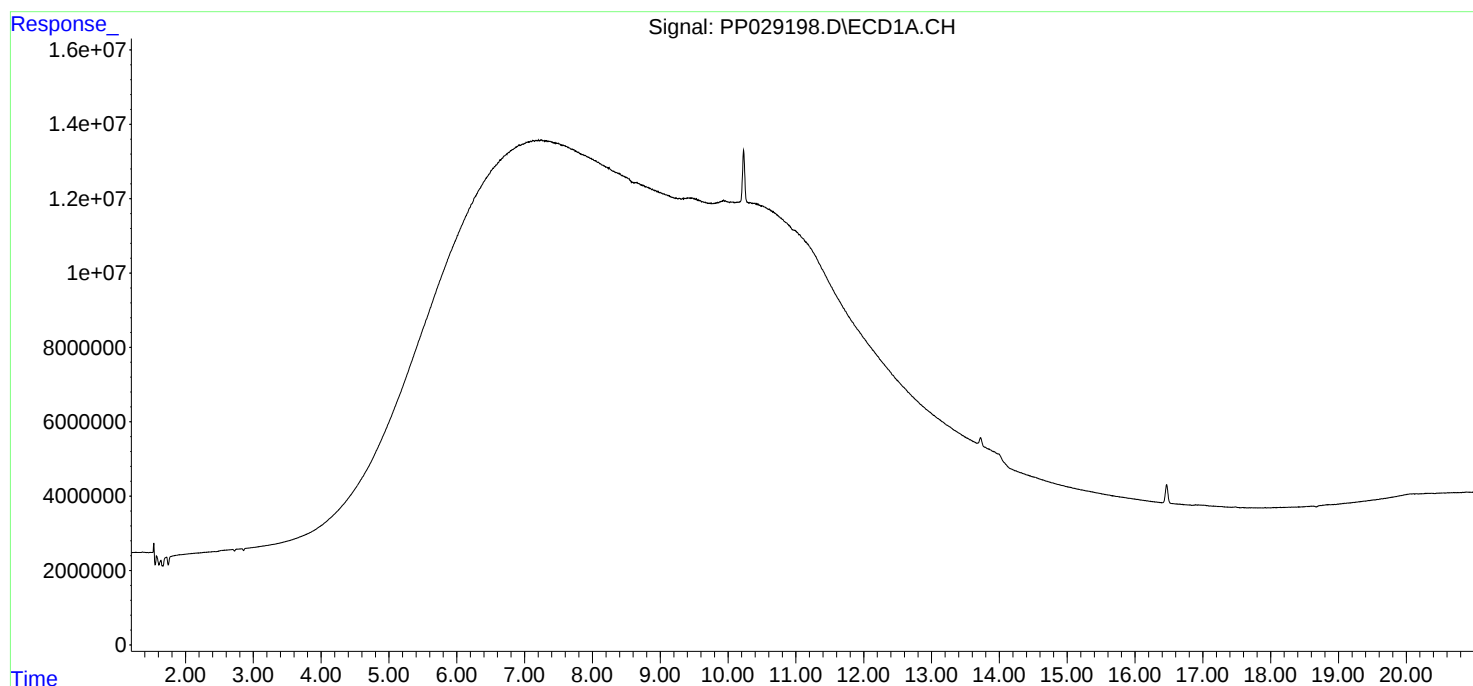


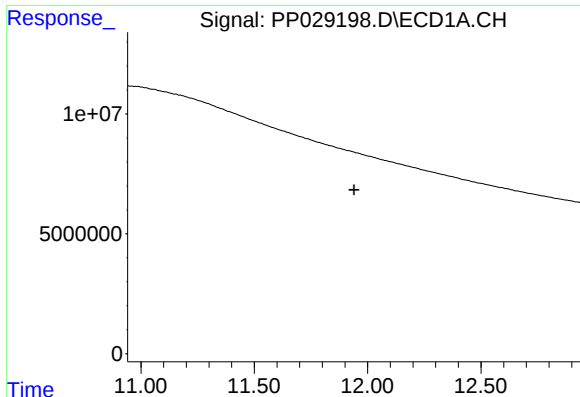

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 11.940 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

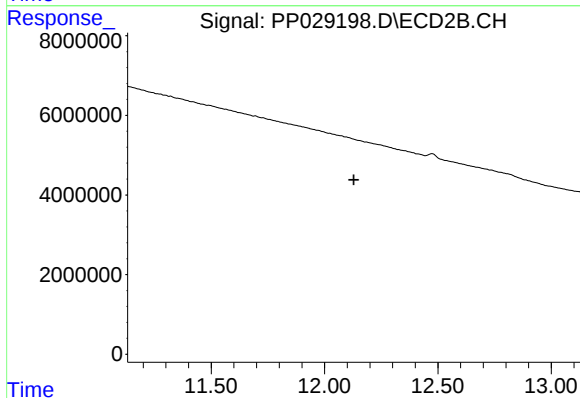


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 12.129 min
Response: 0
Conc: N.D.

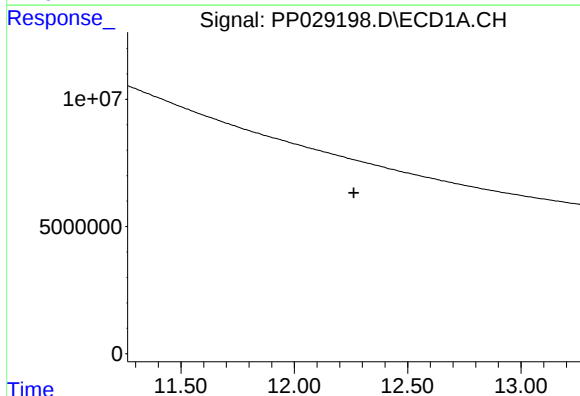


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 12.262 min
Response: 0
Conc: N.D.

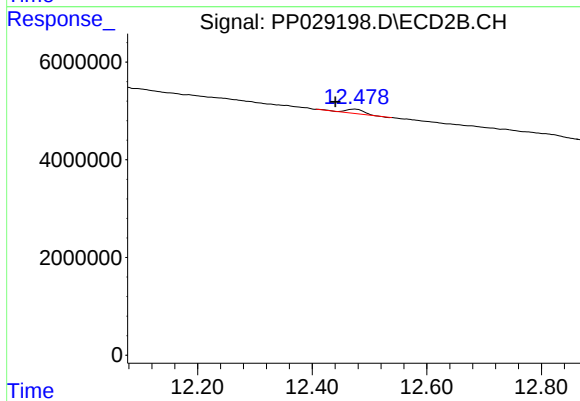

#5 DICAMBA


R.T.: 12.474 min
Delta R.T.: 0.033 min
Response: 1740675
Conc: 13.60 ng/ml

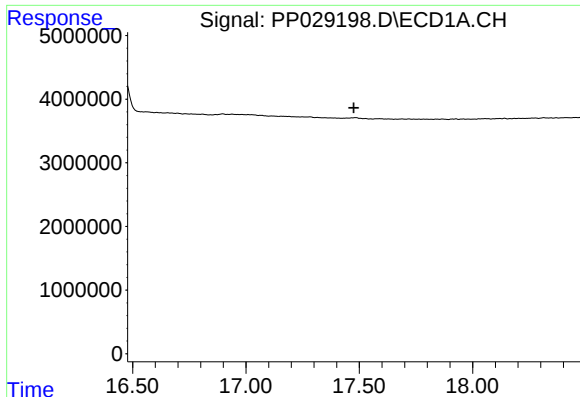

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 17.475 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

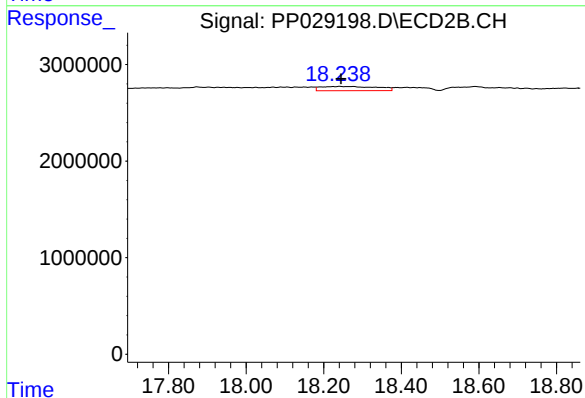


#15 Picloram

R.T.: 18.242 min
Delta R.T.: -0.003 min
Response: 4500286
Conc: 20.00 ng/ml

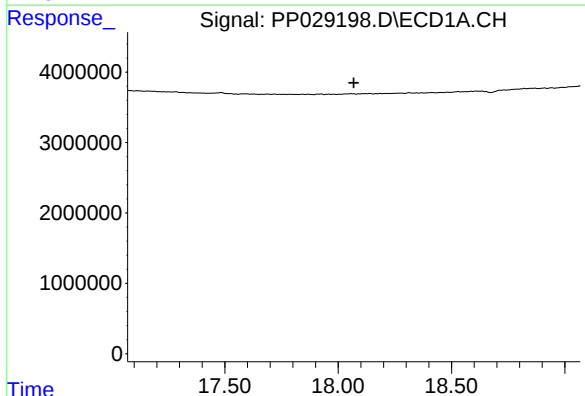

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 18.069 min
Response: 0
Conc: N.D.

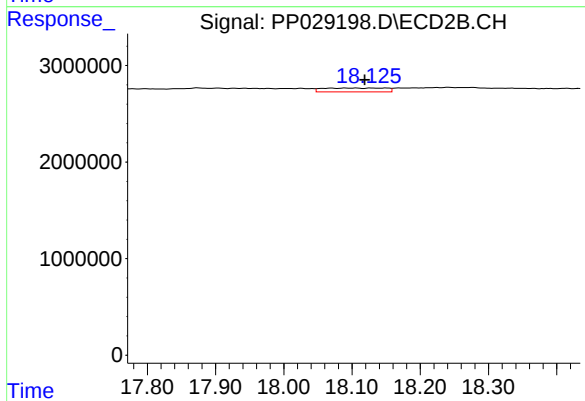

#16 DCPA

R.T.: 18.106 min
Delta R.T.: -0.012 min
Response: 2539729
Conc: 10.93 ng/ml