

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022819\
 Data File : PP029211.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 28 Feb 2019 19:59
 Operator : EI\MA
 Sample : K1643-04
 Misc : hexane
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 00:24:28 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022119.M
 Quant Title : 8080.M
 QLast Update : Fri Feb 22 02:24:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.937	12.129	10045669	13775423	334.228	362.965
Target Compounds							
8) T	DICHLORPROP	0.000	13.563	0	694482	N.D.	20.541 #
9) T	2,4-D	0.000	14.038	0	421504	N.D.	9.296 #
10) T	Pentachlo...	14.215	14.645	3227959	2515265	4.954	4.887
12) T	2,4,5-T	0.000	15.850	0	2679193	N.D.	16.181 #
13) T	2,4-DB	16.225	0.000	2766173	0	144.808	N.D. #
14) T	DINOSEB	0.000	16.843	0	1687839	N.D.	12.877 #
15) T	Picloram	17.475	18.249	1694570	4628303	6.094	20.568 #
16) T	DCPA	0.000	18.116	0	2768950	N.D.	11.915 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022819\
Data File : PP029211.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 28 Feb 2019 19:59
Operator : EI\MA
Sample : K1643-04
Misc : hexane
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 00:24:28 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022119.M
Quant Title : 8080.M
QLast Update : Fri Feb 22 02:24:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-CLPesticides-1 Signal #2 Phase: ZB-CLPesticides-2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

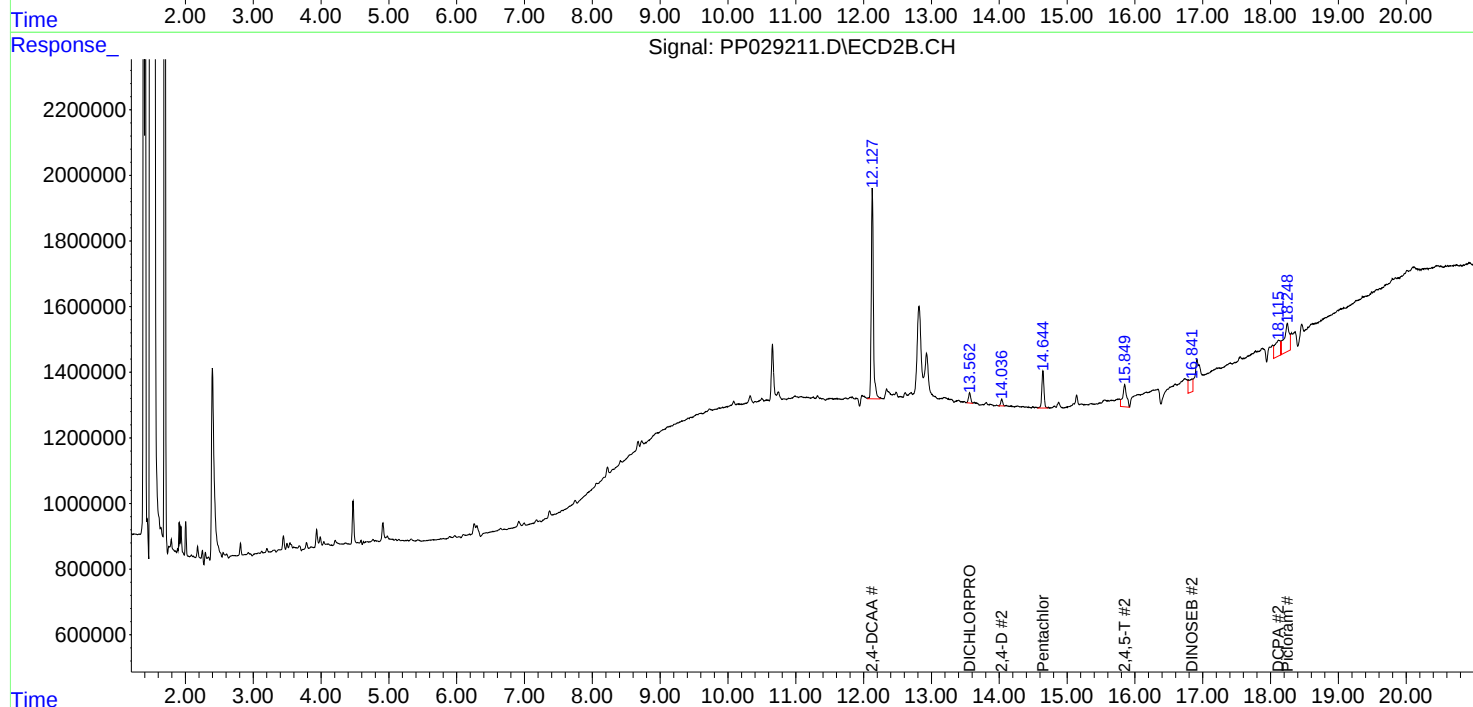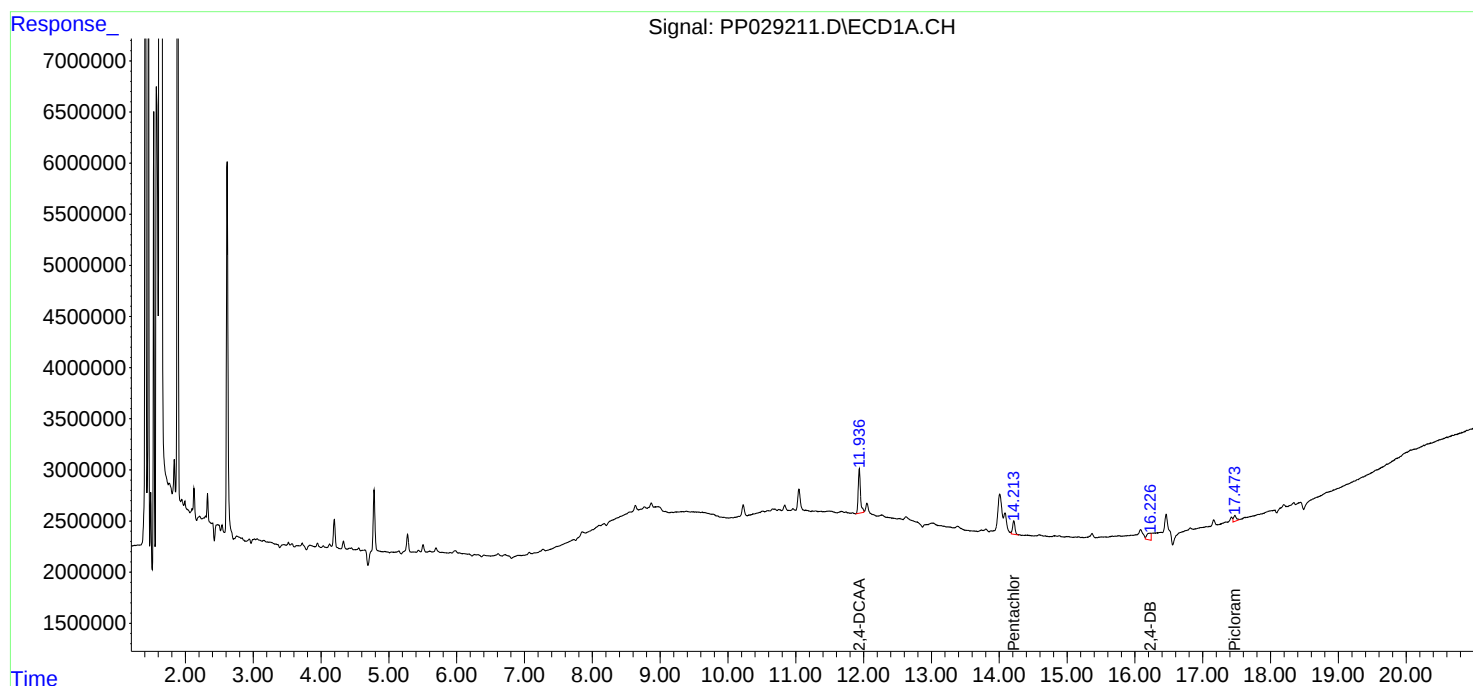


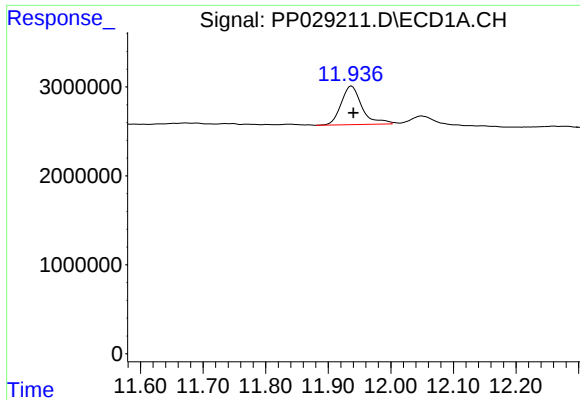

#4 2,4-DCAA


R.T.: 11.937 min
Delta R.T.: -0.003 min
Response: 10045669
Conc: 334.23 ng/ml

Instrument :
ECD_P
ClientSampleId :

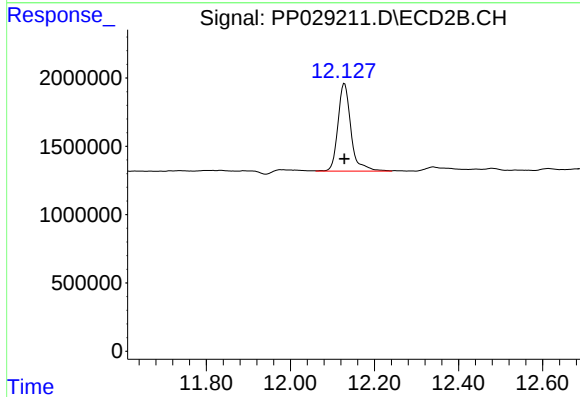


#4 2,4-DCAA

R.T.: 12.129 min
Delta R.T.: 0.000 min
Response: 13775423
Conc: 362.96 ng/ml

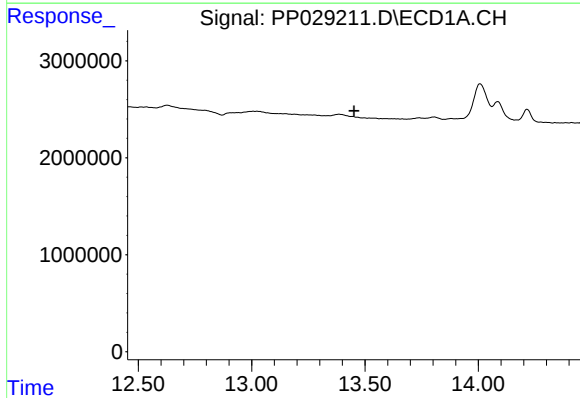


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 13.452 min
Response: 0
Conc: N.D.

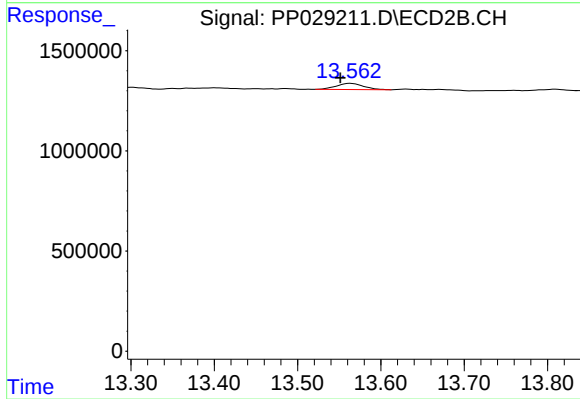

#8 DICHLORPROP


R.T.: 13.563 min
Delta R.T.: 0.012 min
Response: 694482
Conc: 20.54 ng/ml

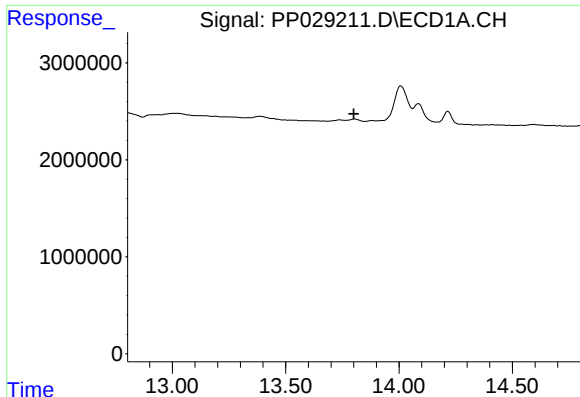

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.800 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

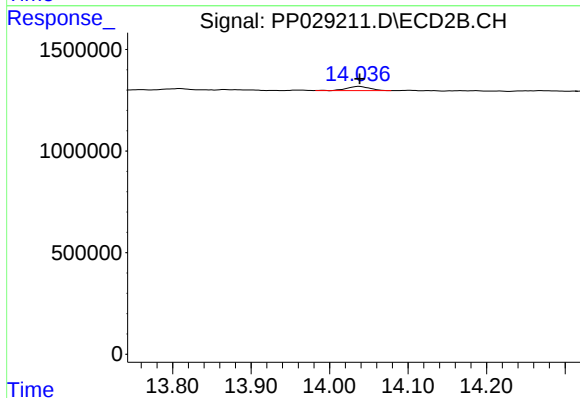


#9 2,4-D

R.T.: 14.038 min
Delta R.T.: 0.000 min
Response: 421504
Conc: 9.30 ng/ml

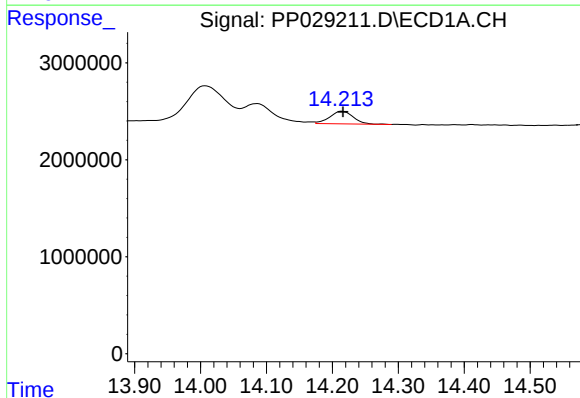


#10 Pentachlorophenol

R.T.: 14.215 min
Delta R.T.: -0.001 min
Response: 3227959
Conc: 4.95 ng/ml

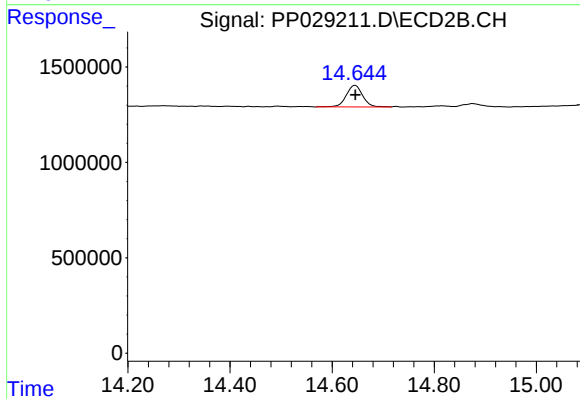

#10 Pentachlorophenol


R.T.: 14.645 min
Delta R.T.: 0.000 min
Response: 2515265
Conc: 4.89 ng/ml

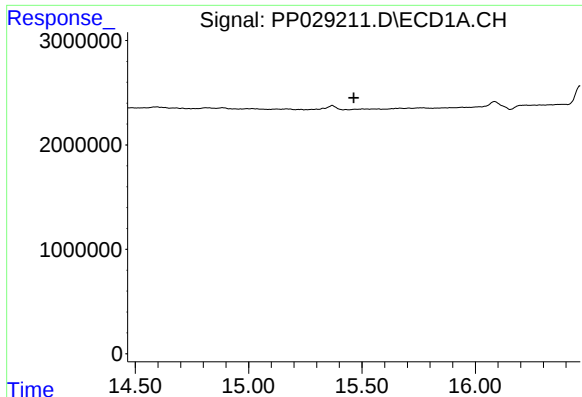

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 15.464 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

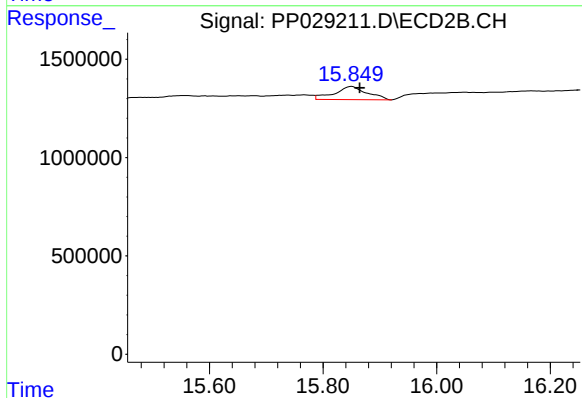


#12 2,4,5-T

R.T.: 15.850 min
Delta R.T.: -0.014 min
Response: 2679193
Conc: 16.18 ng/ml

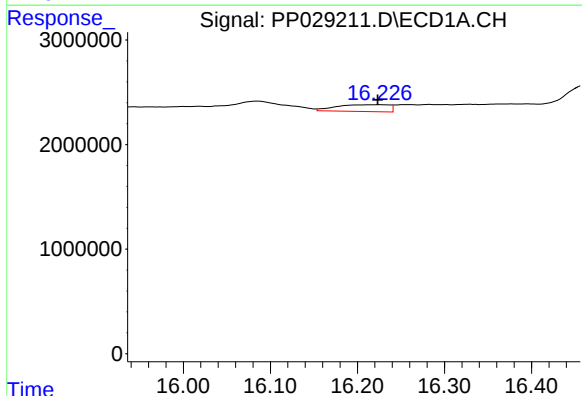


#13 2,4-DB

R.T.: 16.225 min
Delta R.T.: 0.002 min
Response: 2766173
Conc: 144.81 ng/ml

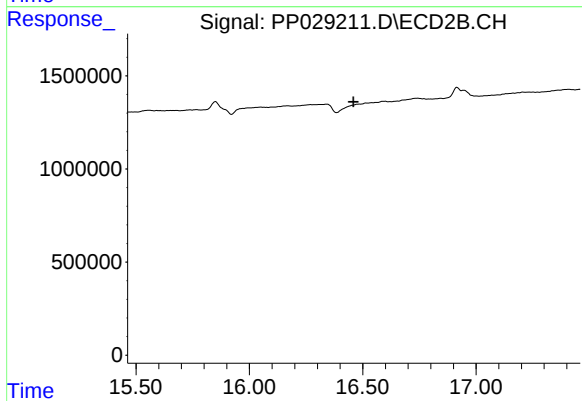

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 16.460 min
Response: 0
Conc: N.D.

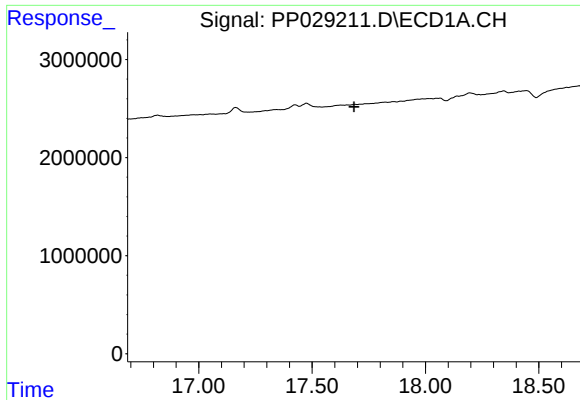

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 17.686 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

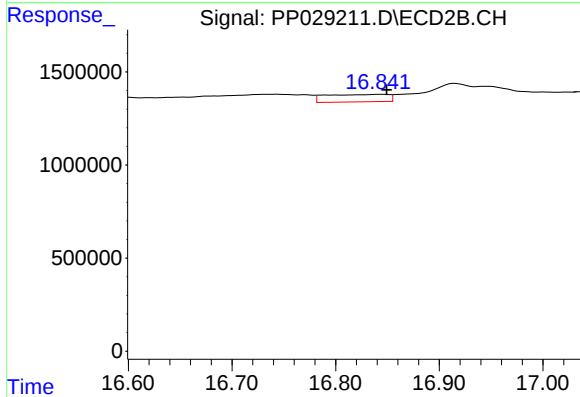


#14 DINOSEB

R.T.: 16.843 min
Delta R.T.: -0.006 min
Response: 1687839
Conc: 12.88 ng/ml

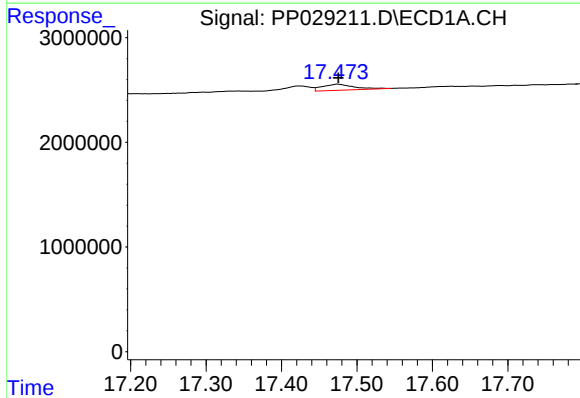


#15 Picloram

R.T.: 17.475 min
Delta R.T.: 0.000 min
Response: 1694570
Conc: 6.09 ng/ml

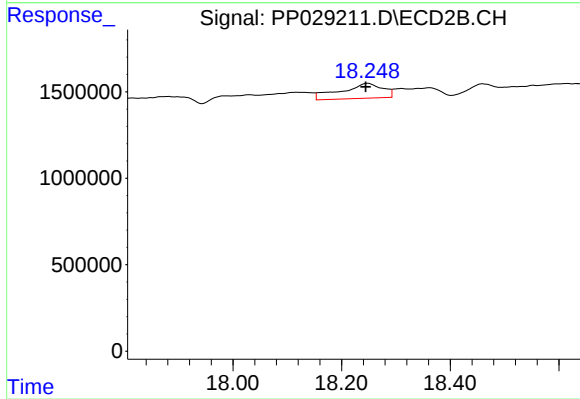

#15 Picloram


R.T.: 18.249 min
Delta R.T.: 0.004 min
Response: 4628303
Conc: 20.57 ng/ml

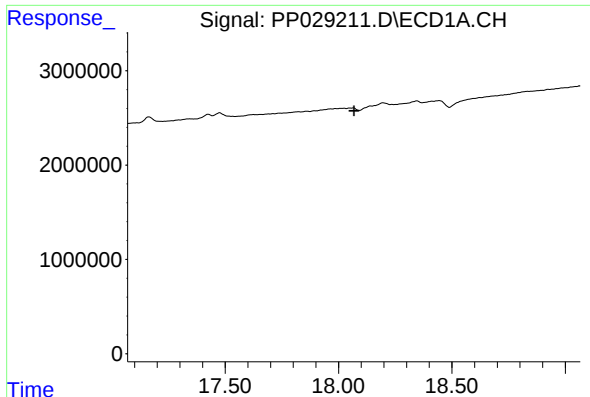

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 18.069 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

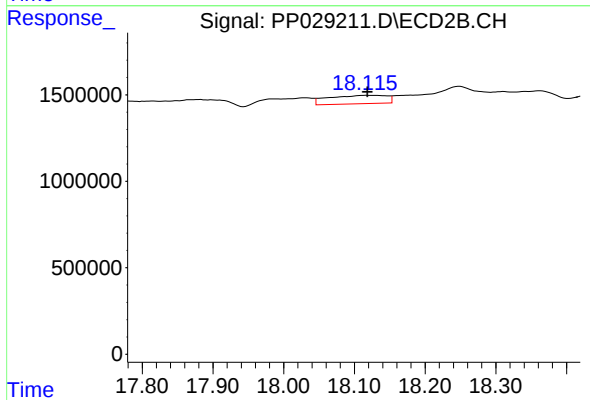

#16 DCPA

R.T.: 18.116 min
Delta R.T.: -0.002 min
Response: 2768950
Conc: 11.91 ng/ml