

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022822\
 Data File : PP044099.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Feb 2022 20:34
 Operator : YP\AJ
 Sample : N1700-01 10X
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 01-A-01-B-01-C

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/01/2022
 Supervised By :Ankita Jodhani 03/01/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 00:44:18 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP021022.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 11 04:48:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.919	3.170	11305859	6247228	5.113m	3.326m#
2) SA Decachlor...	10.058	8.542	2144487	5100000	1.805m	3.144m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP022822\
Data File : PP044099.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Feb 2022 20:34
Operator : YP\AJ
Sample : N1700-01 10X
Misc :
ALS Vial : 32 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
01-A-01-B-01-C


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/01/2022
Supervised By :Ankita Jodhani 03/01/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 00:44:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP021022.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 11 04:48:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

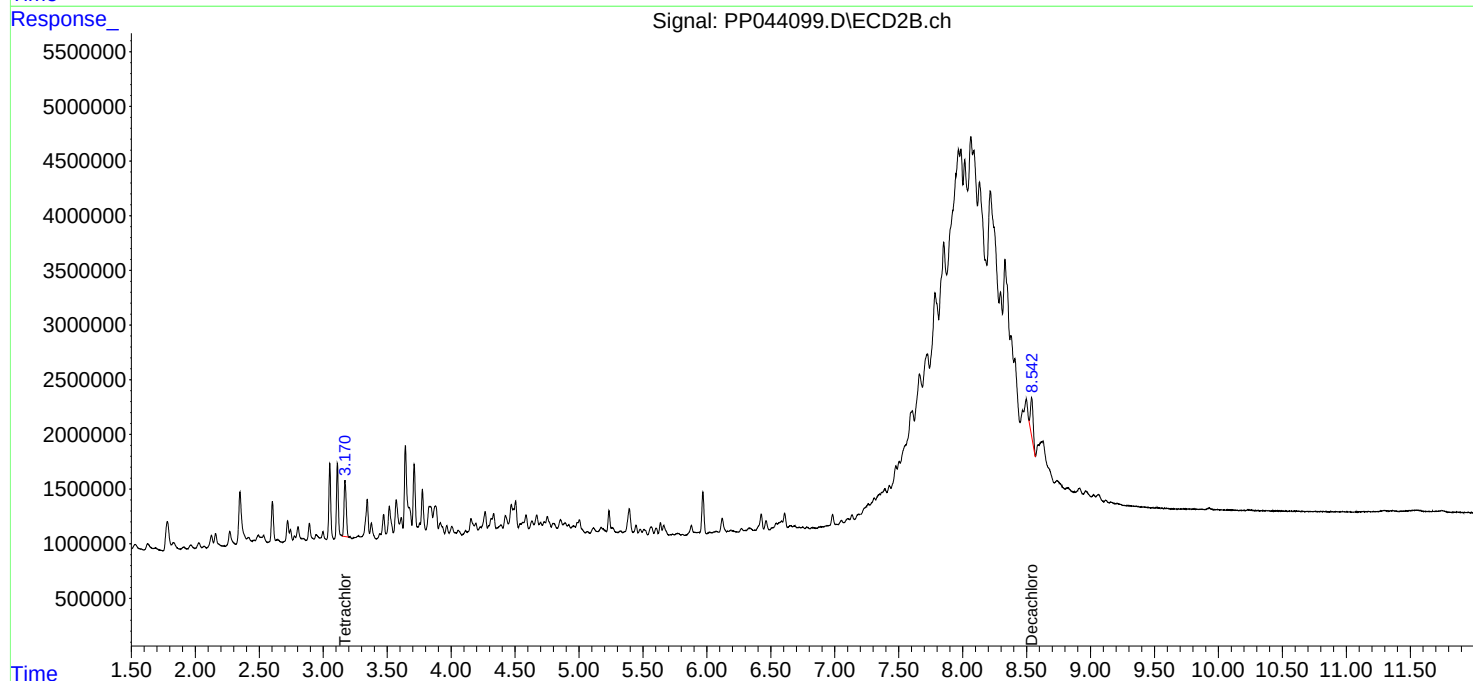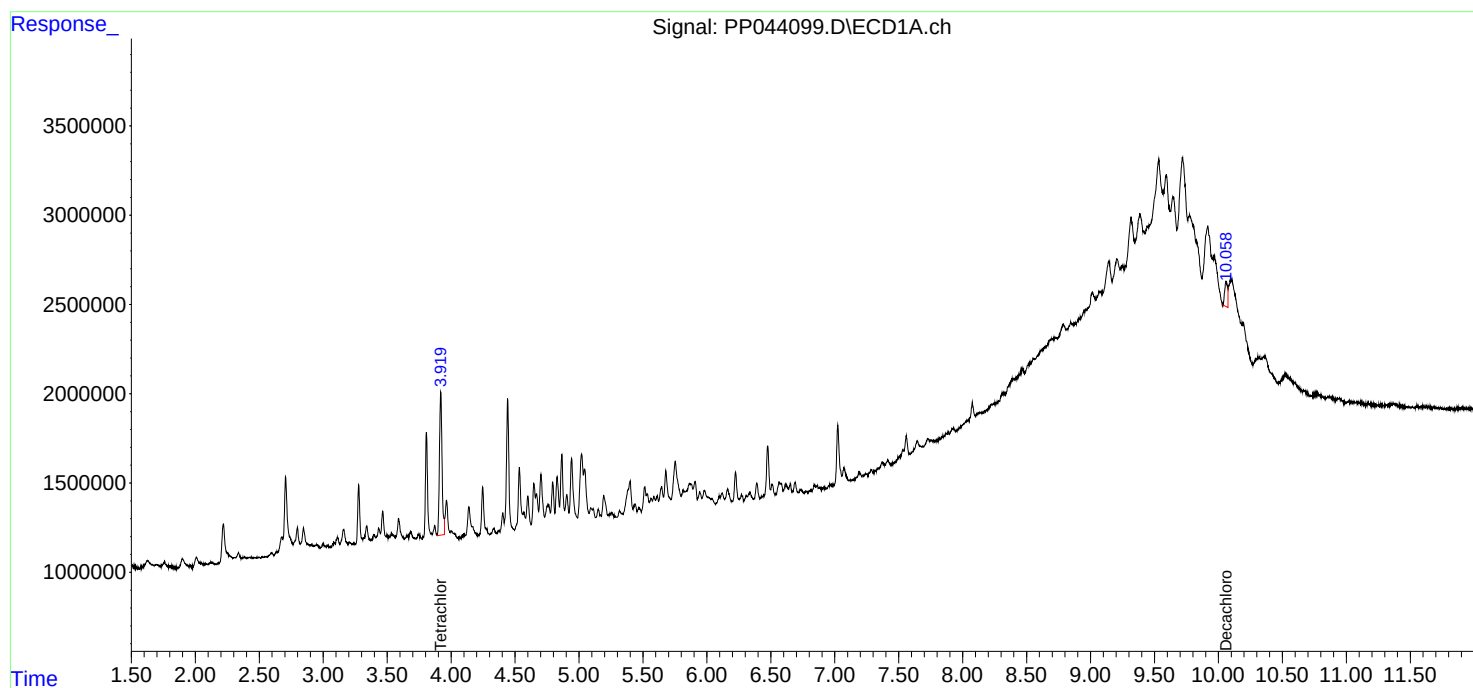

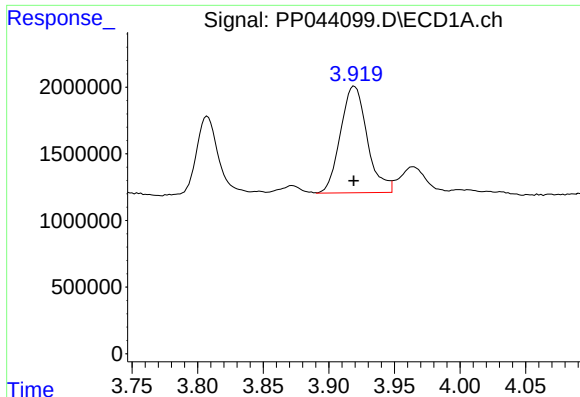


#1 Tetrachloro-m-xylene

R.T.: 3.919 min
Delta R.T.: 0.000 min
Response: 11305859
Conc: 5.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
01-A-01-B-01-C


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/01/2022
Supervised By :Ankita Jodhani 03/01/2022

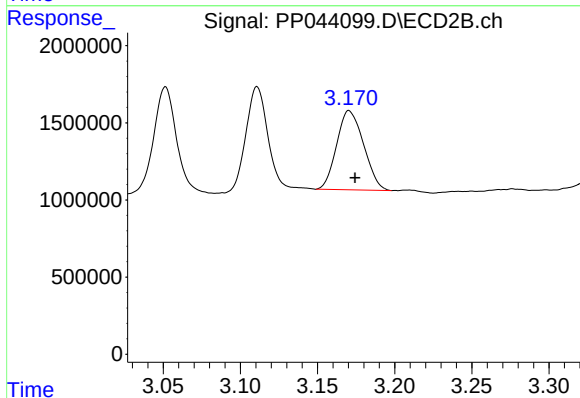


#1 Tetrachloro-m-xylene

R.T.: 3.170 min
Delta R.T.: -0.004 min
Response: 6247228
Conc: 3.33 ng/ml m

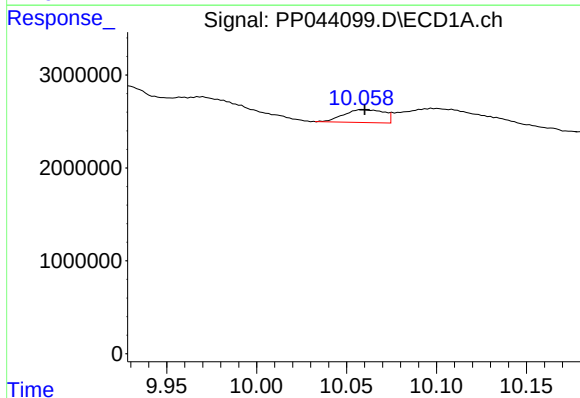

#2 Decachlorobiphenyl

R.T.: 10.058 min
Delta R.T.: -0.002 min
Response: 2144487
Conc: 1.81 ng/ml m

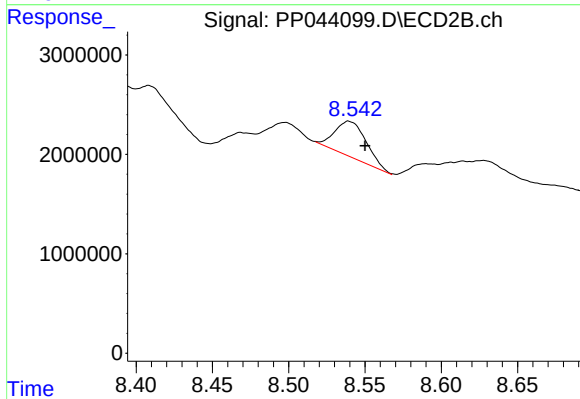

#2 Decachlorobiphenyl

R.T.: 8.542 min
Delta R.T.: -0.008 min
Response: 5100000
Conc: 3.14 ng/ml m