

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030121\
 Data File : PP033614.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Mar 2021 12:06
 Operator : DD\AJ
 Sample : M1489-06 10X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 41129

Manual Integrations
 APPROVED

Ankita
 3/2/2021 8:55:39 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 14:44:45 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 22 12:13:48 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.719	3.993	209367	56206	2.845m	1.276m#
2) SA Decachlor...	10.541	9.254	250979	94404	5.396m	2.988m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030121\
Data File : PP033614.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Mar 2021 12:06
Operator : DD\AJ
Sample : M1489-06 10X
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
41129


Manual Integrations
APPROVED

Ankita
3/2/2021 8:55:39 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 14:44:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022121.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 22 12:13:48 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

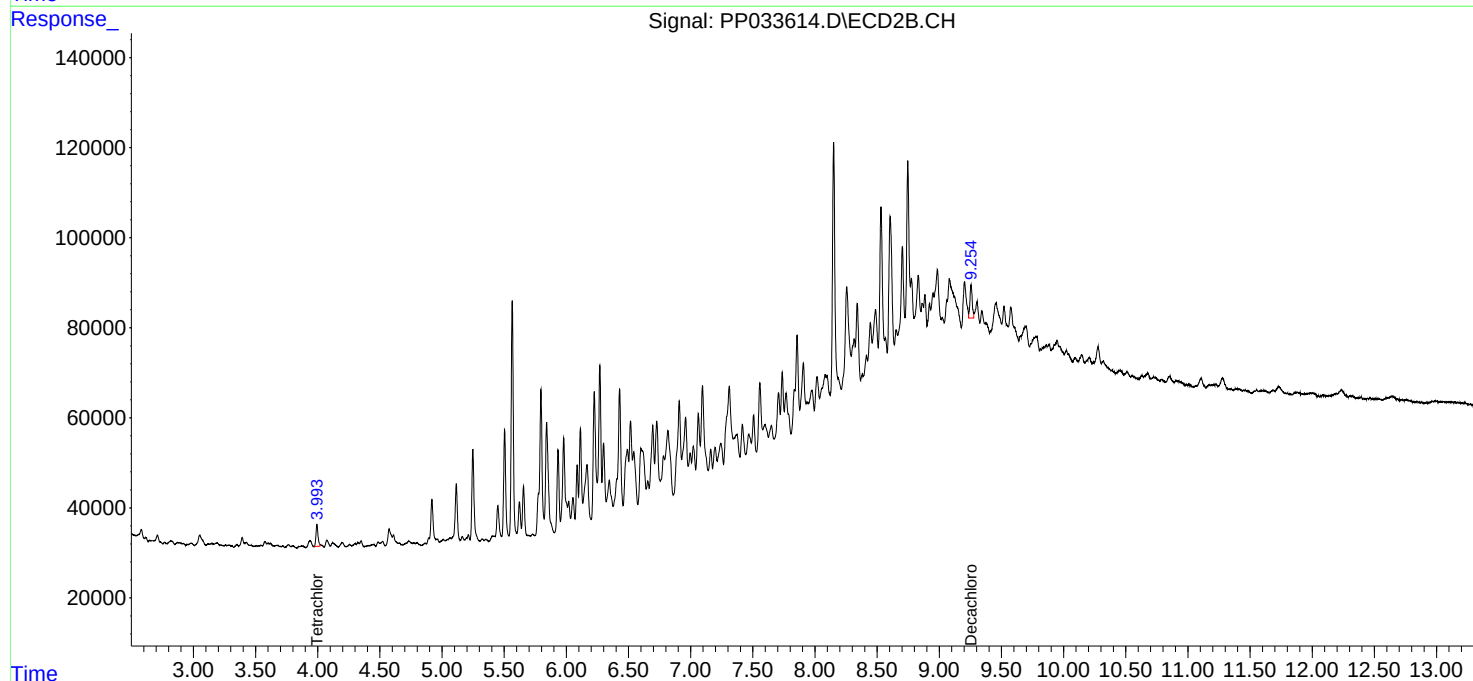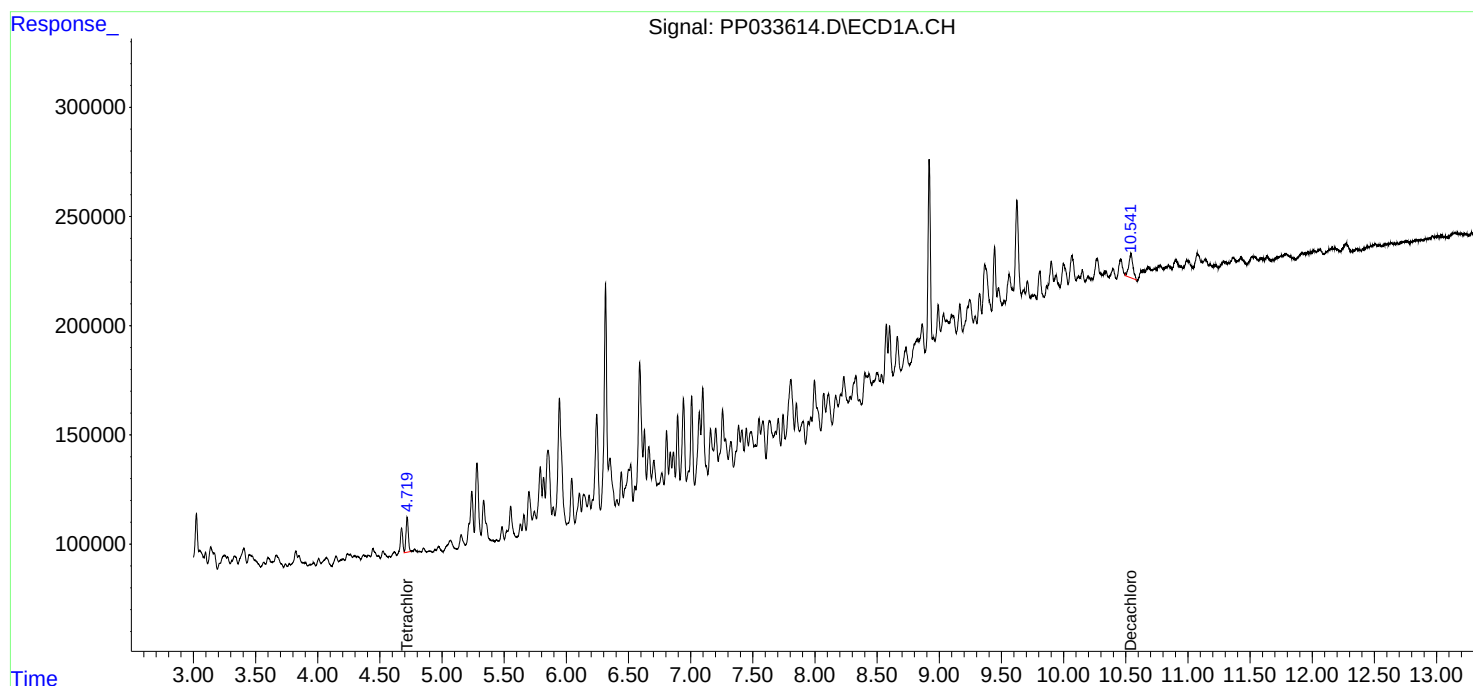

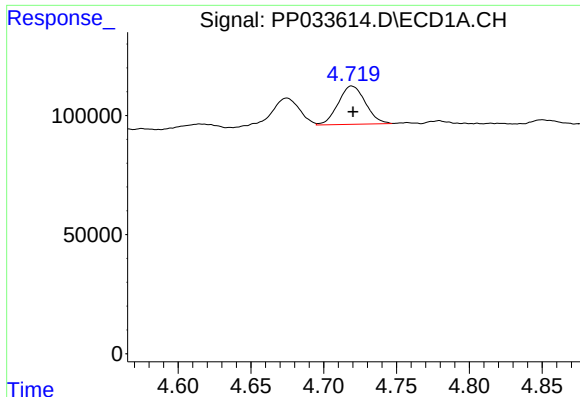


#1 Tetrachloro-m-xylene

R.T.: 4.719 min
Delta R.T.: -0.001 min
Response: 209367
Conc: 2.84 ng/ml m

Instrument :
ECD_P
ClientSampleId :
41129


Manual Integrations
APPROVED

Ankita
3/2/2021 8:55:39 AM

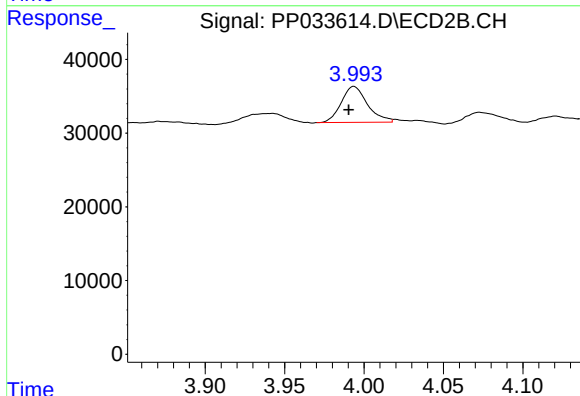


#1 Tetrachloro-m-xylene

R.T.: 3.993 min
Delta R.T.: 0.003 min
Response: 56206
Conc: 1.28 ng/ml m

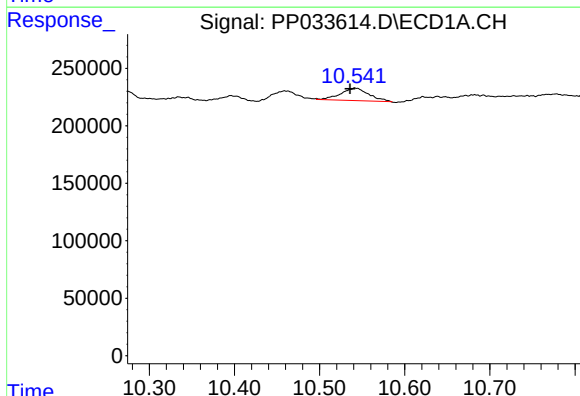

#2 Decachlorobiphenyl

R.T.: 10.541 min
Delta R.T.: 0.005 min
Response: 250979
Conc: 5.40 ng/ml m

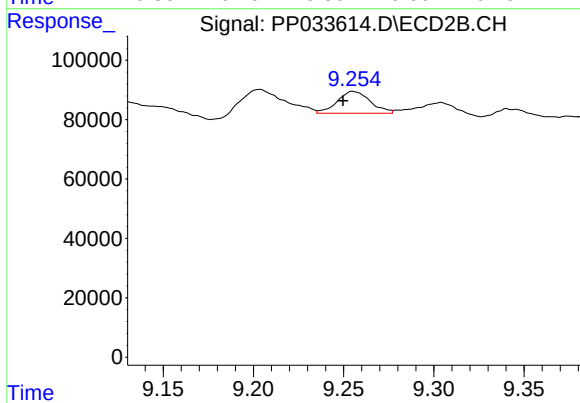

#2 Decachlorobiphenyl

R.T.: 9.254 min
Delta R.T.: 0.005 min
Response: 94404
Conc: 2.99 ng/ml m