

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030121\
 Data File : PP033625.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Mar 2021 15:28
 Operator : DD\AJ
 Sample : M1486-05
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 56-59

Manual Integrations
 APPROVED

Ankita
 3/2/2021 8:55:50 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 17:21:45 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 22 12:13:48 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.723	3.993	1802724	1006290	24.493	22.850
2)	SA Decachlor...	10.536	9.247	842353	589461	18.111	18.655
Target Compounds							
16)	L4 AR-1242-1	6.021	5.234	330664	174578	226.327	191.962m
17)	L4 AR-1242-2	6.044	5.254	440704	236904	197.717	176.156m
18)	L4 AR-1242-3	6.109	5.444	320865	140124	232.219	190.566m
19)	L4 AR-1242-4	6.214	5.540	253309	133079	218.357	194.525
20)	L4 AR-1242-5	6.993	6.100	203310	126763	181.423	167.262

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030121\
Data File : PP033625.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Mar 2021 15:28
Operator : DD\AJ
Sample : M1486-05
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampled :
56-59


Manual Integrations
APPROVED

Ankita
3/2/2021 8:55:50 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 17:21:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022121.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 22 12:13:48 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

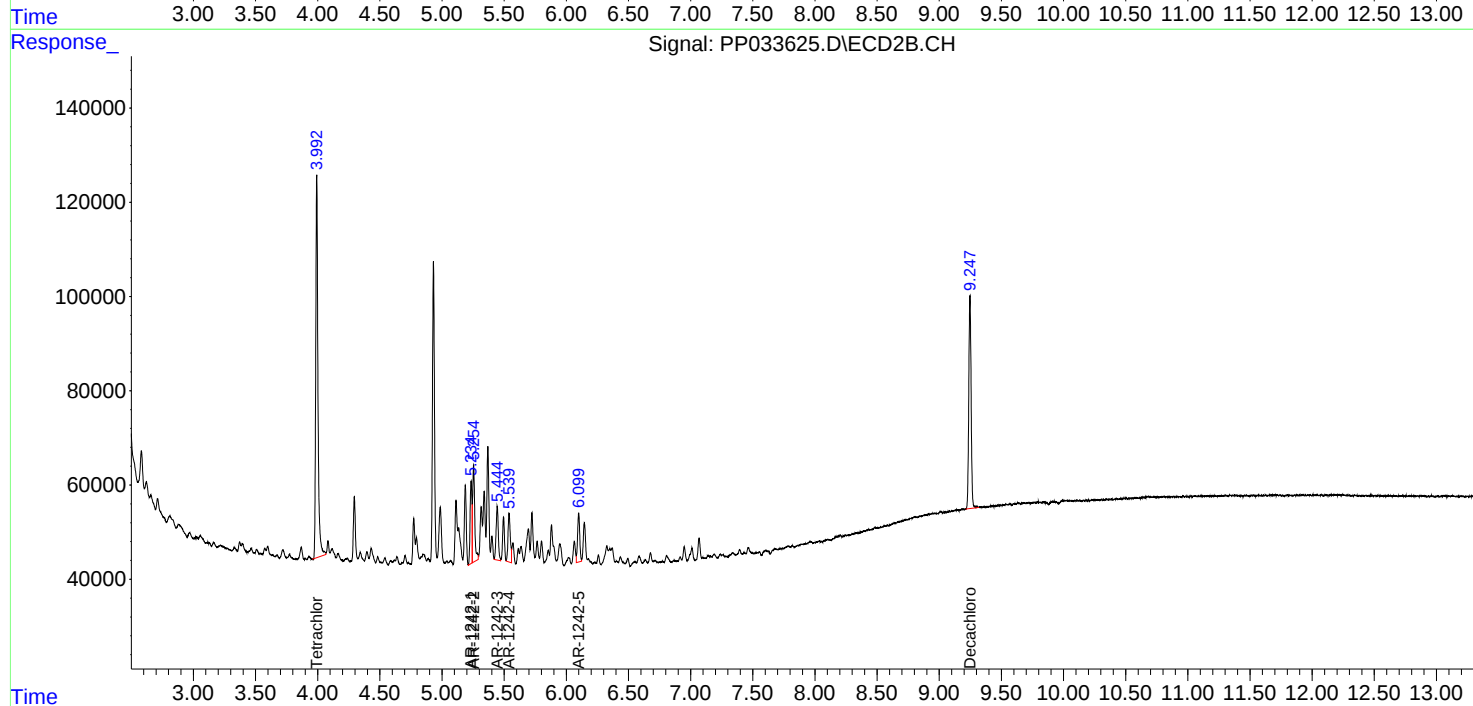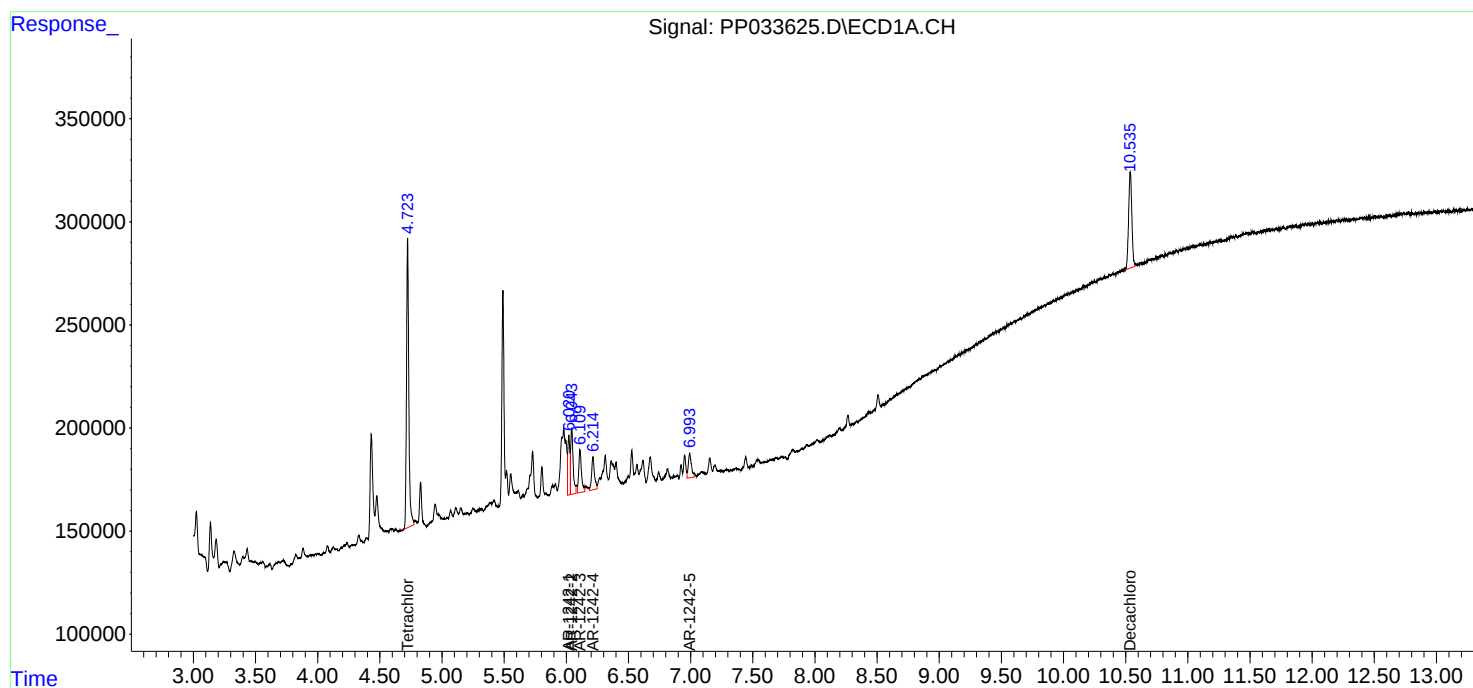

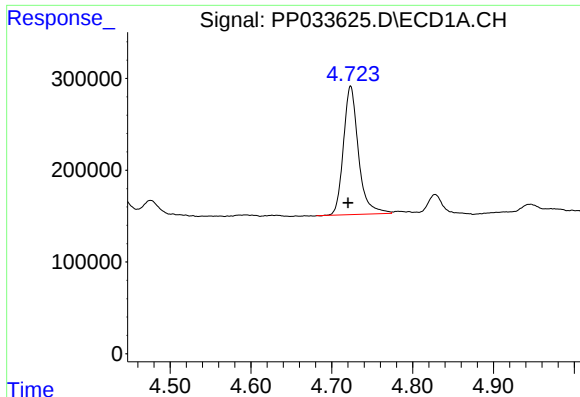


#1 Tetrachloro-m-xylene

R.T.: 4.723 min
Delta R.T.: 0.003 min
Response: 1802724
Conc: 24.49 ng/ml

Instrument :
ECD_P
ClientSampleId :
56-59


Manual Integrations
APPROVED

Ankita
3/2/2021 8:55:50 AM

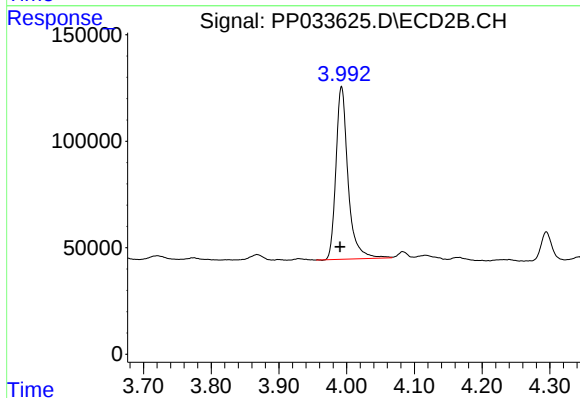


#1 Tetrachloro-m-xylene

R.T.: 3.993 min
Delta R.T.: 0.002 min
Response: 1006290
Conc: 22.85 ng/ml

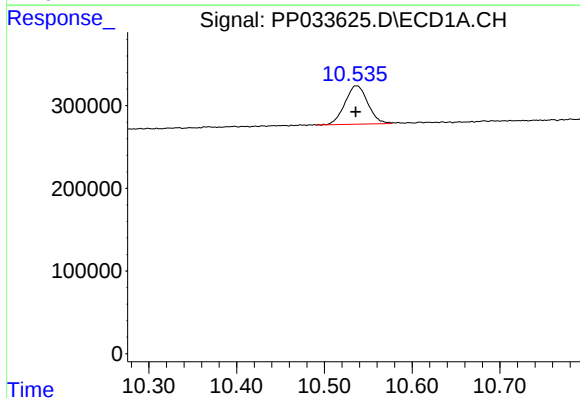


#2 Decachlorobiphenyl

R.T.: 10.536 min
Delta R.T.: 0.000 min
Response: 842353
Conc: 18.11 ng/ml

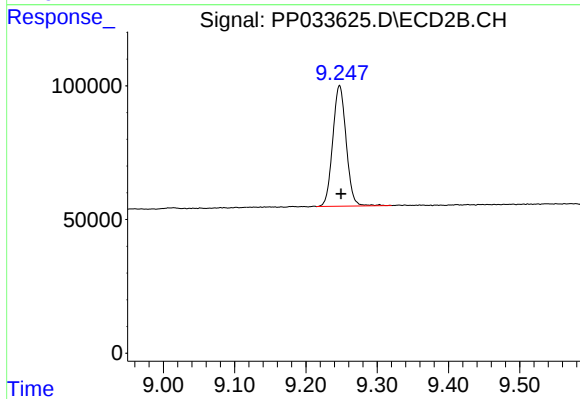

#2 Decachlorobiphenyl

R.T.: 9.247 min
Delta R.T.: -0.002 min
Response: 589461
Conc: 18.66 ng/ml

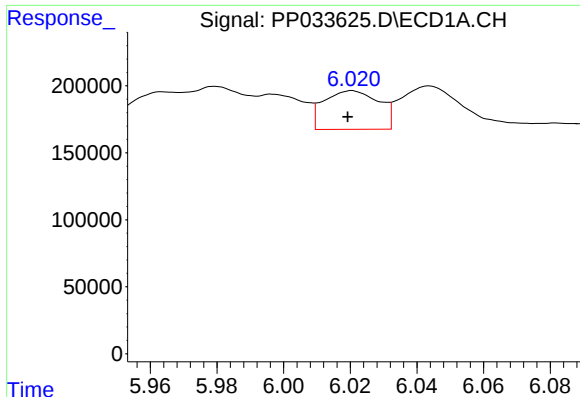


#16 AR-1242-1

R.T.: 6.021 min
Delta R.T.: 0.001 min
Response: 330664
Conc: 226.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
56-59


Manual Integrations
APPROVED

Ankita
3/2/2021 8:55:50 AM

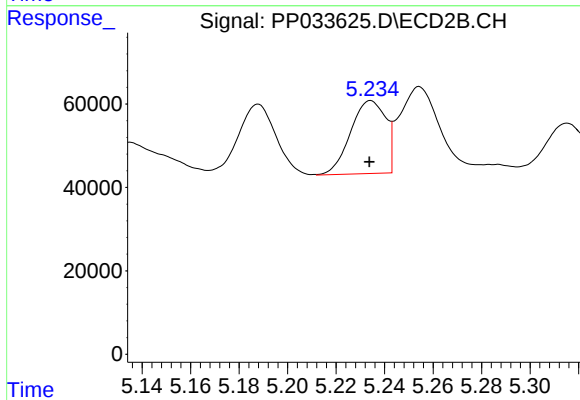


#16 AR-1242-1

R.T.: 5.234 min
Delta R.T.: 0.000 min
Response: 174578
Conc: 191.96 ng/ml m

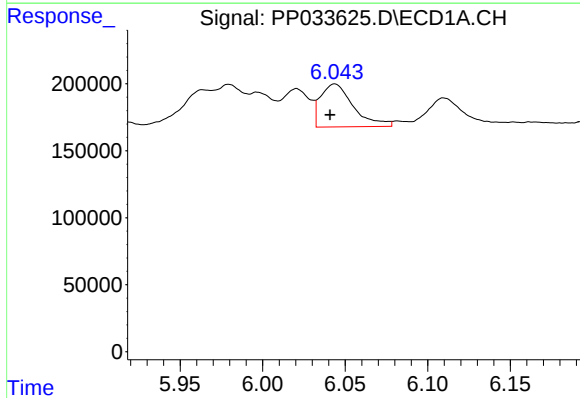


#17 AR-1242-2

R.T.: 6.044 min
Delta R.T.: 0.003 min
Response: 440704
Conc: 197.72 ng/ml

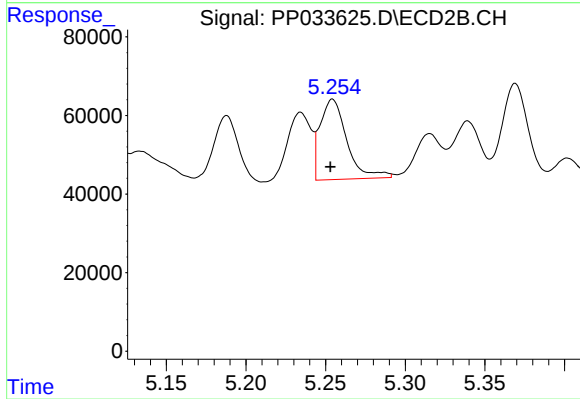

#17 AR-1242-2

R.T.: 5.254 min
Delta R.T.: 0.000 min
Response: 236904
Conc: 176.16 ng/ml m

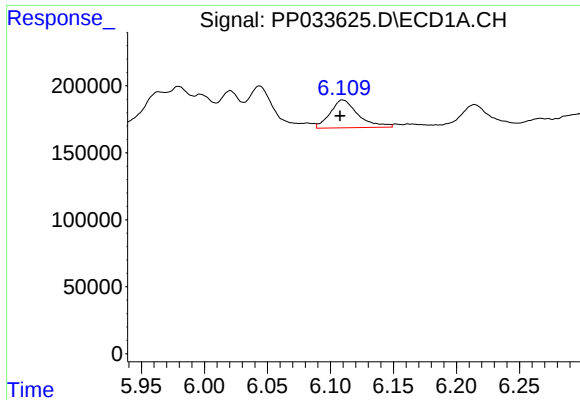


#18 AR-1242-3

R.T.: 6.109 min
Delta R.T.: 0.002 min
Response: 320865
Conc: 232.22 ng/ml

Instrument :
ECD_P
ClientSampleId :
56-59


Manual Integrations
APPROVED

Ankita
3/2/2021 8:55:50 AM

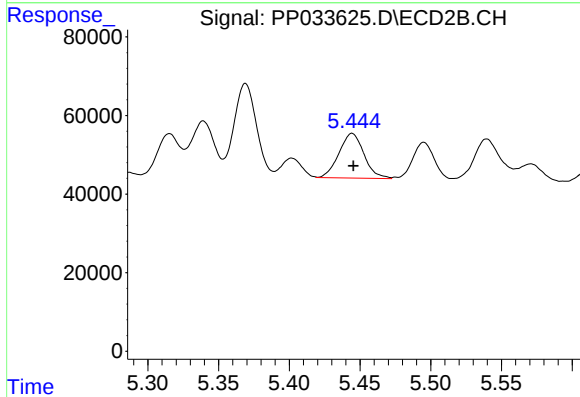


#18 AR-1242-3

R.T.: 5.444 min
Delta R.T.: -0.001 min
Response: 140124
Conc: 190.57 ng/ml m

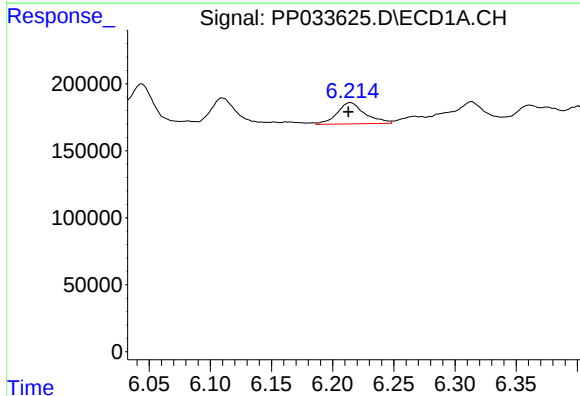


#19 AR-1242-4

R.T.: 6.214 min
Delta R.T.: 0.002 min
Response: 253309
Conc: 218.36 ng/ml

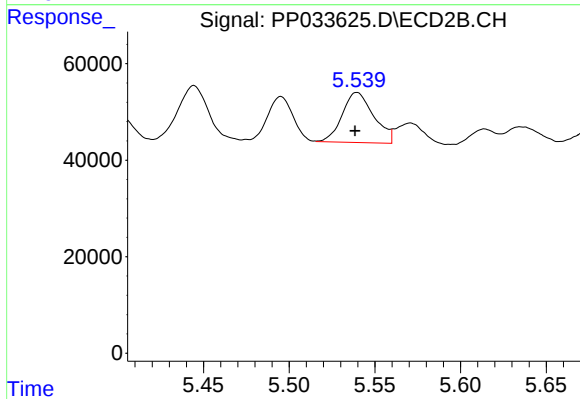

#19 AR-1242-4

R.T.: 5.540 min
Delta R.T.: 0.001 min
Response: 133079
Conc: 194.52 ng/ml

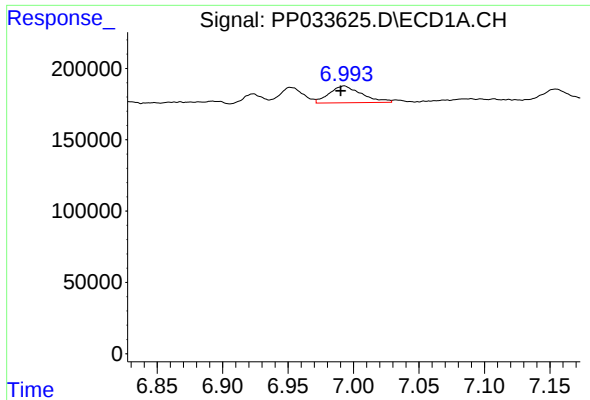


#20 AR-1242-5

R.T.: 6.993 min
Delta R.T.: 0.003 min
Response: 203310
Conc: 181.42 ng/ml

Instrument :
ECD_P
ClientSampleId :
56-59

Manual Integrations
APPROVED

Ankita
3/2/2021 8:55:50 AM

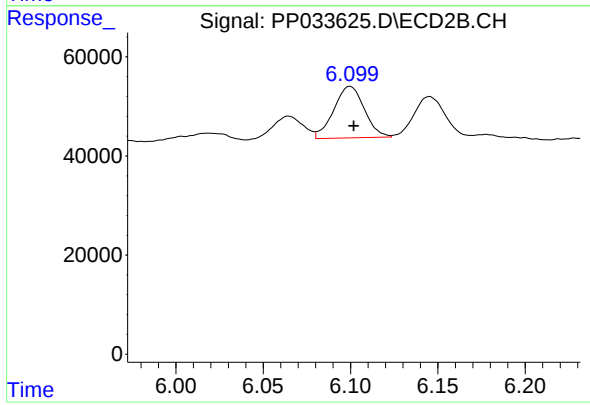

#20 AR-1242-5

R.T.: 6.100 min
Delta R.T.: -0.002 min
Response: 126763
Conc: 167.26 ng/ml