

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030121\
 Data File : PP033628.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Mar 2021 16:19
 Operator : DD\AJ
 Sample : M1488-06
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 41697

Manual Integrations
 APPROVED

Ankita
 3/2/2021 8:55:56 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 17:23:27 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 22 12:13:48 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.724	3.992	1978275	1045470	26.878	23.740m
2) SA Decachlor...	10.537	9.247	692418	488485	14.887	15.460

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030121\
Data File : PP033628.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Mar 2021 16:19
Operator : DD\AJ
Sample : M1488-06
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
41697


Manual Integrations
APPROVED

Ankita
3/2/2021 8:55:56 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 17:23:27 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022121.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 22 12:13:48 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

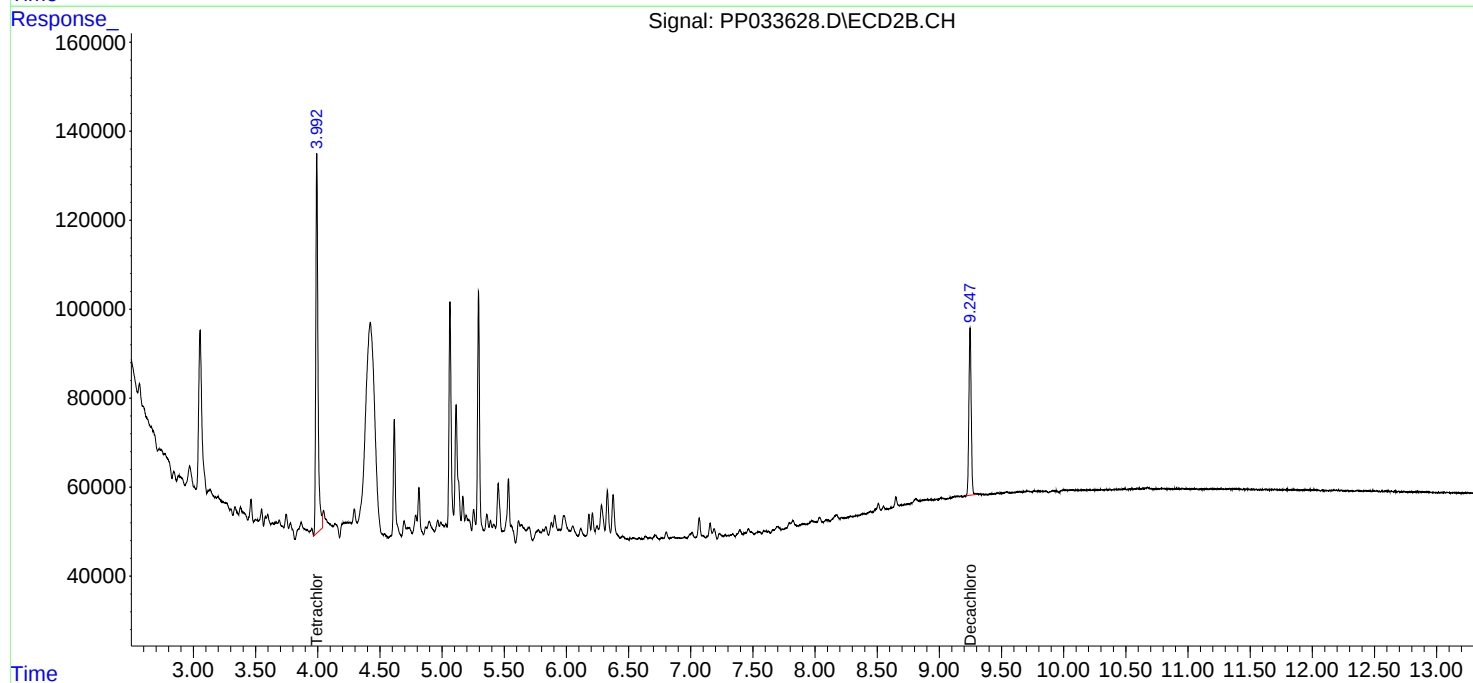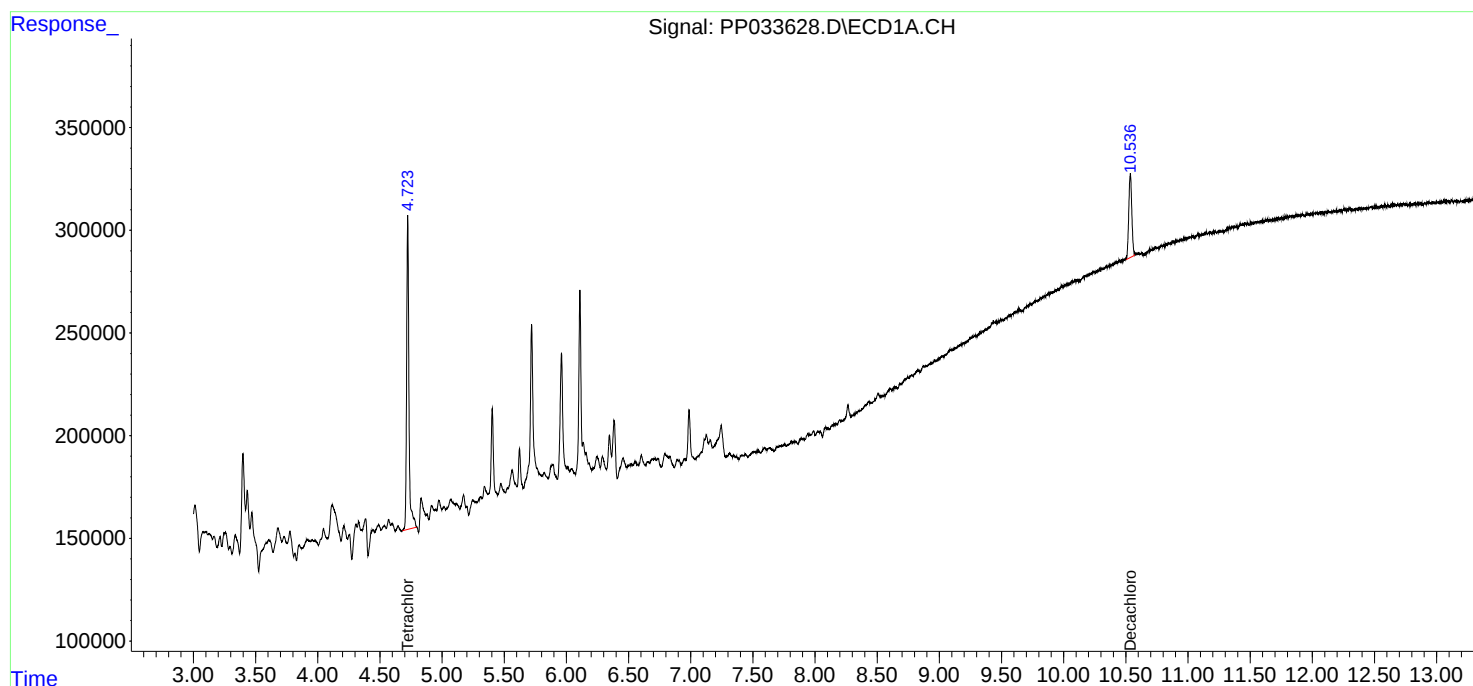

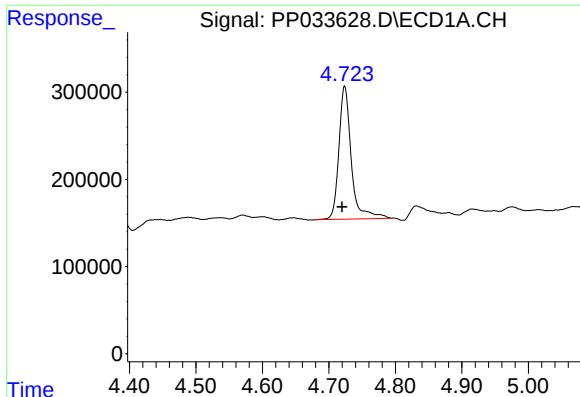


#1 Tetrachloro-m-xylene

R.T.: 4.724 min
Delta R.T.: 0.004 min
Response: 1978275
Conc: 26.88 ng/ml

Instrument :
ECD_P
ClientSampleId :
41697


Manual Integrations
APPROVED

Ankita
3/2/2021 8:55:56 AM

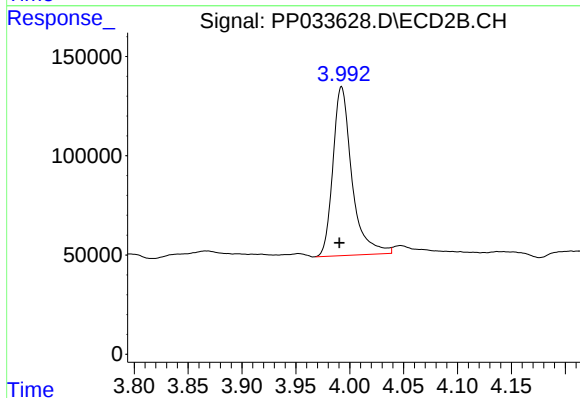


#1 Tetrachloro-m-xylene

R.T.: 3.992 min
Delta R.T.: 0.002 min
Response: 1045470
Conc: 23.74 ng/ml m

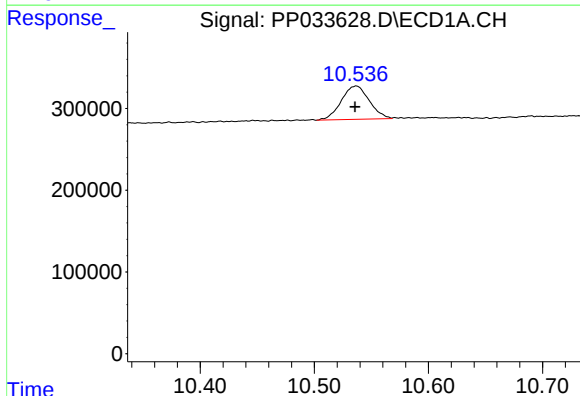

#2 Decachlorobiphenyl

R.T.: 10.537 min
Delta R.T.: 0.001 min
Response: 692418
Conc: 14.89 ng/ml

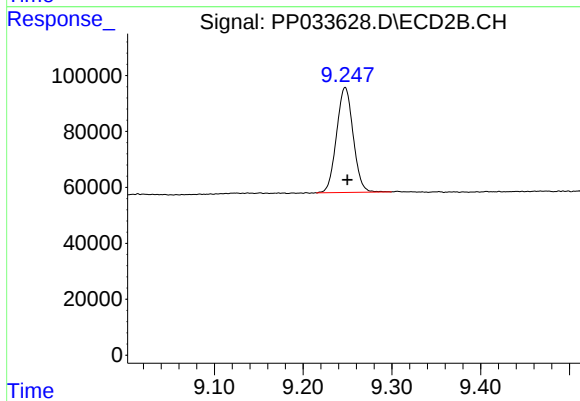

#2 Decachlorobiphenyl

R.T.: 9.247 min
Delta R.T.: -0.002 min
Response: 488485
Conc: 15.46 ng/ml