

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030122\
 Data File : PP044116.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Mar 2022 10:51
 Operator : YP\AJ
 Sample : N1681-04RE
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TP-2-1-8FTRE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/02/2022
 Supervised By :Ankita Jodhani 03/02/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 02 00:08:40 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP021022.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 11 04:48:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.914	3.170	45389499	40914791	20.528	21.783
2) SA Decachlor...	10.057	8.540	55956836	61720985	47.106	38.043m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030122\
Data File : PP044116.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Mar 2022 10:51
Operator : YP\AJ
Sample : N1681-04RE
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
TP-2-1-8FTRE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/02/2022
Supervised By :Ankita Jodhani 03/02/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 02 00:08:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP021022.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 11 04:48:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

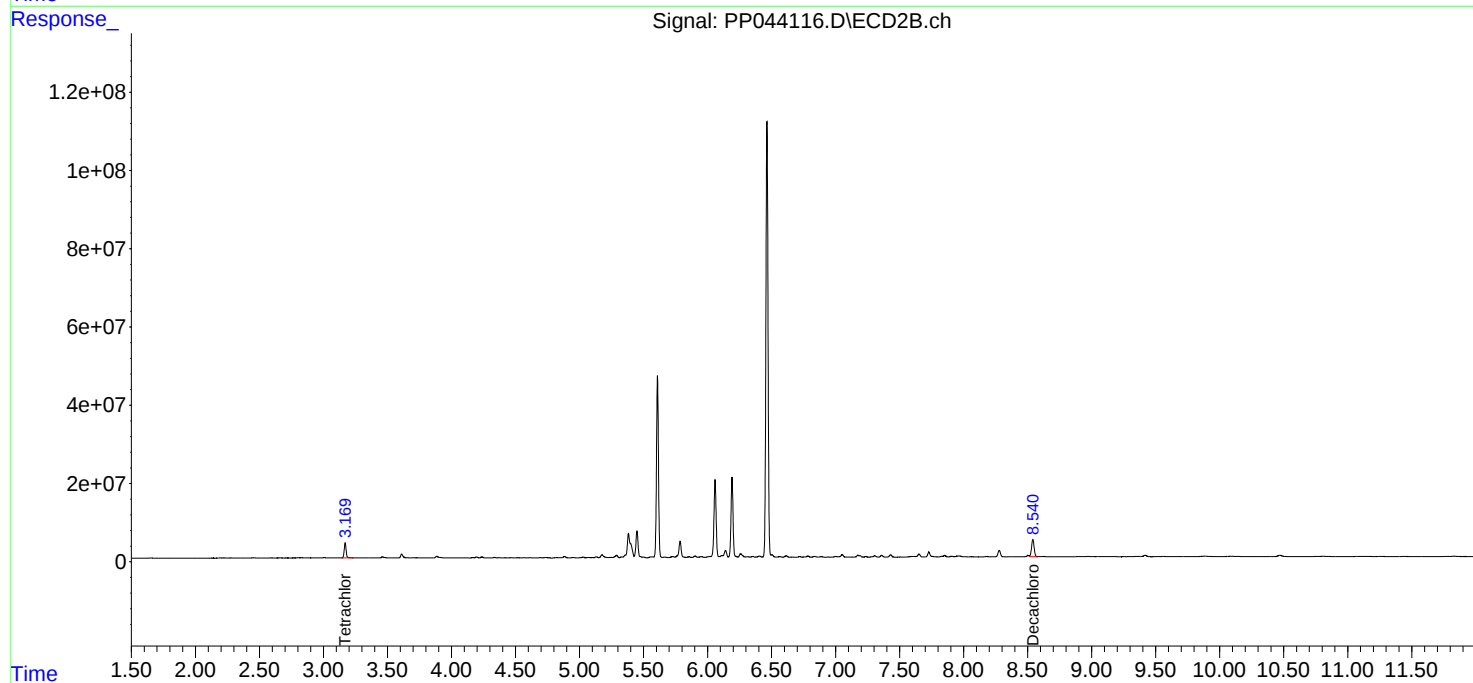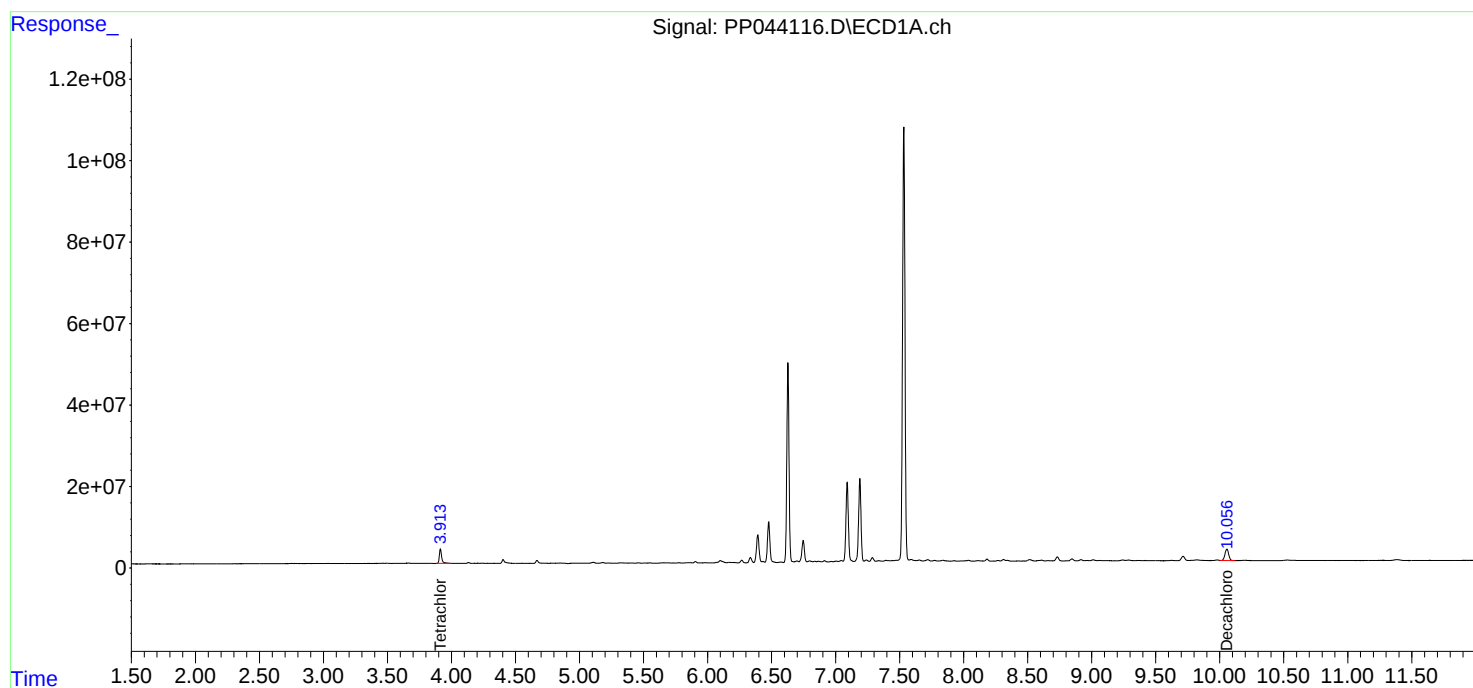

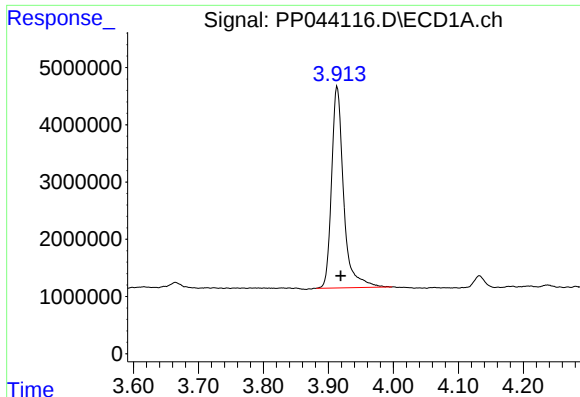


#1 Tetrachloro-m-xylene

R.T.: 3.914 min
Delta R.T.: -0.005 min
Response: 45389499
Conc: 20.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-2-1-8FTRE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/02/2022
Supervised By :Ankita Jodhani 03/02/2022

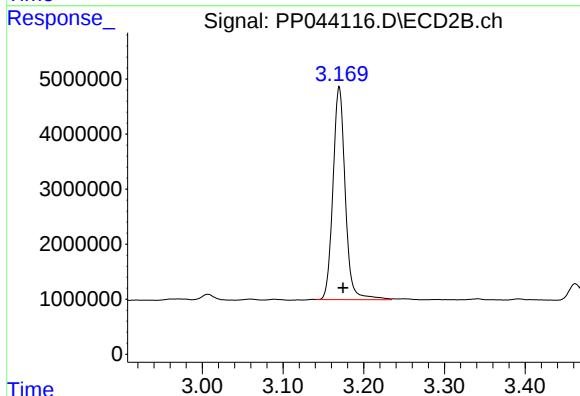


#1 Tetrachloro-m-xylene

R.T.: 3.170 min
Delta R.T.: -0.005 min
Response: 40914791
Conc: 21.78 ng/ml

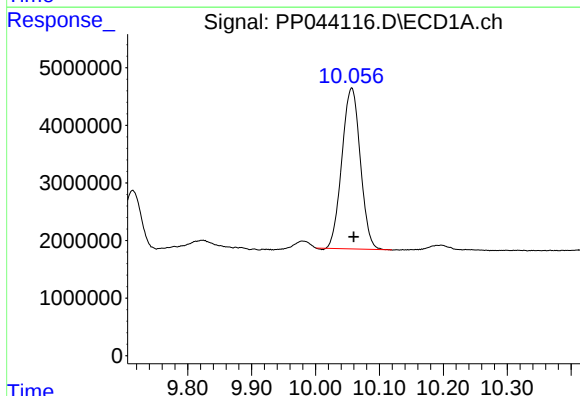

#2 Decachlorobiphenyl

R.T.: 10.057 min
Delta R.T.: -0.003 min
Response: 55956836
Conc: 47.11 ng/ml

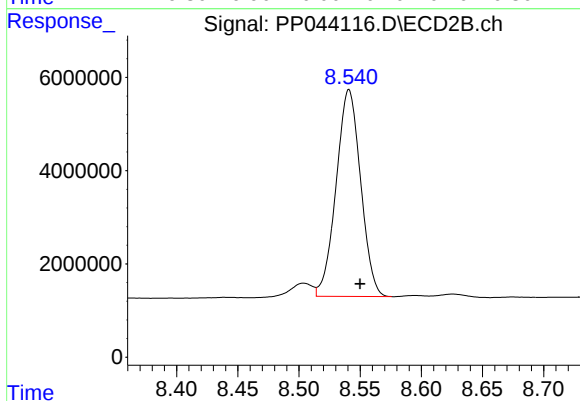

#2 Decachlorobiphenyl

R.T.: 8.540 min
Delta R.T.: -0.010 min
Response: 61720985
Conc: 38.04 ng/ml m