

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030122\
 Data File : PP044133.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Mar 2022 17:57
 Operator : YP\AJ
 Sample : N1705-01DL 2X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 2171-BDL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/02/2022
 Supervised By :Ankita Jodhani 03/02/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 02 00:20:43 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP021022.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Feb 11 04:48:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.914	3.170	22542732	20169244	10.195	10.738
2) SA Decachlor...	10.054	8.539	12955616	16855787	10.906	10.389
Target Compounds						
31) L7 AR-1260-1	6.912	5.902	68743717	70930420	820.897	886.964
32) L7 AR-1260-2	7.195	6.109	85544511	92003492	945.027m	942.148
33) L7 AR-1260-3	7.591	6.271	49903812	77707916	688.437	851.208
34) L7 AR-1260-4	7.839	6.785	68268216	61559691	795.145	760.840
35) L7 AR-1260-5	8.181	7.051	129.7E6	157.6E6	836.796	852.359

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030122\
Data File : PP044133.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Mar 2022 17:57
Operator : YP\AJ
Sample : N1705-01DL 2X
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
2171-BDL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/02/2022
Supervised By :Ankita Jodhani 03/02/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 02 00:20:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP021022.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Feb 11 04:48:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

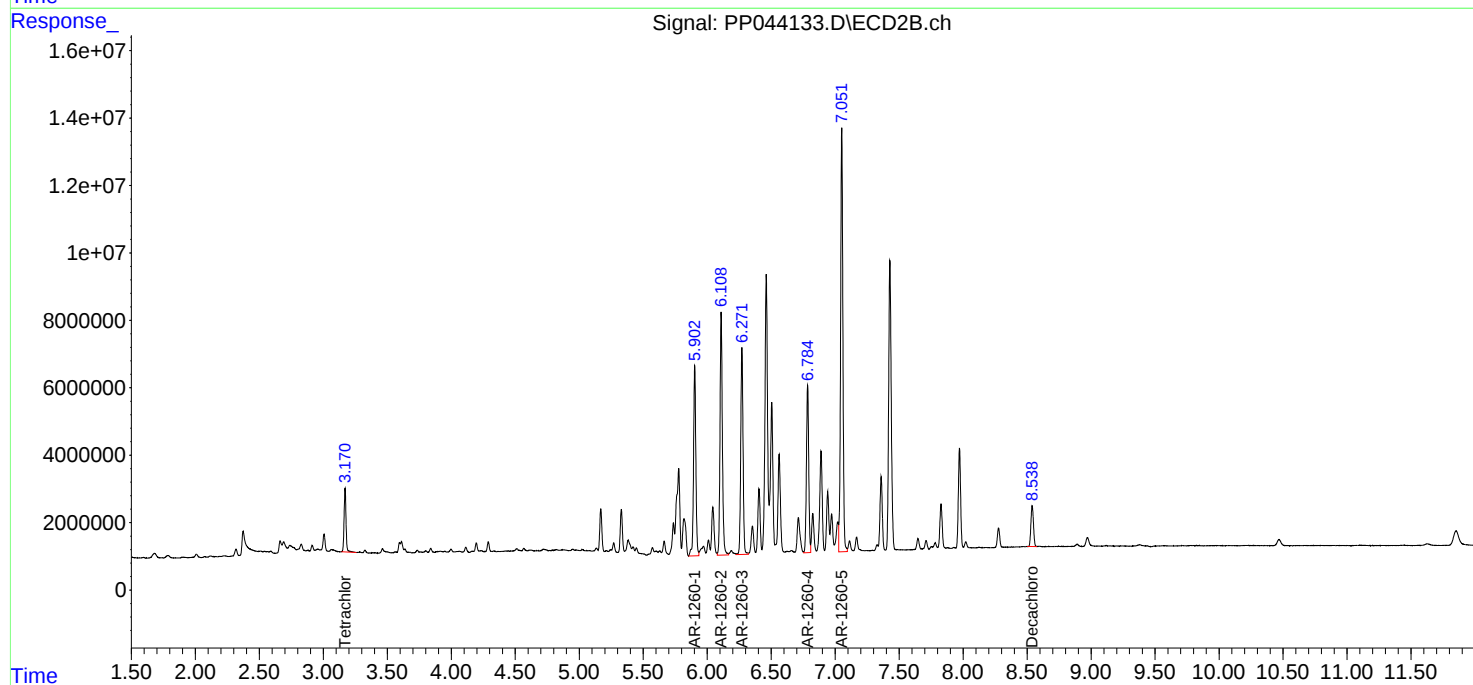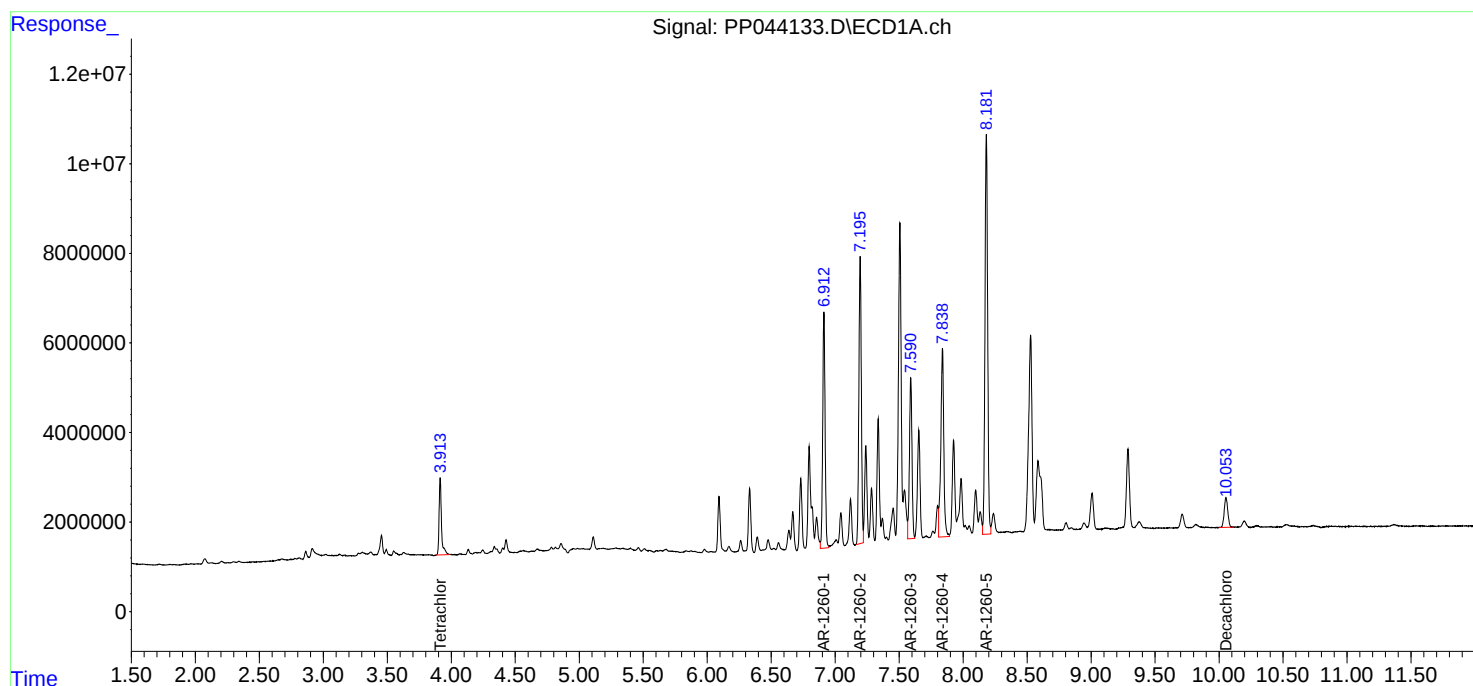

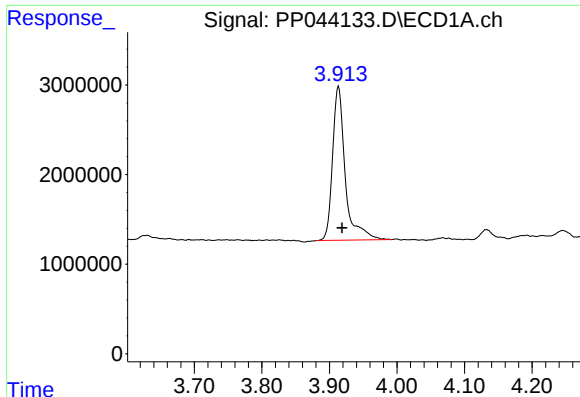


#1 Tetrachloro-m-xylene

R.T.: 3.914 min
Delta R.T.: -0.005 min
Response: 22542732
Conc: 10.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
2171-BDL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/02/2022
Supervised By :Ankita Jodhani 03/02/2022

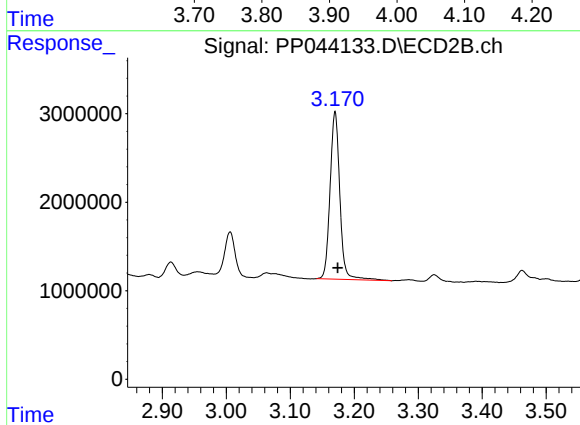


#1 Tetrachloro-m-xylene

R.T.: 3.170 min
Delta R.T.: -0.004 min
Response: 20169244
Conc: 10.74 ng/ml

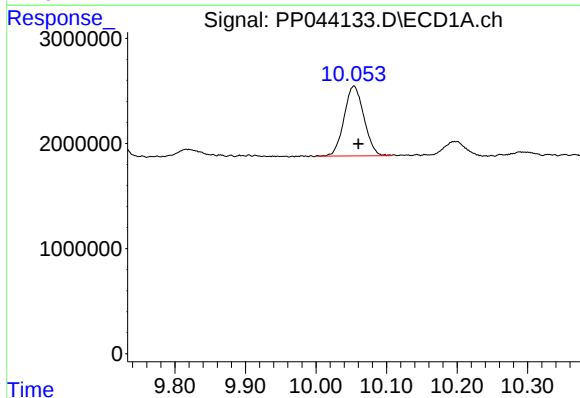


#2 Decachlorobiphenyl

R.T.: 10.054 min
Delta R.T.: -0.006 min
Response: 12955616
Conc: 10.91 ng/ml

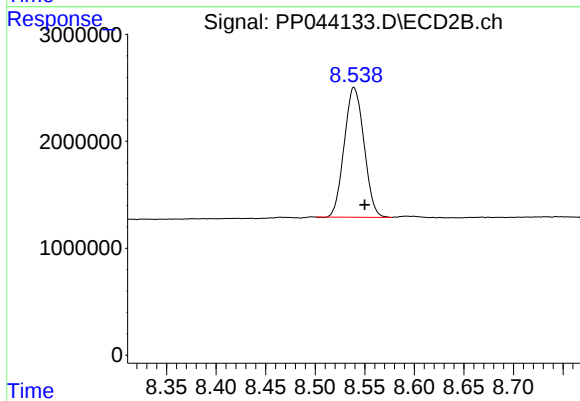

#2 Decachlorobiphenyl

R.T.: 8.539 min
Delta R.T.: -0.011 min
Response: 16855787
Conc: 10.39 ng/ml

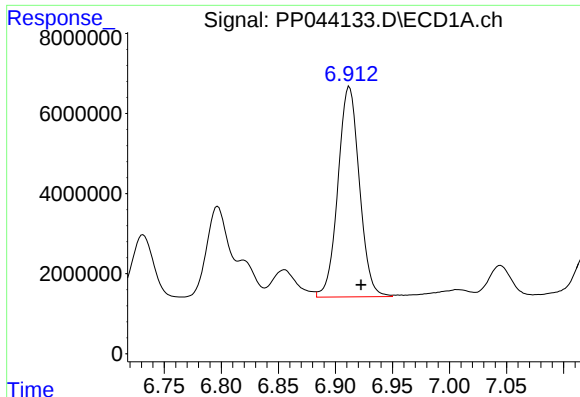


#31 AR-1260-1

R.T.: 6.912 min
Delta R.T.: -0.010 min
Response: 68743717
Conc: 820.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
2171-BDL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/02/2022
Supervised By :Ankita Jodhani 03/02/2022

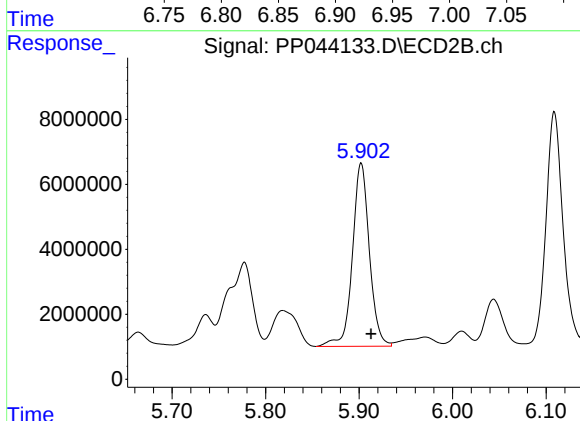


#31 AR-1260-1

R.T.: 5.902 min
Delta R.T.: -0.011 min
Response: 70930420
Conc: 886.96 ng/ml

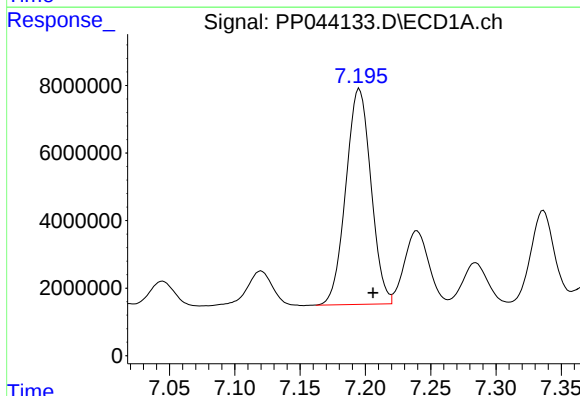


#32 AR-1260-2

R.T.: 7.195 min
Delta R.T.: -0.011 min
Response: 85544511
Conc: 945.03 ng/ml m

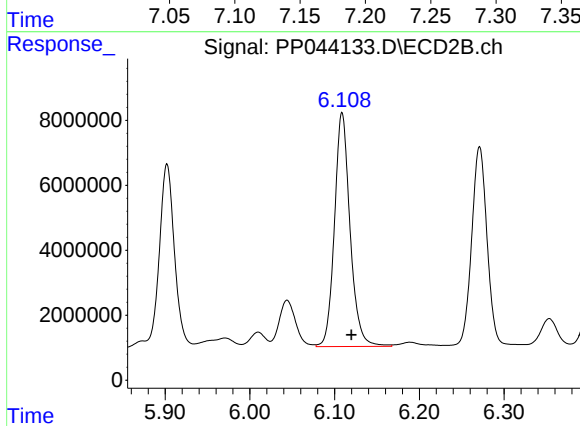

#32 AR-1260-2

R.T.: 6.109 min
Delta R.T.: -0.011 min
Response: 92003492
Conc: 942.15 ng/ml

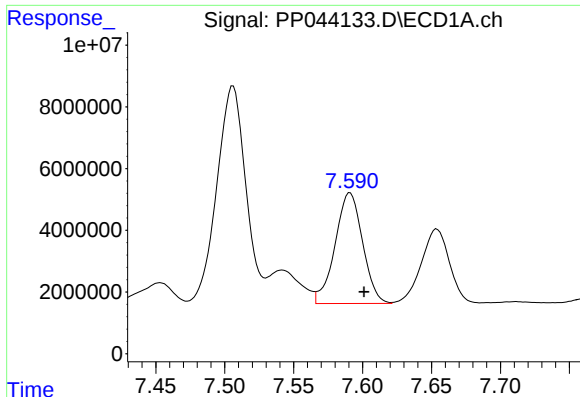


#33 AR-1260-3

R.T.: 7.591 min
Delta R.T.: -0.010 min
Response: 49903812
Conc: 688.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
2171-BDL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/02/2022
Supervised By :Ankita Jodhani 03/02/2022

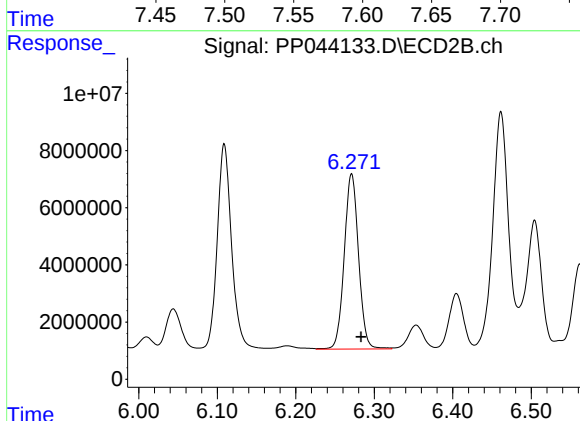


#33 AR-1260-3

R.T.: 6.271 min
Delta R.T.: -0.012 min
Response: 77707916
Conc: 851.21 ng/ml

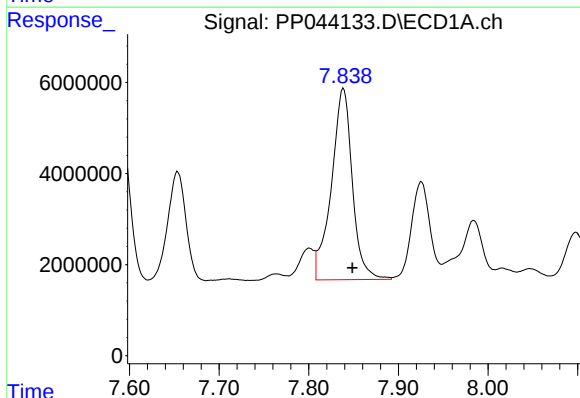


#34 AR-1260-4

R.T.: 7.839 min
Delta R.T.: -0.010 min
Response: 68268216
Conc: 795.14 ng/ml

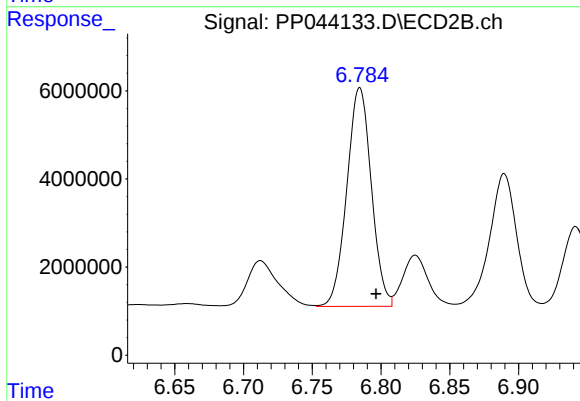

#34 AR-1260-4

R.T.: 6.785 min
Delta R.T.: -0.012 min
Response: 61559691
Conc: 760.84 ng/ml

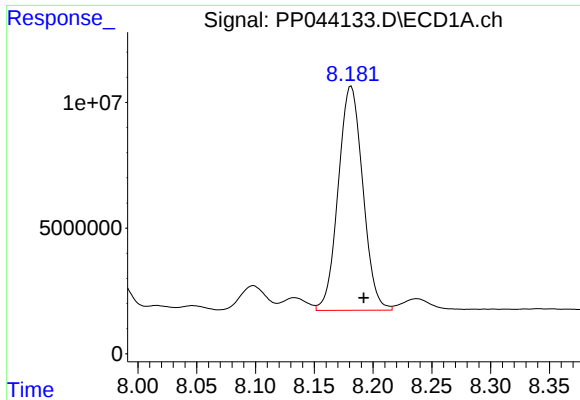


#35 AR-1260-5

R.T.: 8.181 min
Delta R.T.: -0.011 min
Response: 129709453
Conc: 836.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
2171-BDL

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/02/2022
Supervised By :Ankita Jodhani 03/02/2022

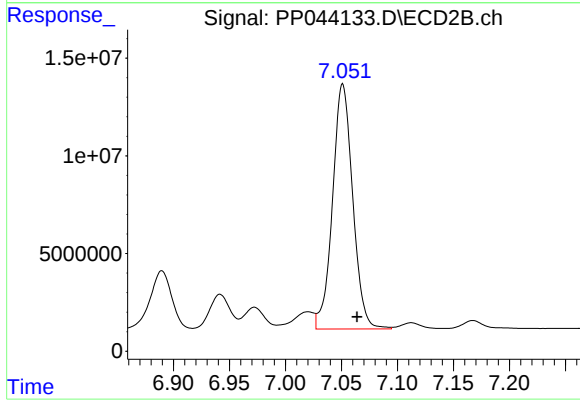

#35 AR-1260-5

R.T.: 7.051 min
Delta R.T.: -0.013 min
Response: 157571428
Conc: 852.36 ng/ml