

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030123\
 Data File : PP056132.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Mar 2023 16:58
 Operator : YP\AJ
 Sample : 01739-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SAMPLE-1-COMP-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 01 20:38:54 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP021723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 20 05:24:03 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.321	3.564	36580755	28053095	22.703	19.212
2) SA Decachlor...	10.066	8.565	33436126	19149696	16.391	16.879

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030123\
Data File : PP056132.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Mar 2023 16:58
Operator : YP\AJ
Sample : 01739-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
SAMPLE-1-COMP-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 01 20:38:54 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP021723.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 20 05:24:03 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

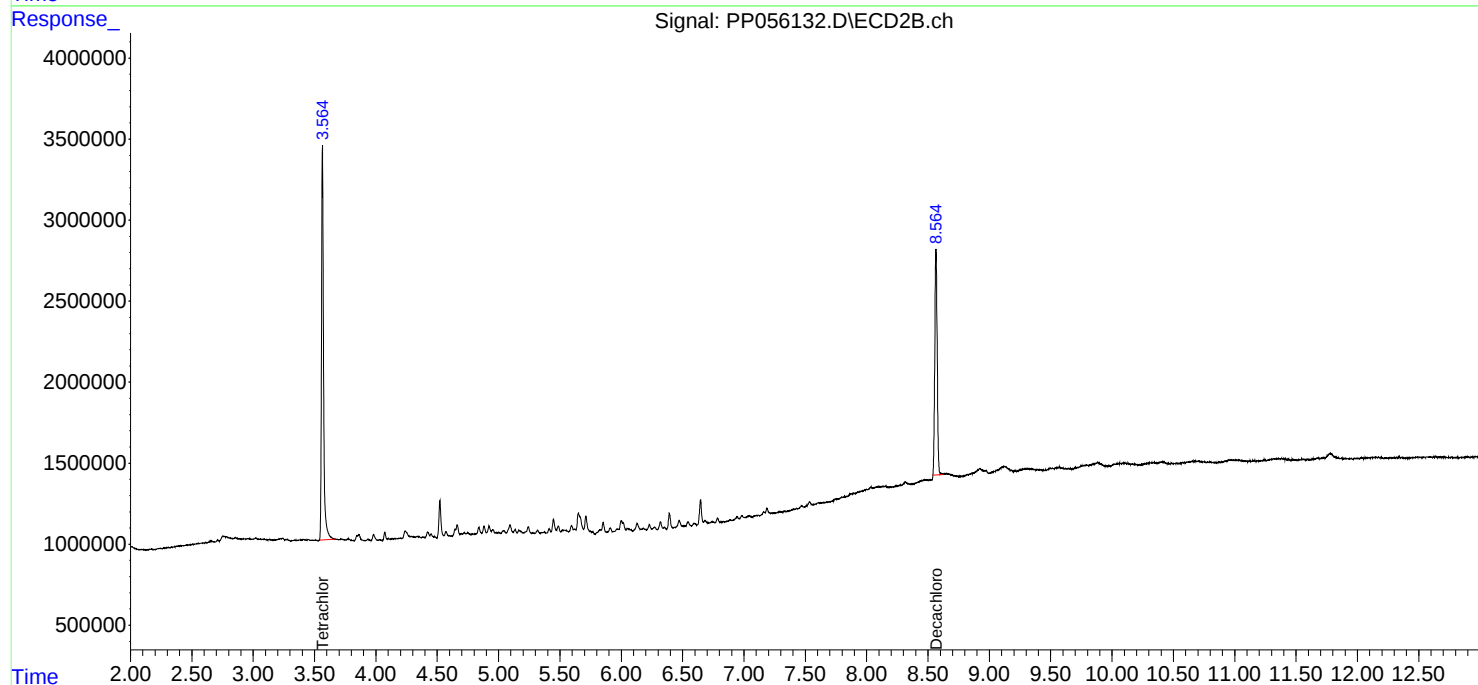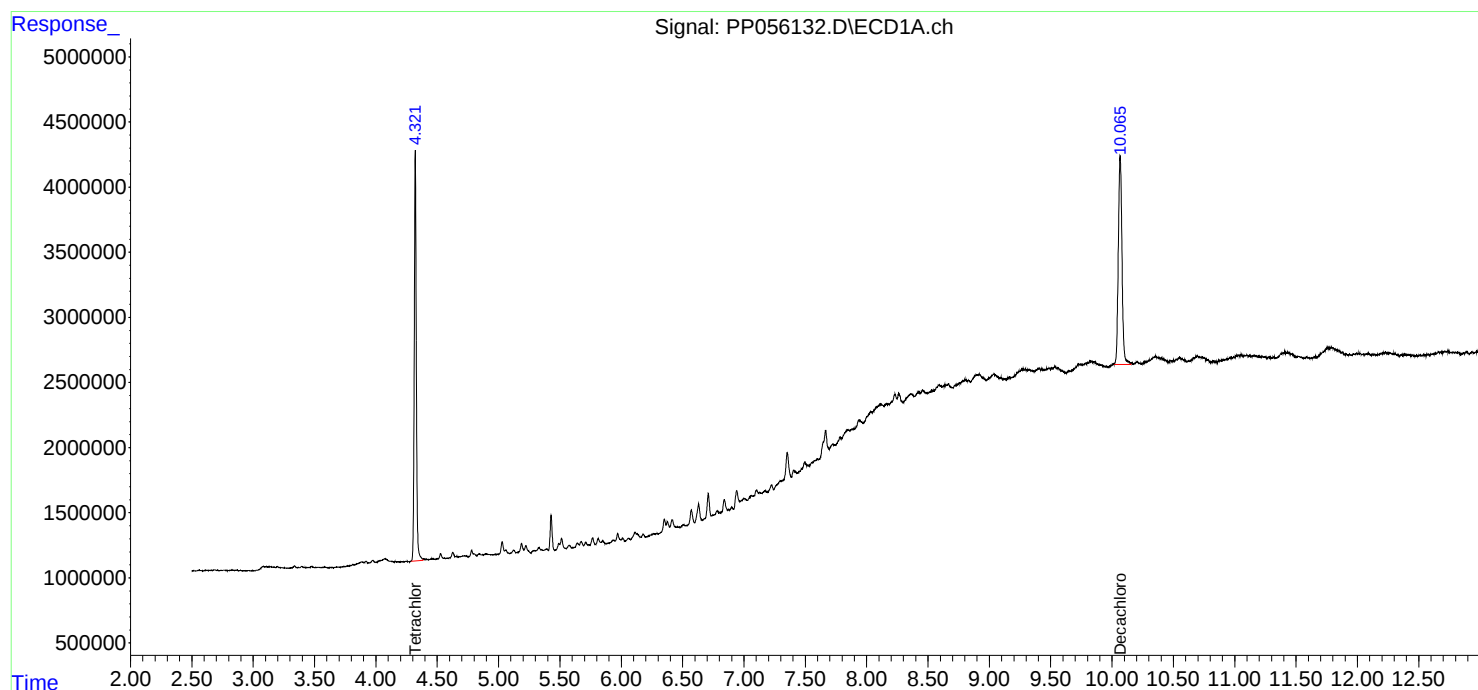


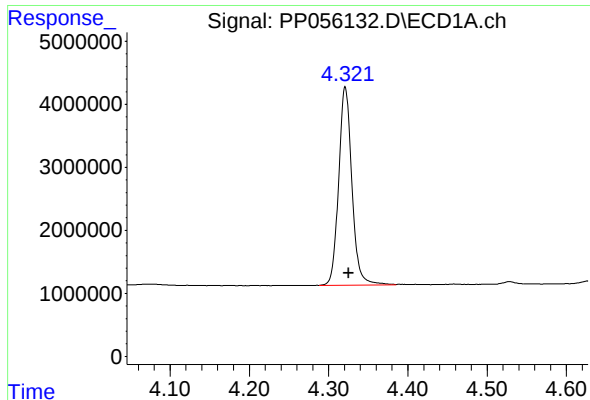

#1 Tetrachloro-m-xylene


R.T.: 4.321 min
Delta R.T.: -0.004 min
Response: 36580755
Conc: 22.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
SAMPLE-1-COMP-1

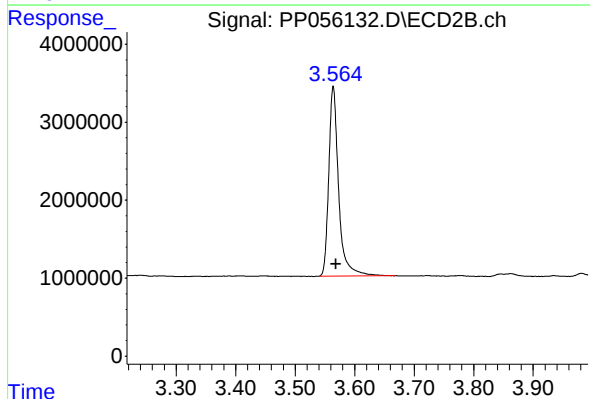


#1 Tetrachloro-m-xylene

R.T.: 3.564 min
Delta R.T.: -0.005 min
Response: 28053095
Conc: 19.21 ng/ml

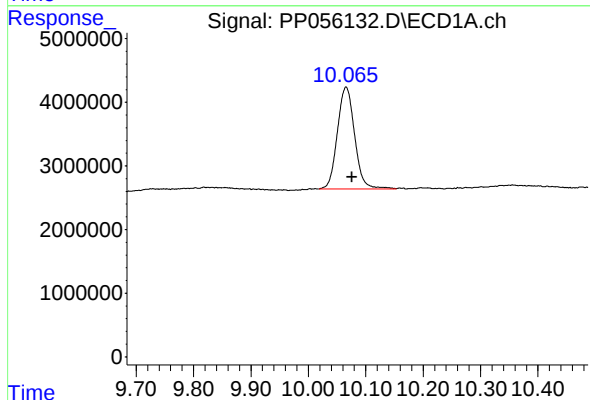

#2 Decachlorobiphenyl

R.T.: 10.066 min
Delta R.T.: -0.010 min
Response: 33436126
Conc: 16.39 ng/ml

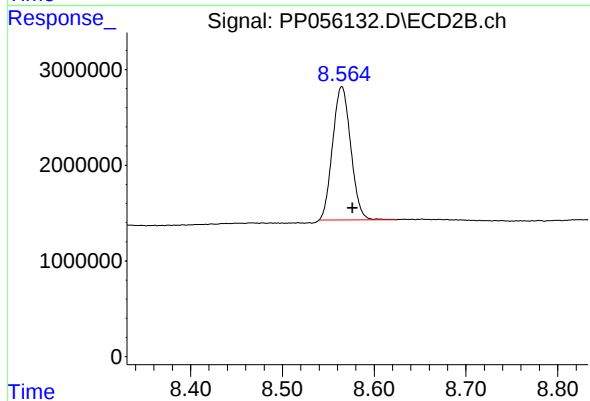

#2 Decachlorobiphenyl

R.T.: 8.565 min
Delta R.T.: -0.012 min
Response: 19149696
Conc: 16.88 ng/ml