

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030322\
 Data File : PP044211.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Mar 2022 14:51
 Operator : YP\AJ
 Sample : N1731-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 VACLOT-TOPSOIL-GRILLO-01

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/04/2022
 Supervised By :Ankita Jodhani 03/04/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 04 01:00:34 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 03 02:21:53 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.910	3.166	34833992	33458792	16.812m	19.125
2) SA Decachlor...	10.051	8.535	16451824	19121600	11.953	12.465

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030322\
Data File : PP044211.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Mar 2022 14:51
Operator : YP\AJ
Sample : N1731-01
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
VACLOT-TOPSOIL-GRILLO-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/04/2022
Supervised By :Ankita Jodhani 03/04/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 04 01:00:34 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 03 02:21:53 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

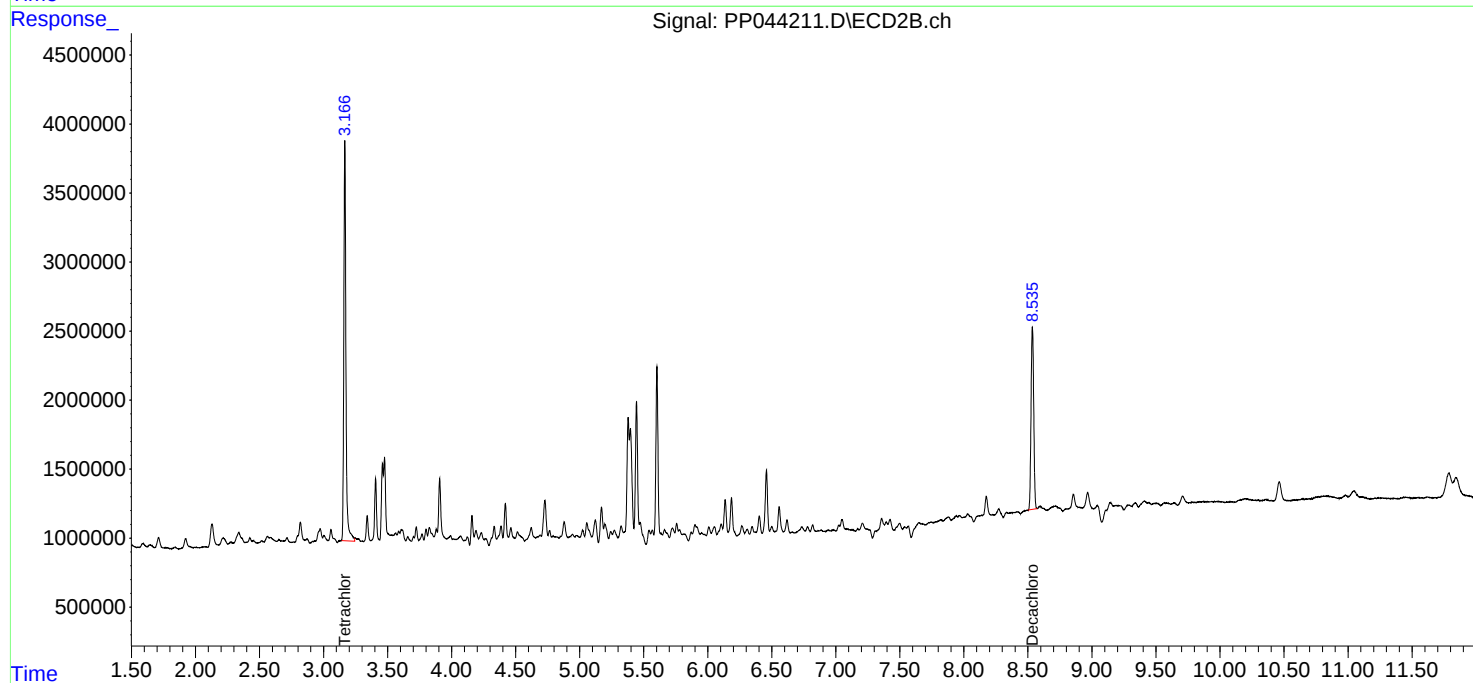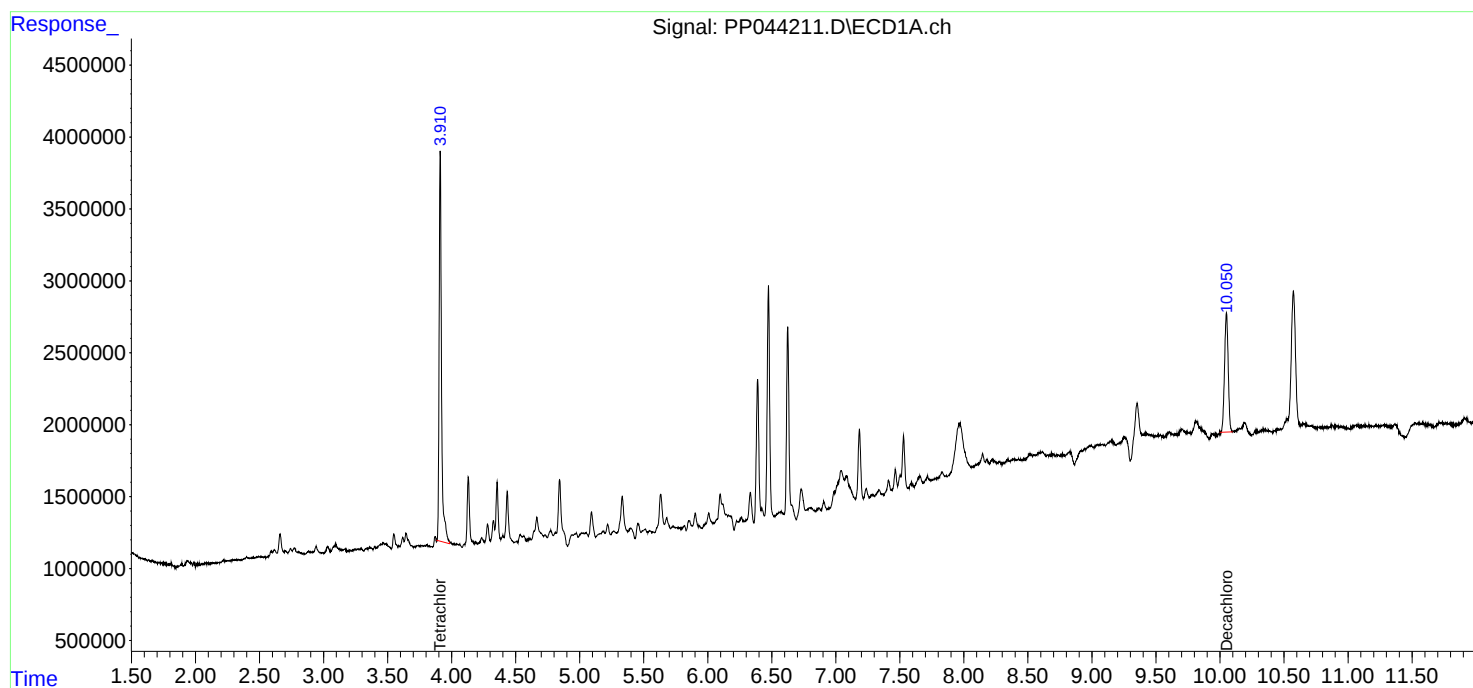

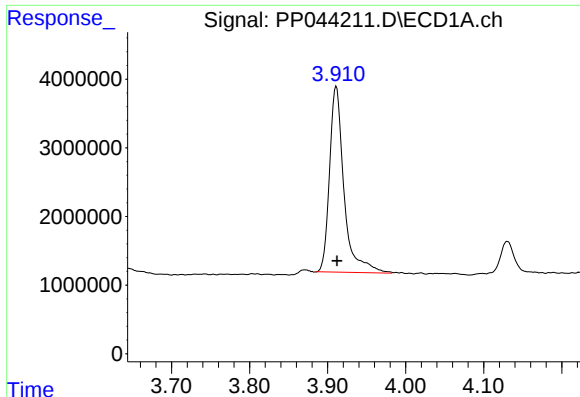


#1 Tetrachloro-m-xylene

R.T.: 3.910 min
Delta R.T.: -0.002 min
Response: 34833992
Conc: 16.81 ng/ml

Instrument :
ECD_P
ClientSampleId :
VACLOT-TOPSOIL-GRILLO-01


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/04/2022
Supervised By :Ankita Jodhani 03/04/2022

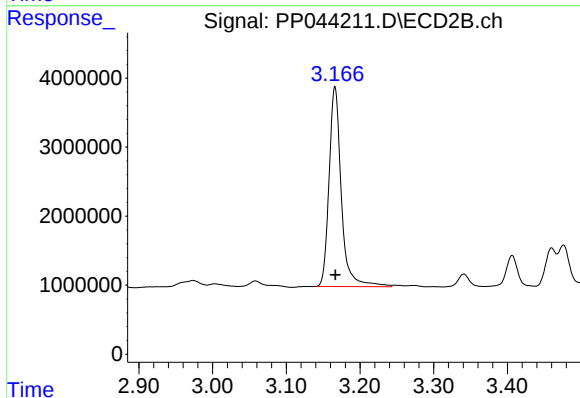


#1 Tetrachloro-m-xylene

R.T.: 3.166 min
Delta R.T.: 0.000 min
Response: 33458792
Conc: 19.13 ng/ml

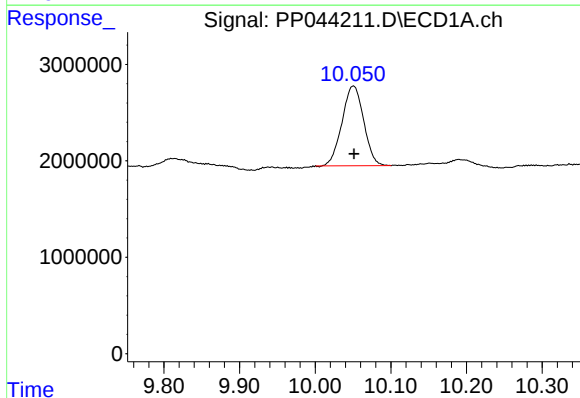

#2 Decachlorobiphenyl

R.T.: 10.051 min
Delta R.T.: 0.000 min
Response: 16451824
Conc: 11.95 ng/ml

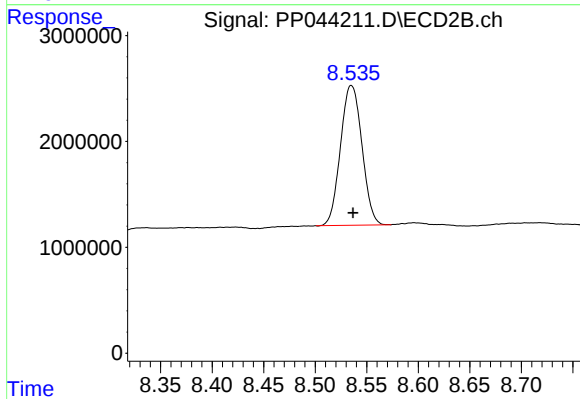

#2 Decachlorobiphenyl

R.T.: 8.535 min
Delta R.T.: -0.002 min
Response: 19121600
Conc: 12.47 ng/ml