

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030323\
 Data File : PP056182.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Mar 2023 15:12
 Operator : YP\AJ
 Sample : 01760-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 RBR200058

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/06/2023
 Supervised By :Ankita Jodhani 03/06/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 03 20:59:35 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP021723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 20 05:24:03 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.327	3.572	37095123	25541263	23.023	17.492
2) SA Decachlor...	10.066	8.564	47500660	32361267	23.285m	28.525

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030323\
Data File : PP056182.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Mar 2023 15:12
Operator : YP\AJ
Sample : 01760-01
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
RBR200058


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/06/2023
Supervised By :Ankita Jodhani 03/06/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 03 20:59:35 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP021723.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 20 05:24:03 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

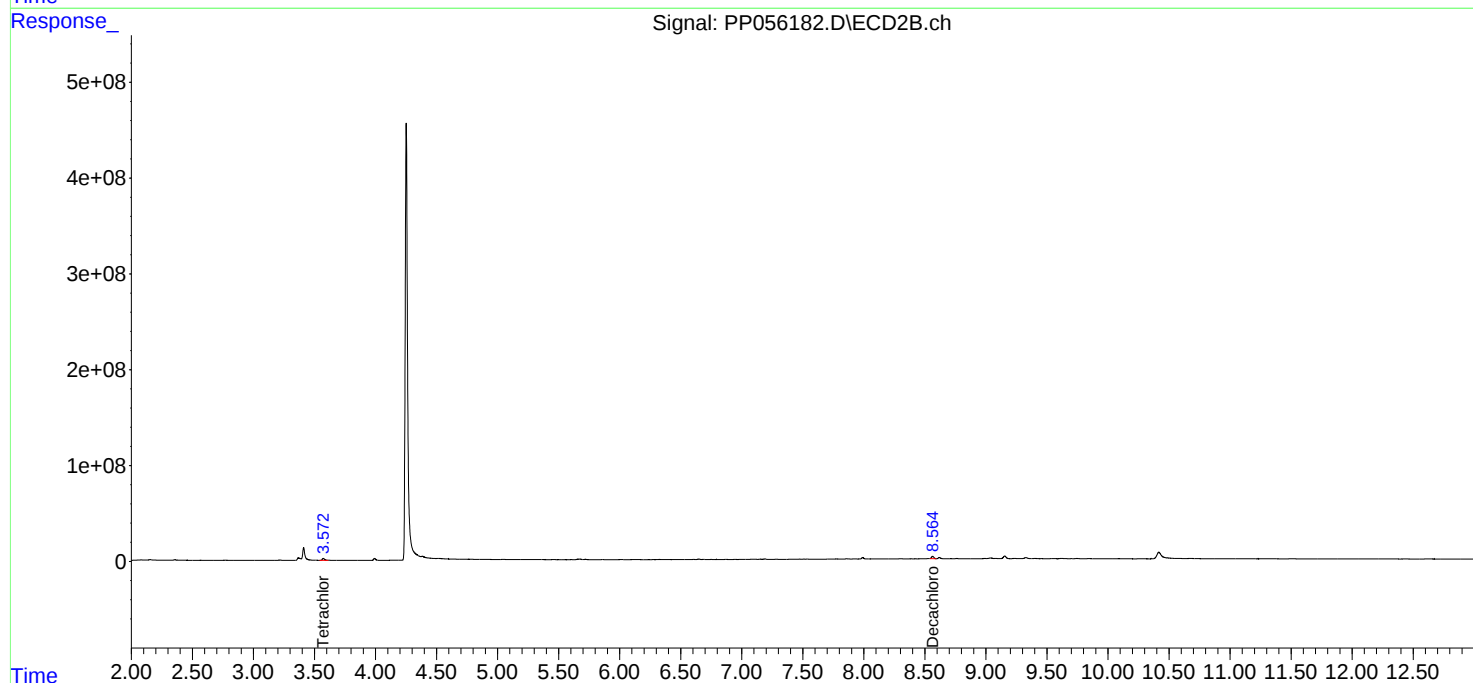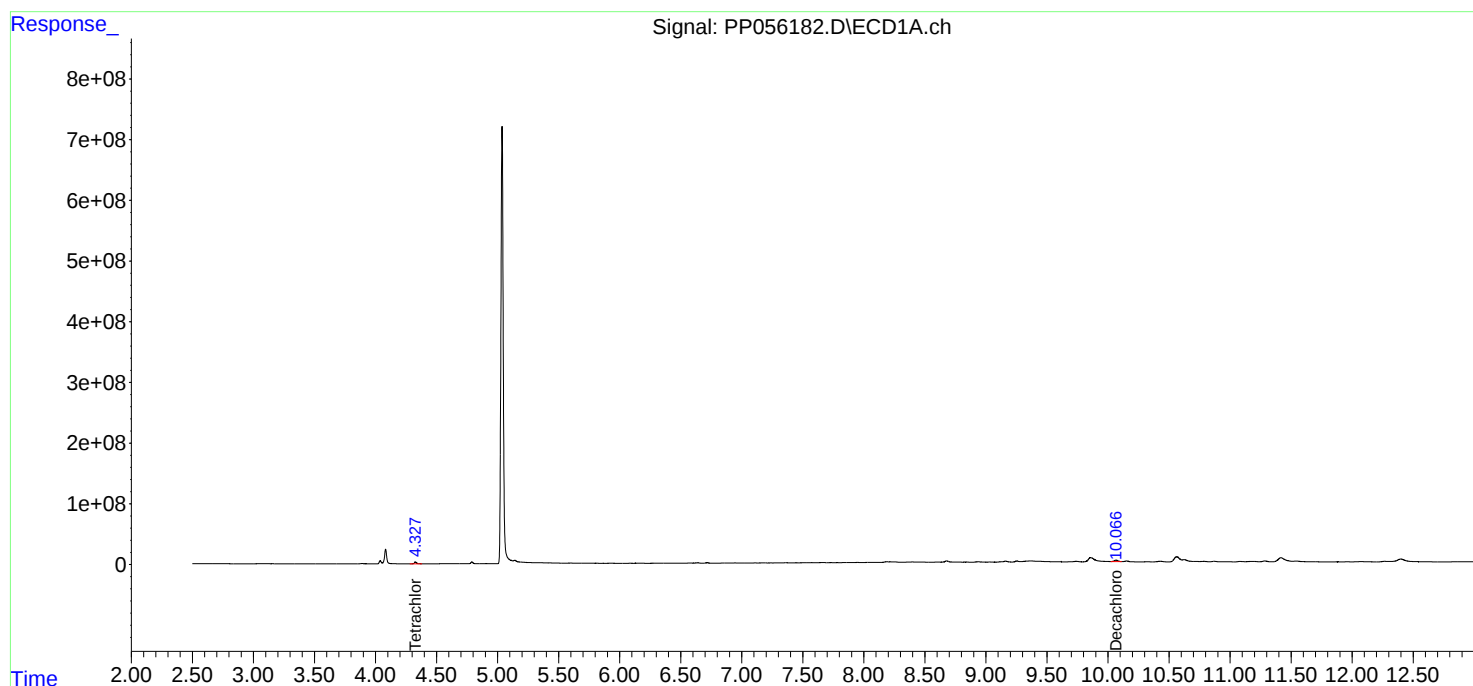

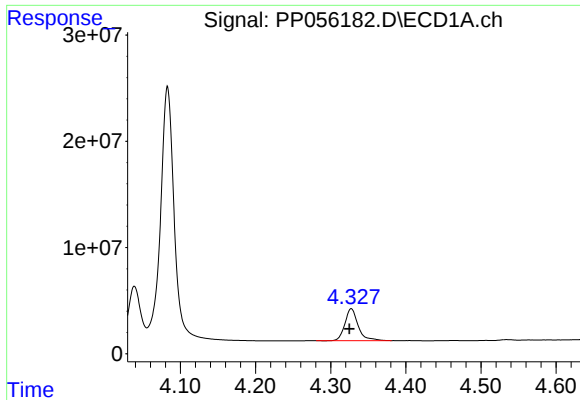


#1 Tetrachloro-m-xylene

R.T.: 4.327 min
Delta R.T.: 0.002 min
Response: 37095123
Conc: 23.02 ng/ml

Instrument :
ECD_P
ClientSampleId :
RBR200058


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/06/2023
Supervised By :Ankita Jodhani 03/06/2023

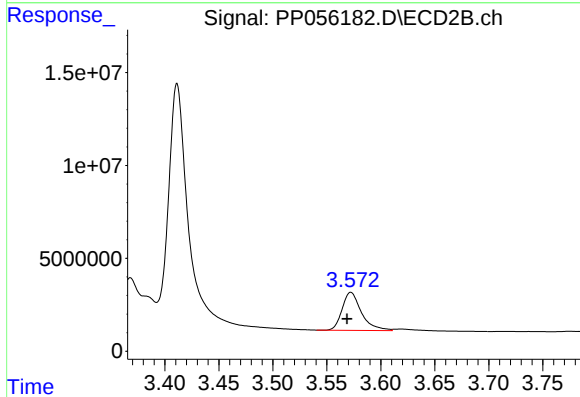


#1 Tetrachloro-m-xylene

R.T.: 3.572 min
Delta R.T.: 0.004 min
Response: 25541263
Conc: 17.49 ng/ml

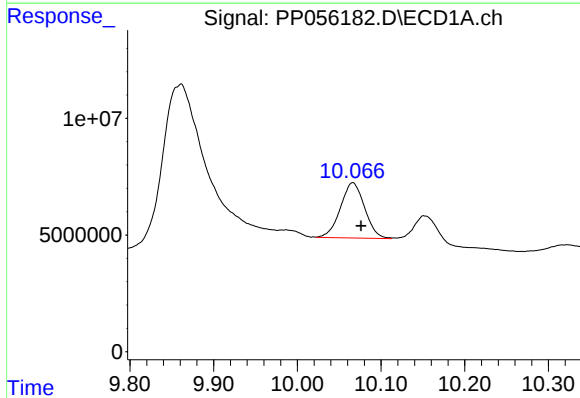

#2 Decachlorobiphenyl

R.T.: 10.066 min
Delta R.T.: -0.010 min
Response: 47500660
Conc: 23.29 ng/ml m

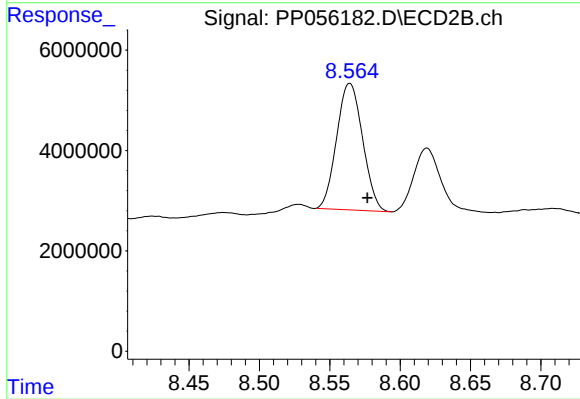

#2 Decachlorobiphenyl

R.T.: 8.564 min
Delta R.T.: -0.012 min
Response: 32361267
Conc: 28.52 ng/ml