

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030323\
 Data File : PP056196.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Mar 2023 19:45
 Operator : YP\AJ
 Sample : 01758-09 10X
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 FMC-1222

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/06/2023
 Supervised By :Ankita Jodhani 03/06/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 03 21:03:30 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP021723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 20 05:24:03 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.320	3.565	2839353	1932010	1.762m	1.323
2) SA Decachlor...	10.066	8.563	3642849	2797532	1.786	2.466 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030323\
Data File : PP056196.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Mar 2023 19:45
Operator : YP\AJ
Sample : 01758-09 10X
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
FMC-1222


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/06/2023
Supervised By :Ankita Jodhani 03/06/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 03 21:03:30 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP021723.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 20 05:24:03 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

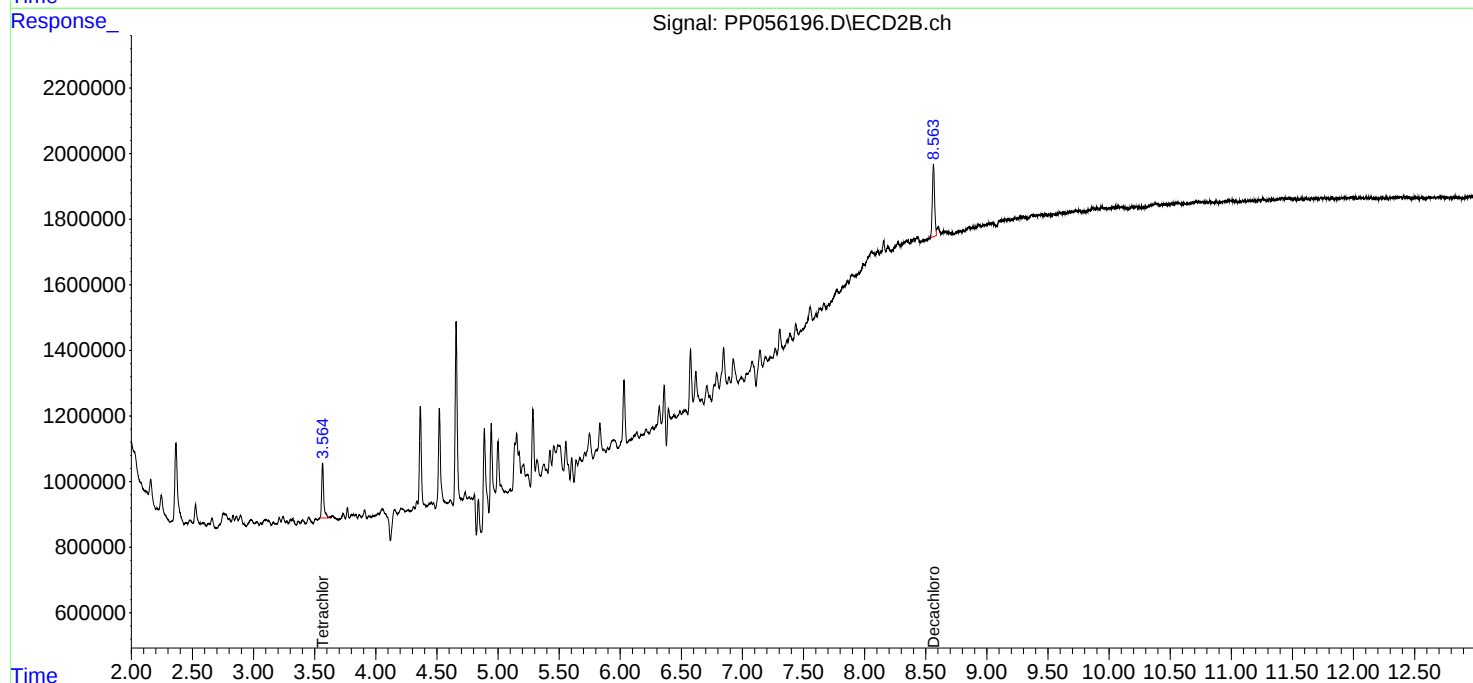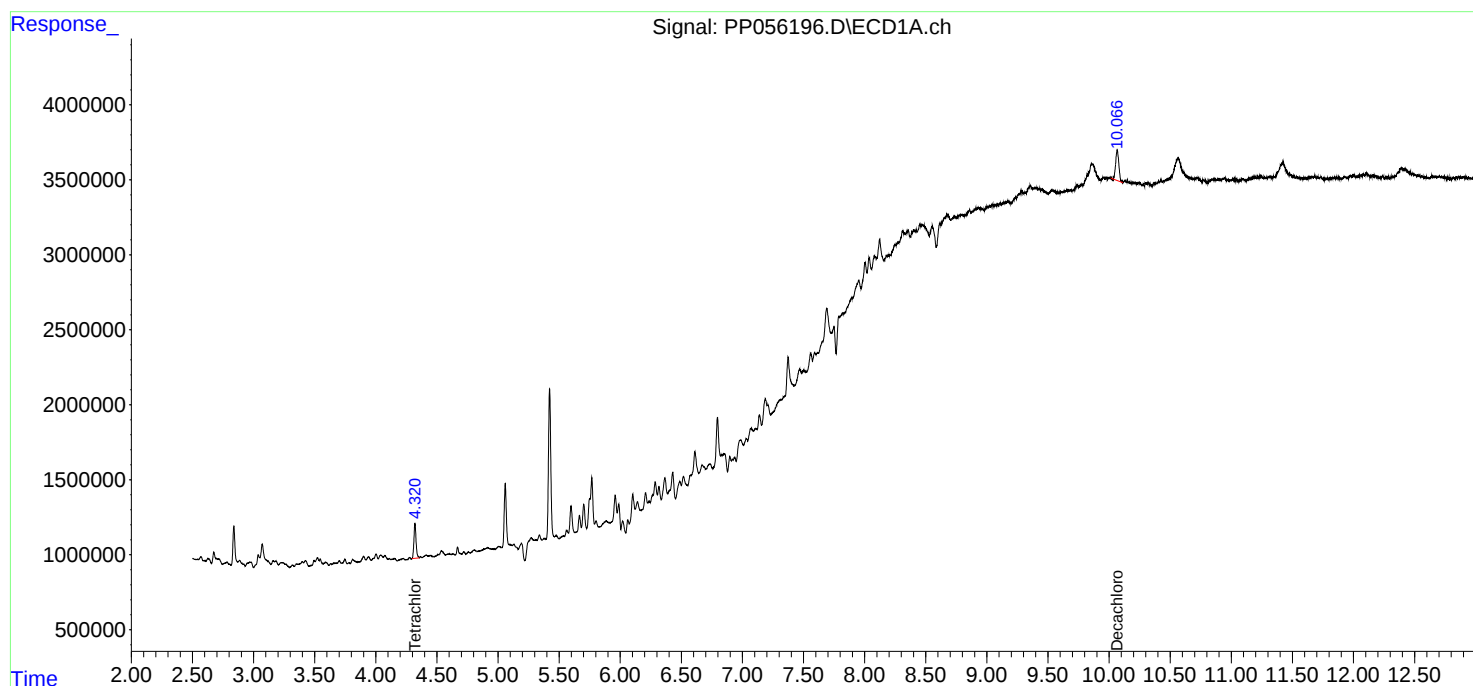

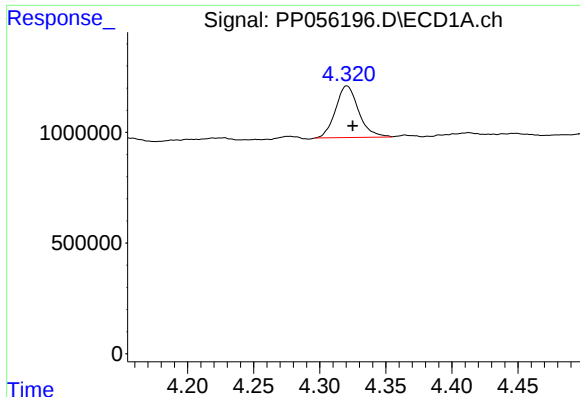


#1 Tetrachloro-m-xylene

R.T.: 4.320 min
Delta R.T.: -0.005 min
Response: 2839353
Conc: 1.76 ng/ml

Instrument :
ECD_P
ClientSampleId :
FMC-1222


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/06/2023
Supervised By :Ankita Jodhani 03/06/2023

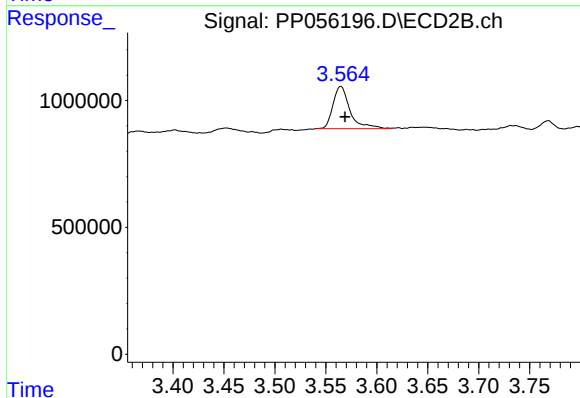


#1 Tetrachloro-m-xylene

R.T.: 3.565 min
Delta R.T.: -0.004 min
Response: 1932010
Conc: 1.32 ng/ml

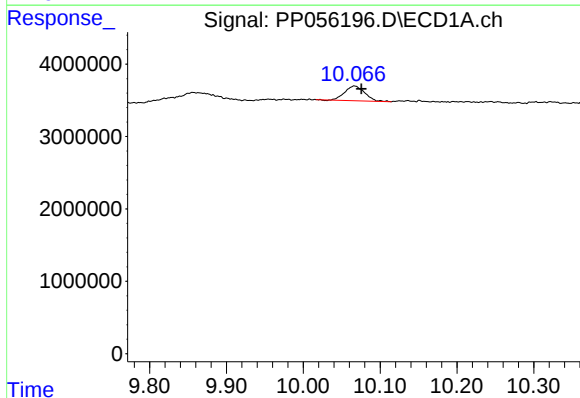

#2 Decachlorobiphenyl

R.T.: 10.066 min
Delta R.T.: -0.009 min
Response: 3642849
Conc: 1.79 ng/ml

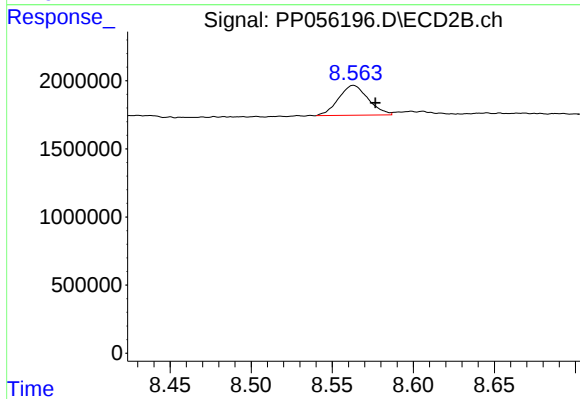

#2 Decachlorobiphenyl

R.T.: 8.563 min
Delta R.T.: -0.013 min
Response: 2797532
Conc: 2.47 ng/ml