

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030325\
 Data File : PP070198.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Mar 2025 19:47
 Operator : YP\AJ
 Sample : Q1476-02
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TRE-25-0016

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/04/2025
 Supervised By :Ankita Jodhani 03/04/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 04 03:15:16 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 25 05:10:19 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.523	3.828	22848288	22251084	15.568m	23.274 #
2) SA Decachlor...	10.248	8.880	21408548	19303015	18.795	17.805

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030325\
Data File : PP070198.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Mar 2025 19:47
Operator : YP\AJ
Sample : Q1476-02
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
TRE-25-0016


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/04/2025
Supervised By :Ankita Jodhani 03/04/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 04 03:15:16 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022425.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 25 05:10:19 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

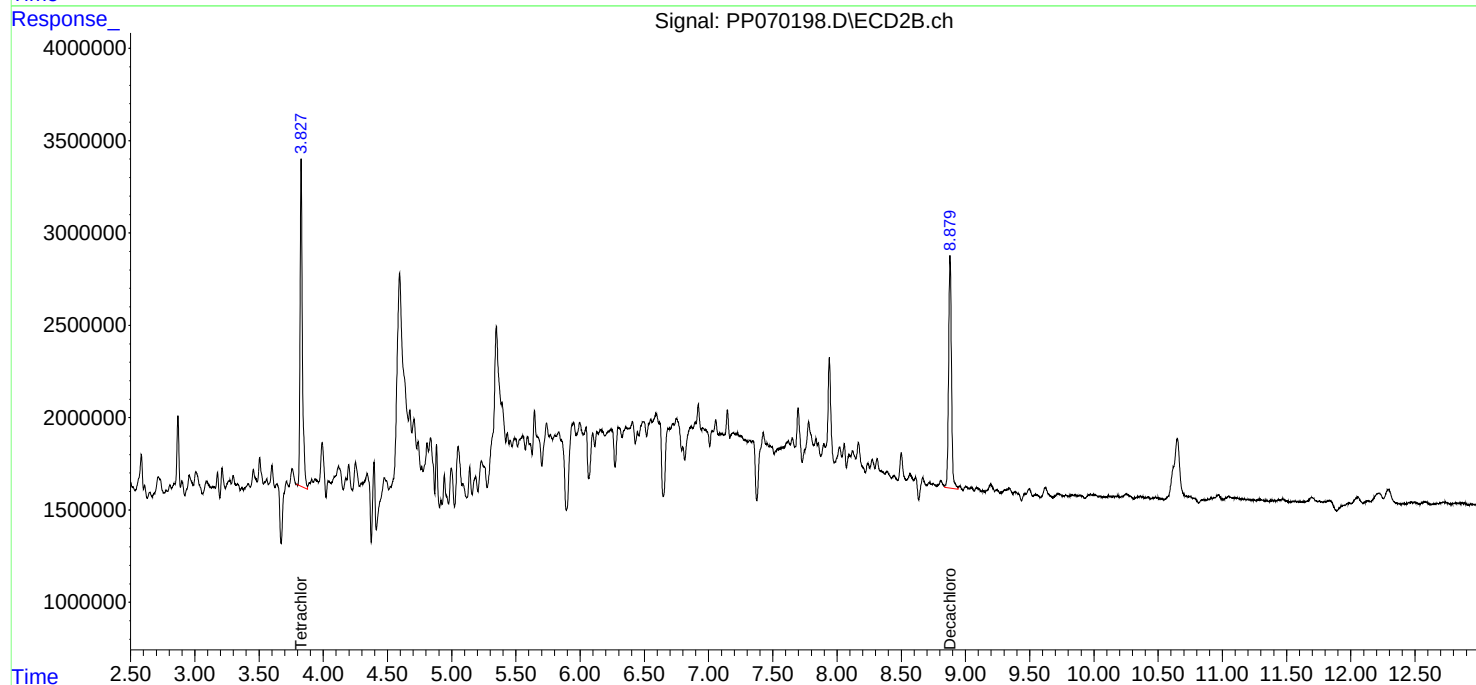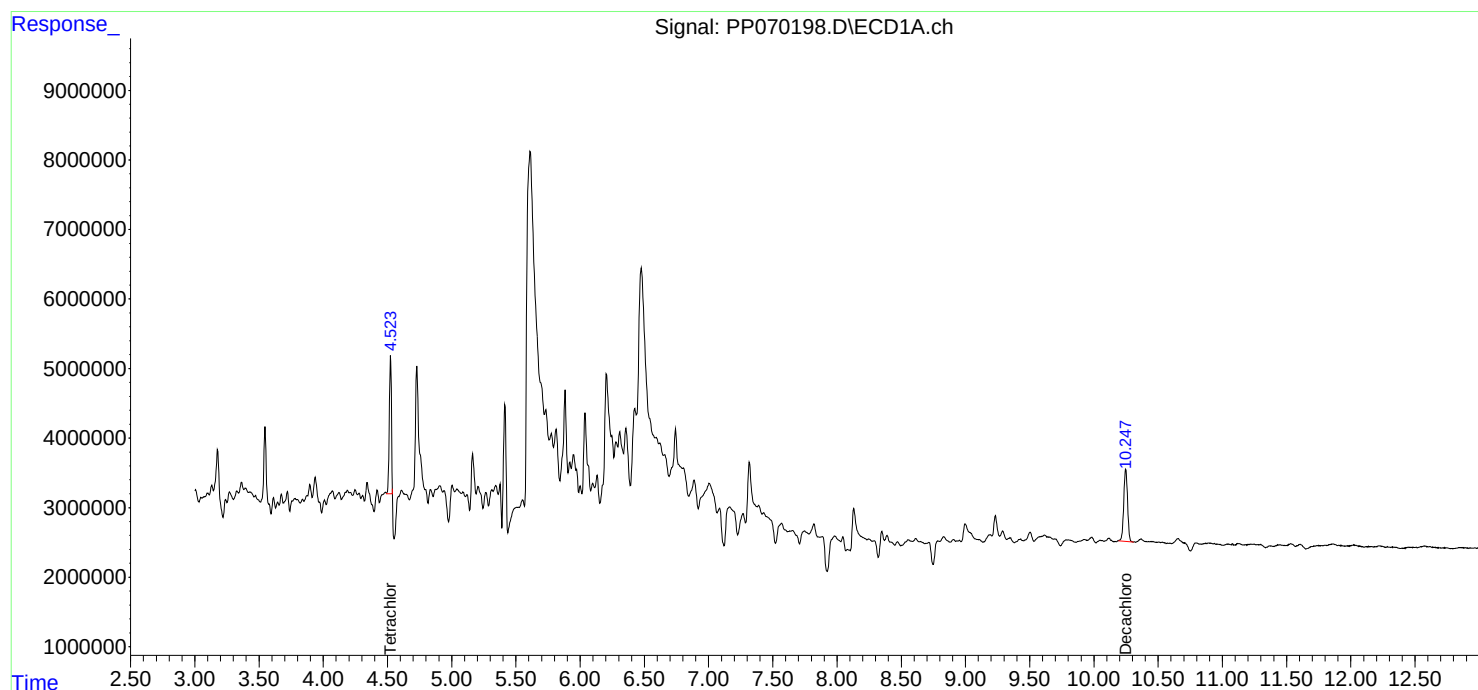

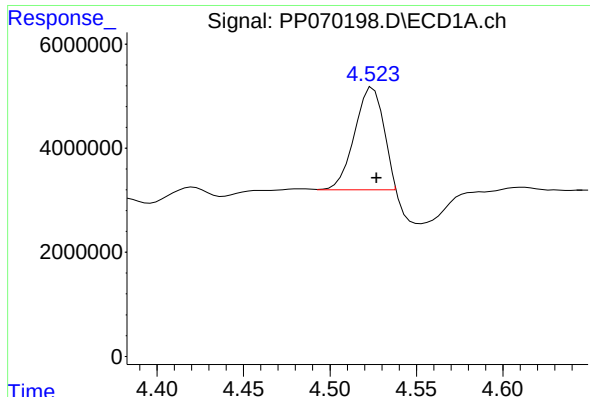


#1 Tetrachloro-m-xylene

R.T.: 4.523 min
Delta R.T.: -0.004 min
Response: 22848288
Conc: 15.57 ng/ml

Instrument :
ECD_P
ClientSampleId :
TRE-25-0016


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/04/2025
Supervised By :Ankita Jodhani 03/04/2025

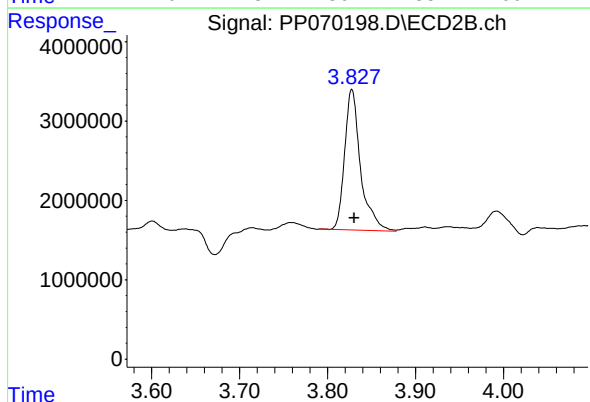


#1 Tetrachloro-m-xylene

R.T.: 3.828 min
Delta R.T.: -0.003 min
Response: 22251084
Conc: 23.27 ng/ml

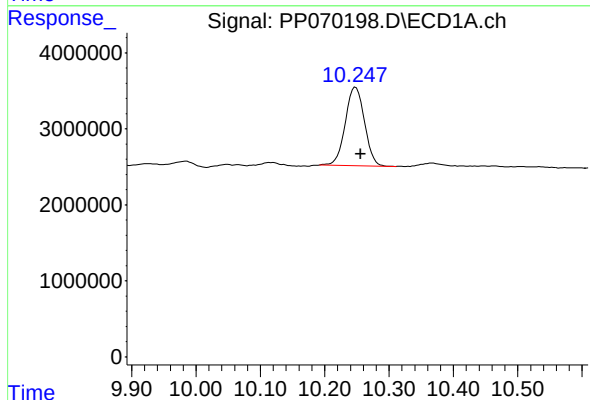

#2 Decachlorobiphenyl

R.T.: 10.248 min
Delta R.T.: -0.008 min
Response: 21408548
Conc: 18.80 ng/ml

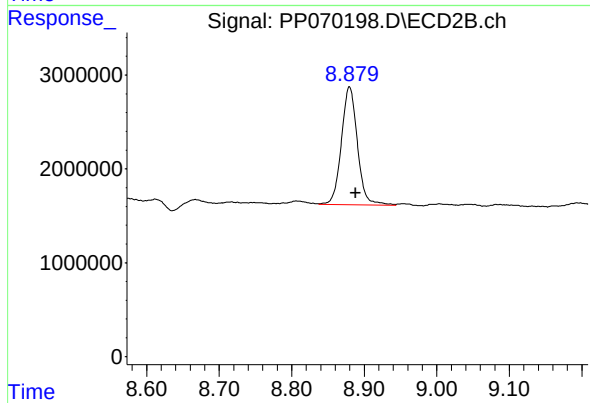

#2 Decachlorobiphenyl

R.T.: 8.880 min
Delta R.T.: -0.008 min
Response: 19303015
Conc: 17.81 ng/ml