

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030421\
 Data File : PP033643.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 04 Mar 2021 9:33
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 04:40:24 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 05 04:37:34 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.859	4.271	2442302	840716	21.261	21.116
2)	SA Decachlor...	10.792	9.618	2024533	506772	22.373	21.693
Target Compounds							
32)	L7 AR-1260-2	8.101f	0.000	16128	0	3.389	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030421\
Data File : PP033643.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 04 Mar 2021 9:33
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 04:40:24 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030421.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 05 04:37:34 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

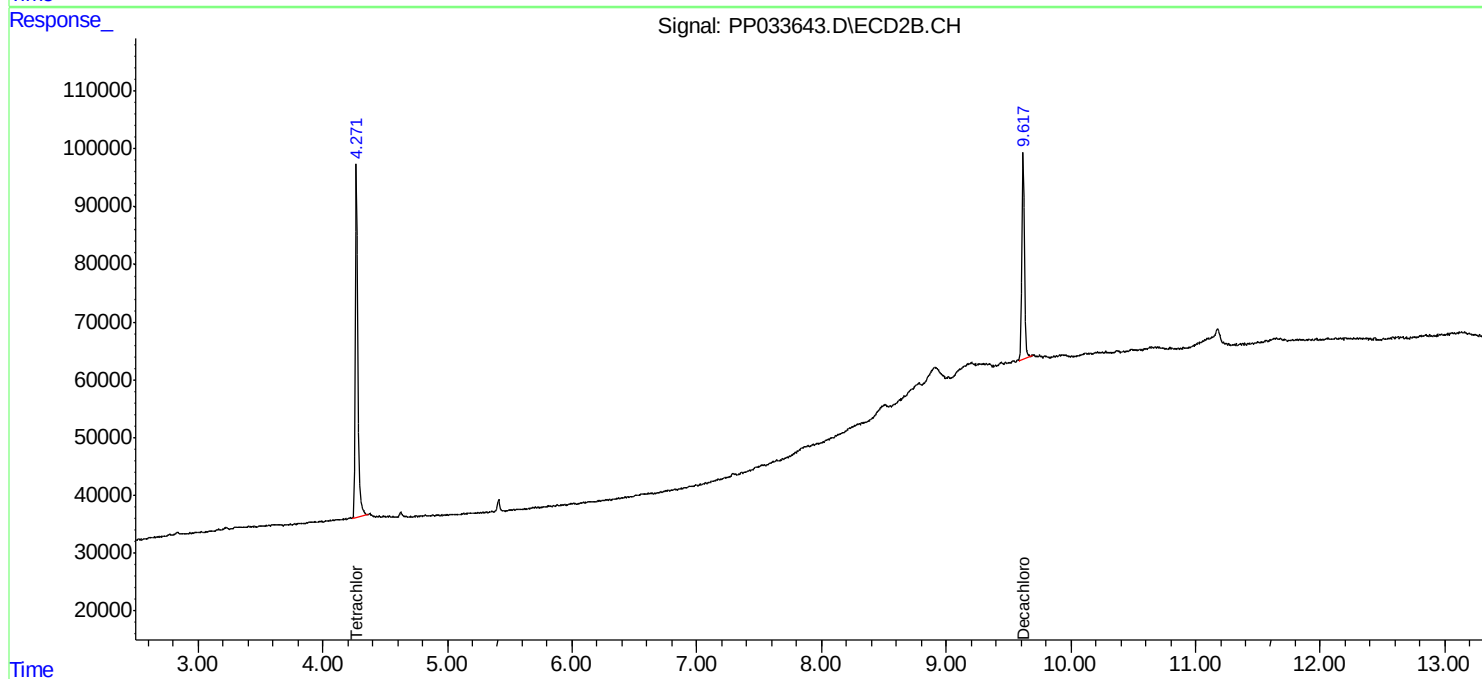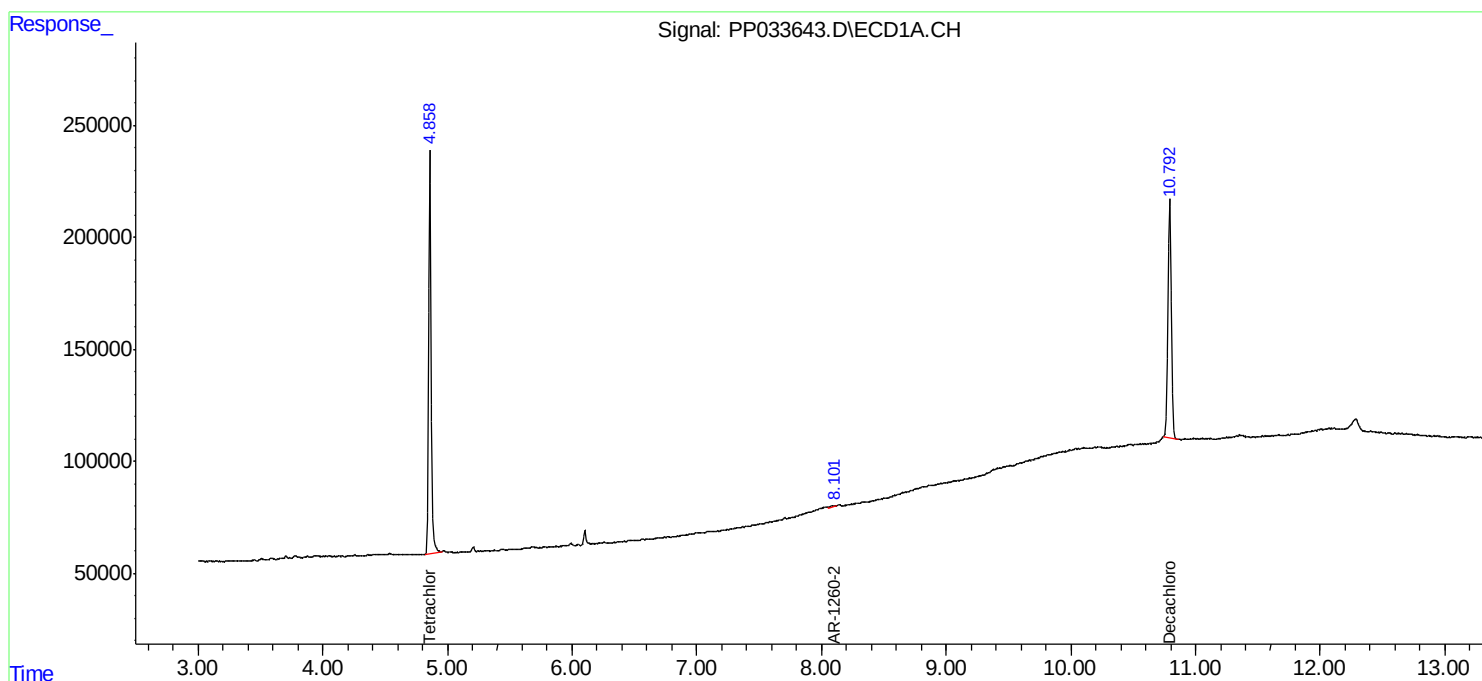


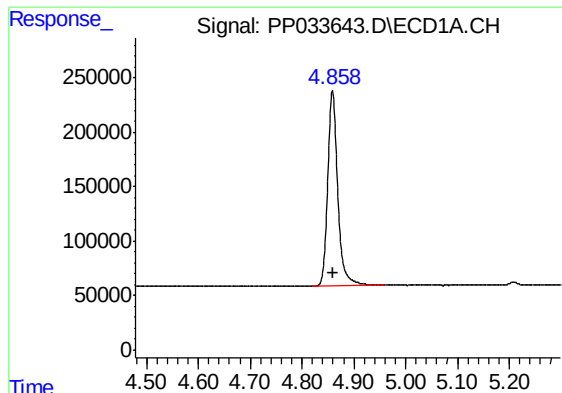

#1 Tetrachloro-m-xylene


R.T.: 4.859 min
Delta R.T.: 0.000 min
Response: 2442302
Conc: 21.26 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

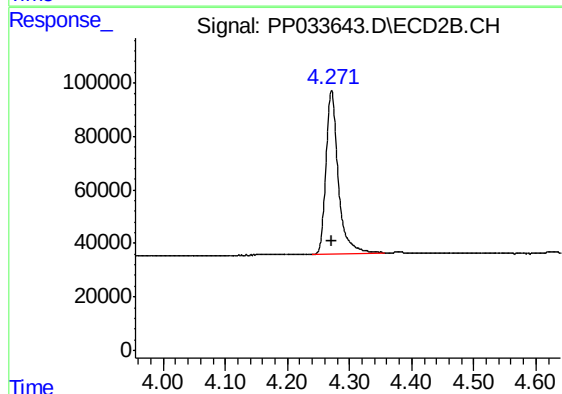


#1 Tetrachloro-m-xylene

R.T.: 4.271 min
Delta R.T.: 0.000 min
Response: 840716
Conc: 21.12 ng/ml

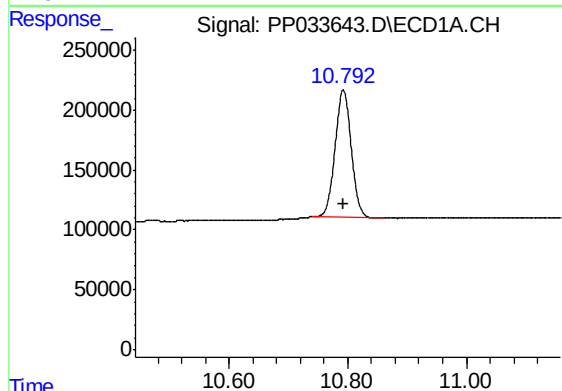


#2 Decachlorobiphenyl

R.T.: 10.792 min
Delta R.T.: 0.000 min
Response: 2024533
Conc: 22.37 ng/ml

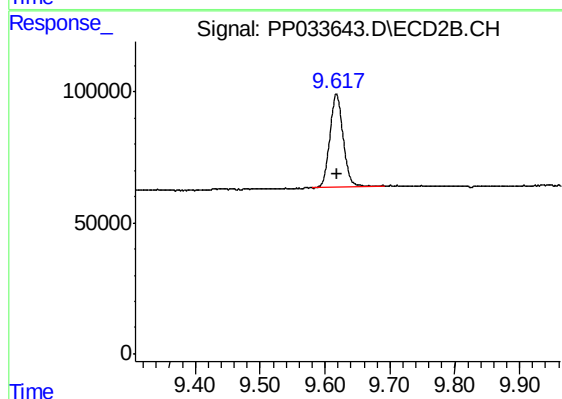

#2 Decachlorobiphenyl


R.T.: 9.618 min
Delta R.T.: 0.000 min
Response: 506772
Conc: 21.69 ng/ml

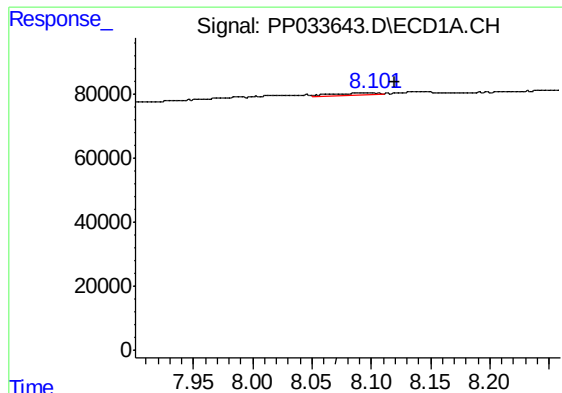

#32 AR-1260-2

R.T.: 8.101 min
Delta R.T.: -0.019 min
Response: 16128
Conc: 3.39 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

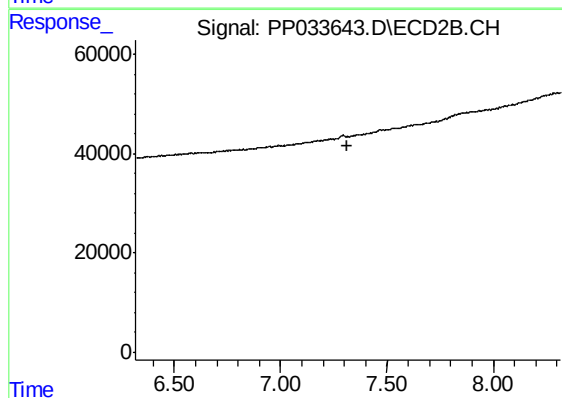

#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.316 min
Response: 0
Conc: N.D.