

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030422\
 Data File : PP044260.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Mar 2022 13:36
 Operator : YP\AJ
 Sample : N1792-02 10X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 KZ71910-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/07/2022
 Supervised By :Ankita Jodhani 03/07/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 00:56:06 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 03 02:21:53 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.911	3.165	3422667	3509519	1.652m	2.006m
2) SA Decachlor...	10.047	8.536	2545026	2837803	1.849m	1.850m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030422\
Data File : PP044260.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Mar 2022 13:36
Operator : YP\AJ
Sample : N1792-02 10X
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
KZ71910-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/07/2022
Supervised By :Ankita Jodhani 03/07/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 00:56:06 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 03 02:21:53 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

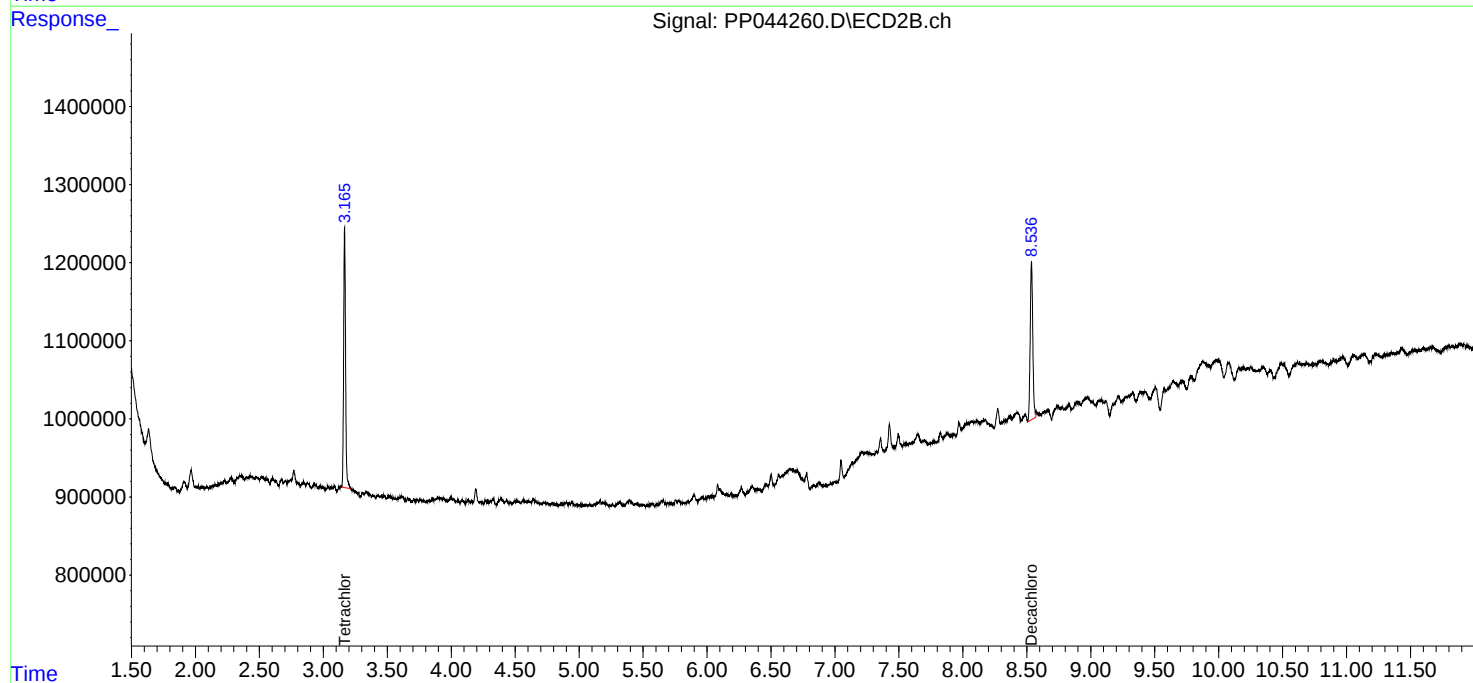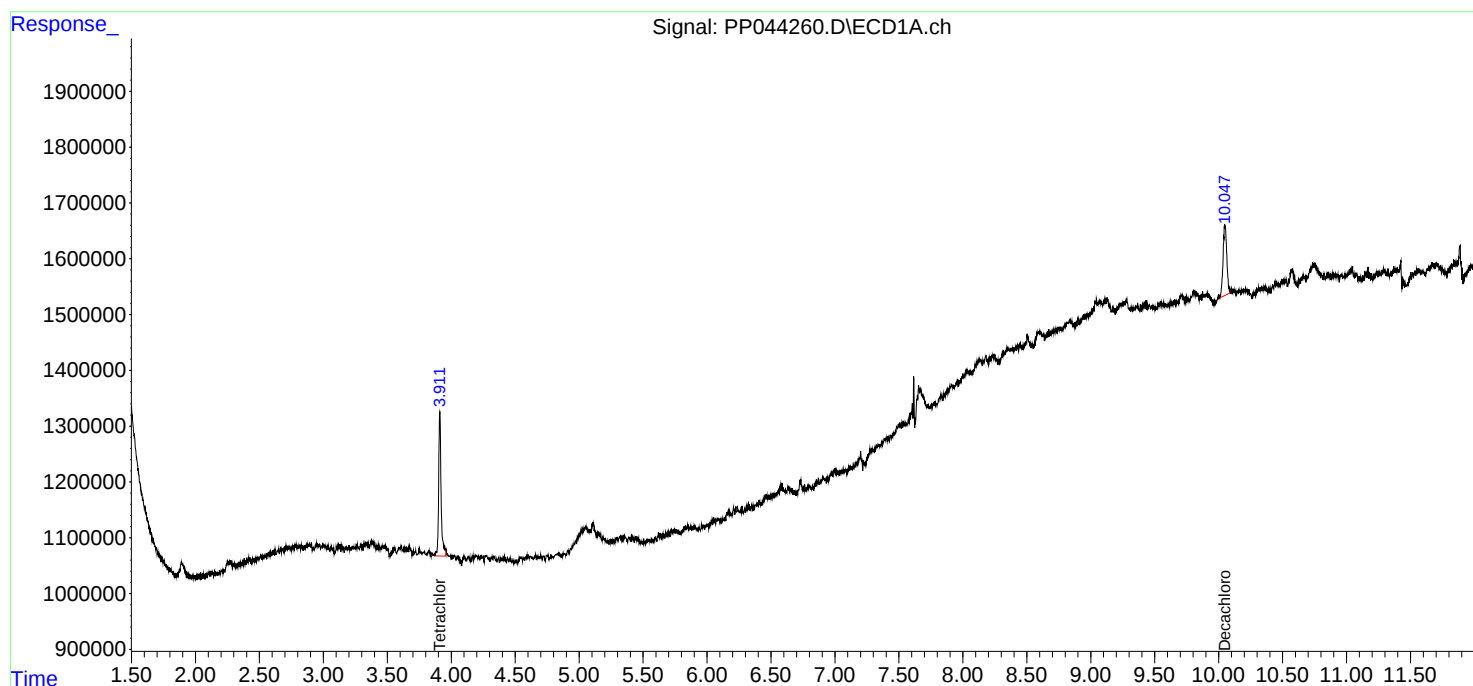

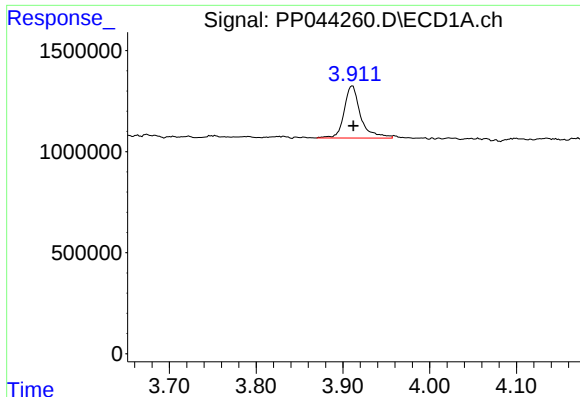


#1 Tetrachloro-m-xylene

R.T.: 3.911 min
Delta R.T.: -0.001 min
Response: 3422667
Conc: 1.65 ng/ml

Instrument :
ECD_P
ClientSampleId :
KZ71910-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/07/2022
Supervised By :Ankita Jodhani 03/07/2022

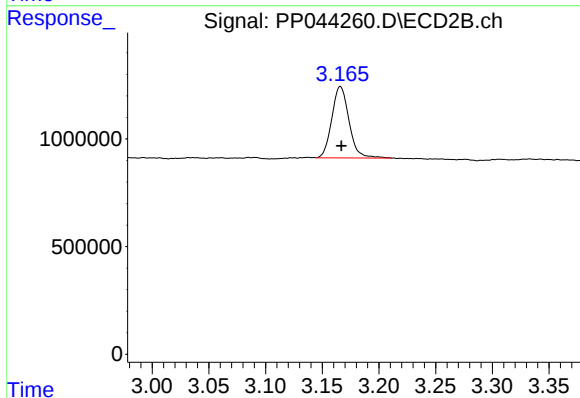


#1 Tetrachloro-m-xylene

R.T.: 3.165 min
Delta R.T.: -0.001 min
Response: 3509519
Conc: 2.01 ng/ml m

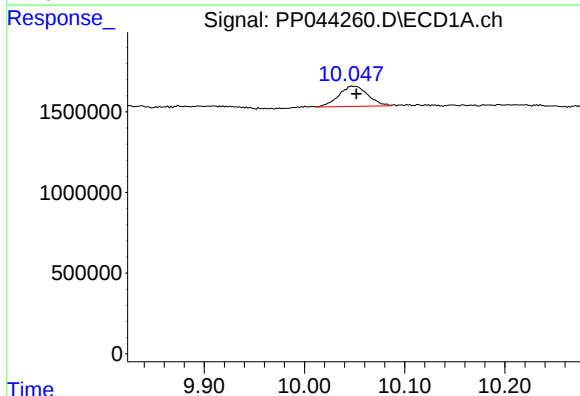

#2 Decachlorobiphenyl

R.T.: 10.047 min
Delta R.T.: -0.005 min
Response: 2545026
Conc: 1.85 ng/ml m

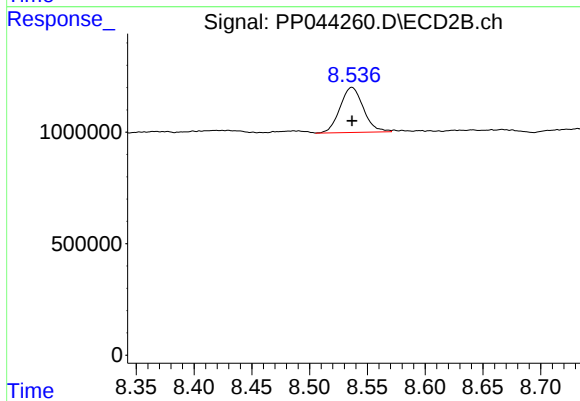

#2 Decachlorobiphenyl

R.T.: 8.536 min
Delta R.T.: 0.000 min
Response: 2837803
Conc: 1.85 ng/ml m