

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030425\
 Data File : PP070212.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Mar 2025 11:57
 Operator : YP\AJ
 Sample : Q1476-03RE 10X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TRE-25-0017RE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/05/2025
 Supervised By :Ankita Jodhani 03/05/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 04 12:11:59 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 25 05:10:19 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.526	3.828	2629364	3016680	1.792m	3.155m#
2) SA Decachlor...	10.254	8.882	3645359	2818594	3.200	2.600

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030425\
Data File : PP070212.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Mar 2025 11:57
Operator : YP\AJ
Sample : Q1476-03RE 10X
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
TRE-25-0017RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/05/2025
Supervised By :Ankita Jodhani 03/05/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 04 12:11:59 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022425.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 25 05:10:19 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

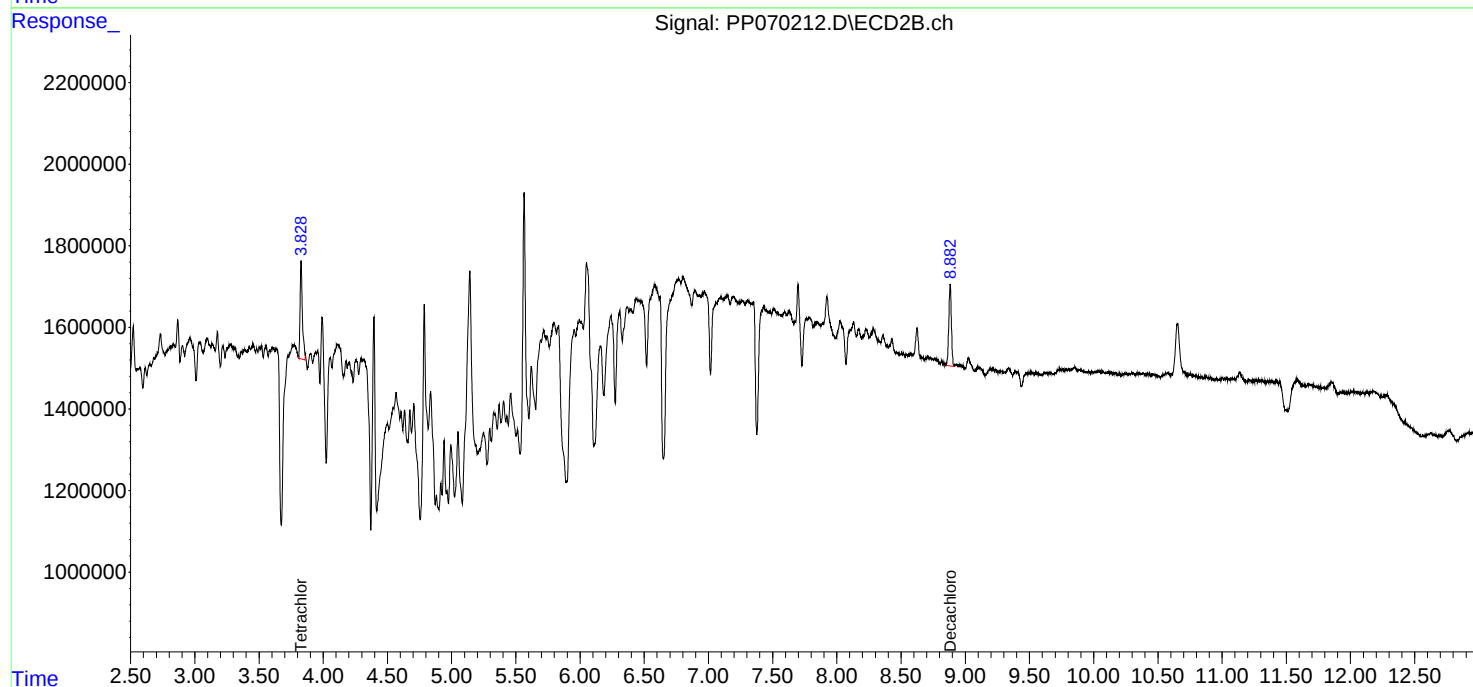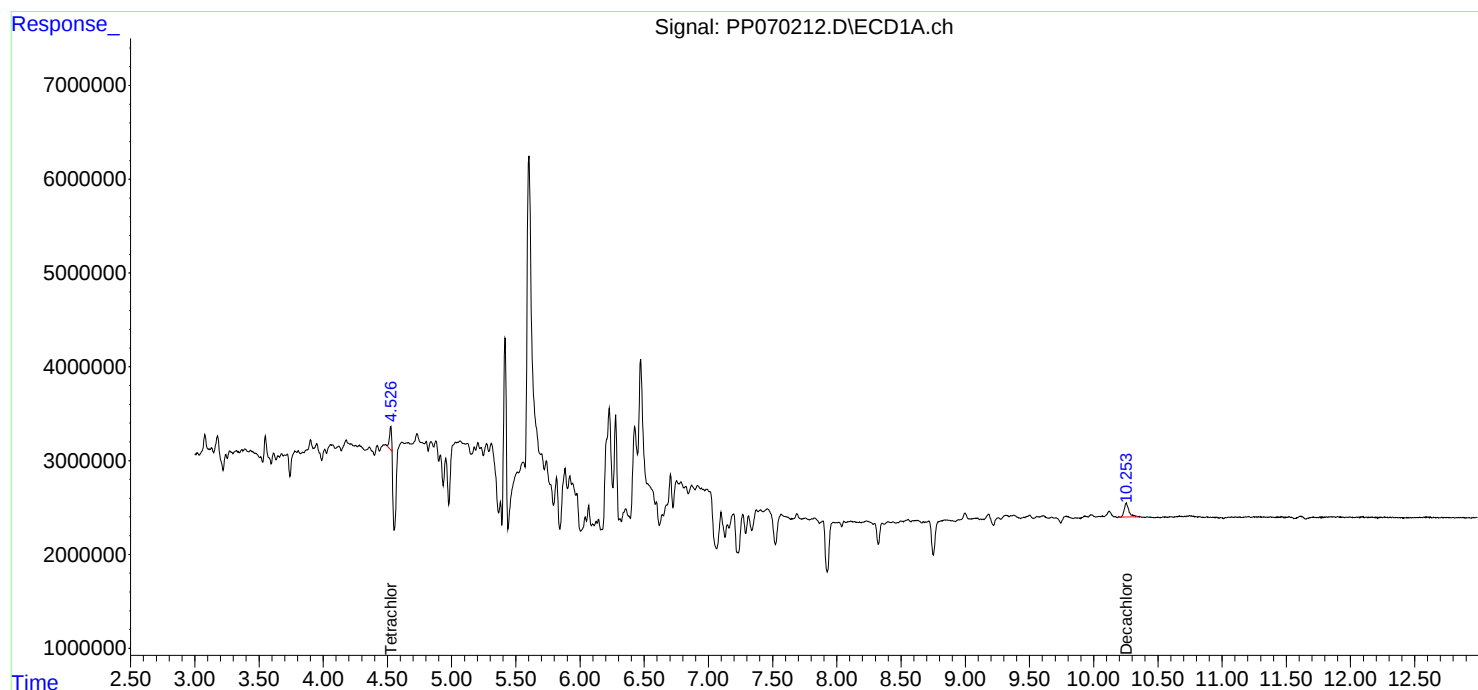

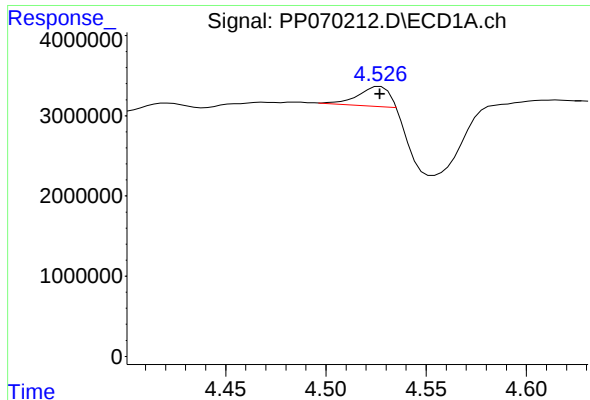


#1 Tetrachloro-m-xylene

R.T.: 4.526 min
Delta R.T.: -0.001 min
Response: 2629364
Conc: 1.79 ng/ml

Instrument :
ECD_P
ClientSampleId :
TRE-25-0017RE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/05/2025
Supervised By :Ankita Jodhani 03/05/2025

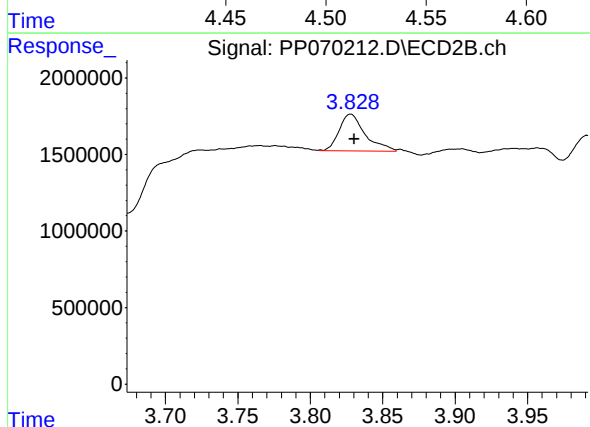


#1 Tetrachloro-m-xylene

R.T.: 3.828 min
Delta R.T.: -0.003 min
Response: 3016680
Conc: 3.16 ng/ml m

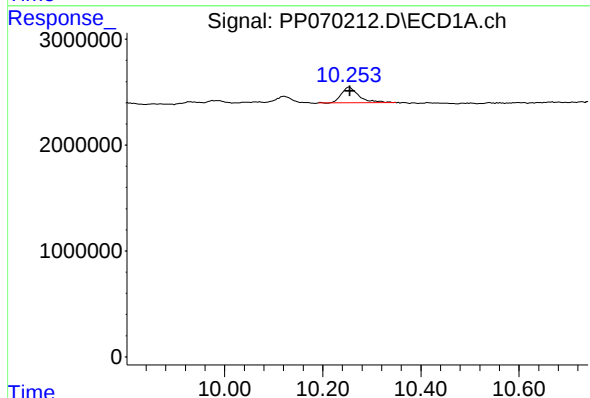

#2 Decachlorobiphenyl

R.T.: 10.254 min
Delta R.T.: -0.002 min
Response: 3645359
Conc: 3.20 ng/ml

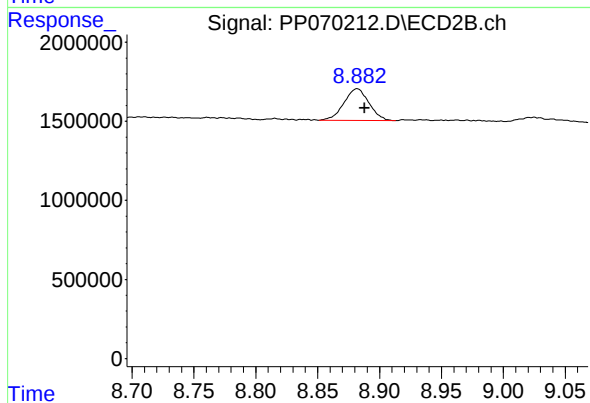

#2 Decachlorobiphenyl

R.T.: 8.882 min
Delta R.T.: -0.006 min
Response: 2818594
Conc: 2.60 ng/ml