

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030425\
 Data File : PP070220.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Mar 2025 16:29
 Operator : YP\AJ
 Sample : Q1480-17
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TP-3

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/05/2025
 Supervised By :Ankita Jodhani 03/05/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 00:43:21 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 25 05:10:19 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.523	3.829	27728071	20886092	18.893m	21.847
2) SA Decachlor...	10.250	8.882	17485399	16125915	15.351	14.875

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030425\
Data File : PP070220.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Mar 2025 16:29
Operator : YP\AJ
Sample : Q1480-17
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleID :
TP-3


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/05/2025
Supervised By :Ankita Jodhani 03/05/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 00:43:21 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022425.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 25 05:10:19 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

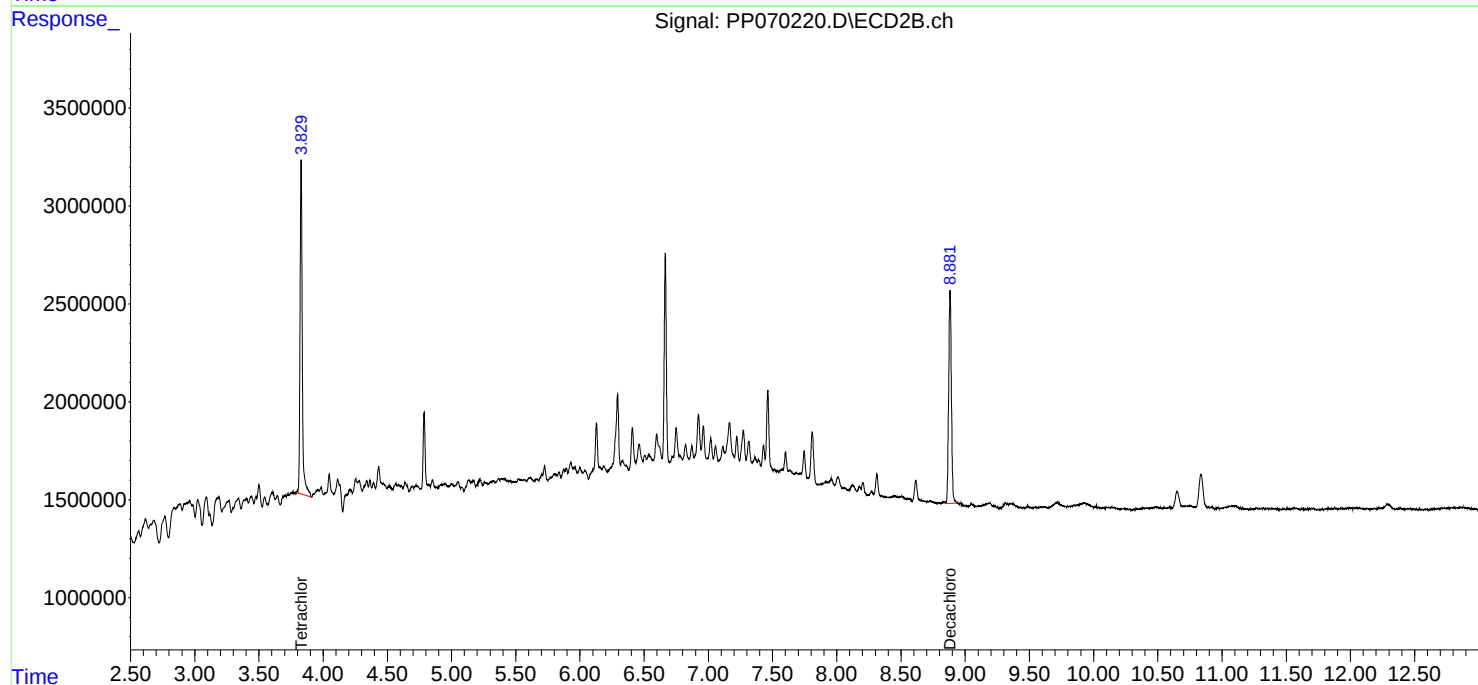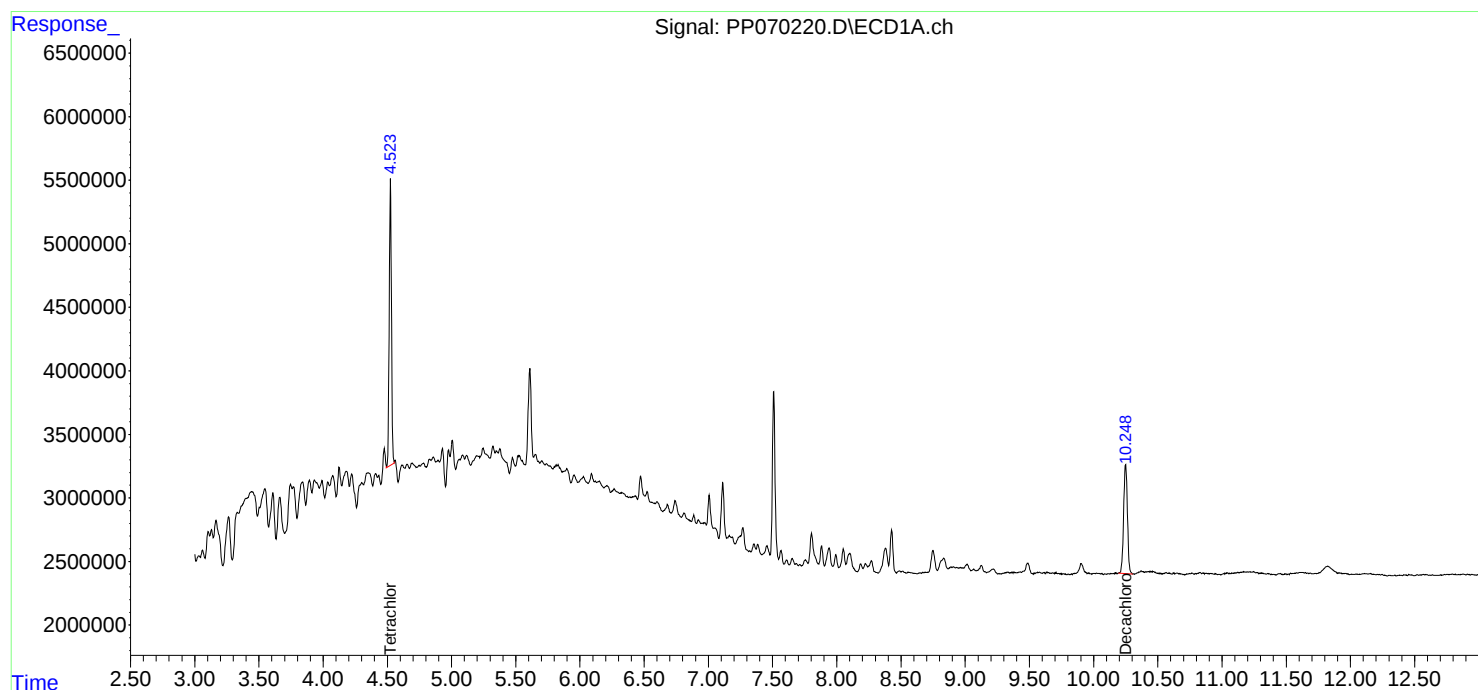

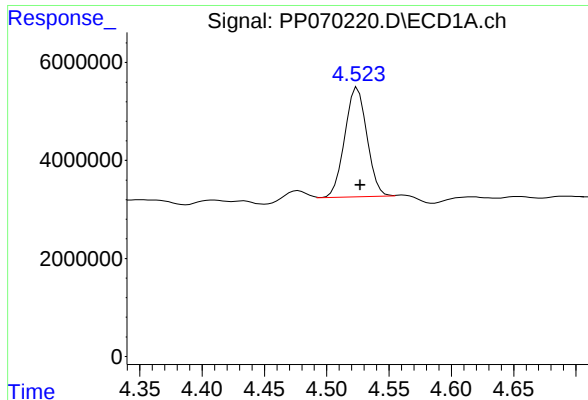


#1 Tetrachloro-m-xylene

R.T.: 4.523 min
Delta R.T.: -0.004 min
Response: 27728071
Conc: 18.89 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-3


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/05/2025
Supervised By :Ankita Jodhani 03/05/2025

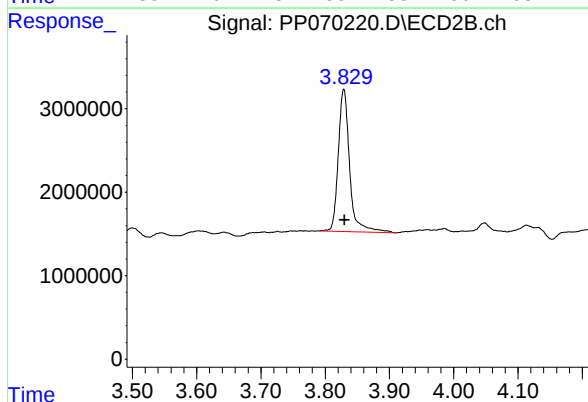


#1 Tetrachloro-m-xylene

R.T.: 3.829 min
Delta R.T.: -0.001 min
Response: 20886092
Conc: 21.85 ng/ml

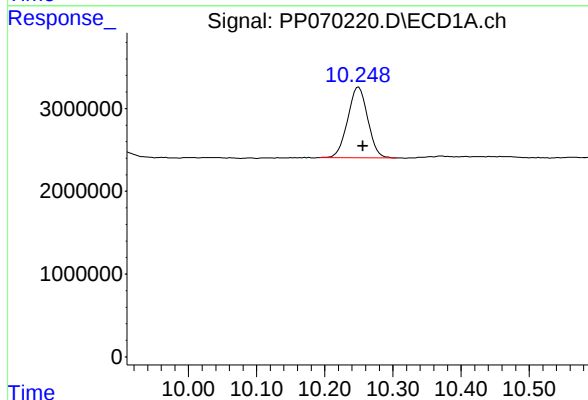

#2 Decachlorobiphenyl

R.T.: 10.250 min
Delta R.T.: -0.006 min
Response: 17485399
Conc: 15.35 ng/ml

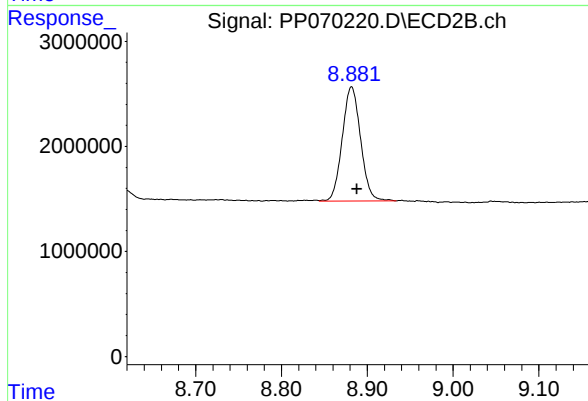

#2 Decachlorobiphenyl

R.T.: 8.882 min
Delta R.T.: -0.006 min
Response: 16125915
Conc: 14.87 ng/ml