

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030425\
 Data File : PP070236.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Mar 2025 21:21
 Operator : YP\AJ
 Sample : Q1480-33
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TP-3-WATER-SAMPLE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 00:47:53 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 25 05:10:19 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.525	3.828	32520690	21152137	22.159	22.125
2) SA Decachlor...	10.249	8.880	17273347	17164930	15.165	15.833

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030425\
Data File : PP070236.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Mar 2025 21:21
Operator : YP\AJ
Sample : Q1480-33
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
TP-3-WATER-SAMPLE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 00:47:53 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022425.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 25 05:10:19 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

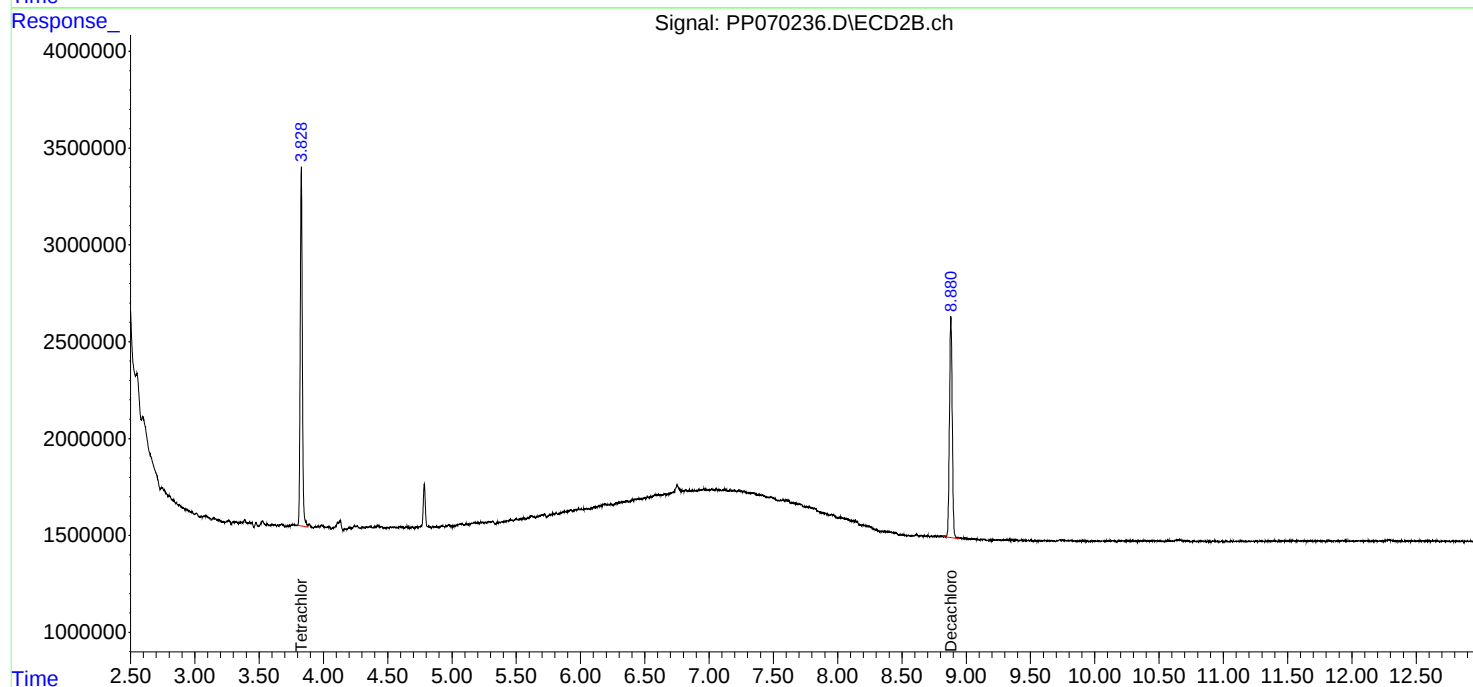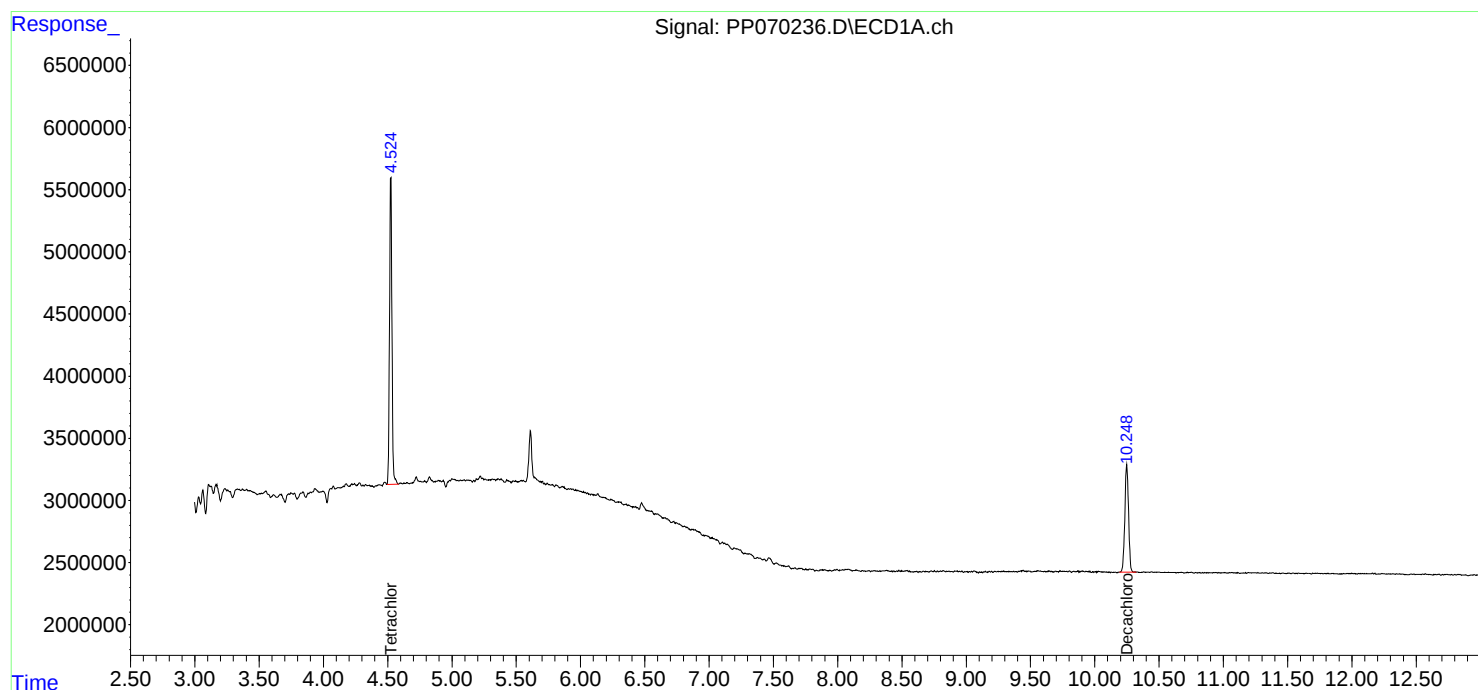


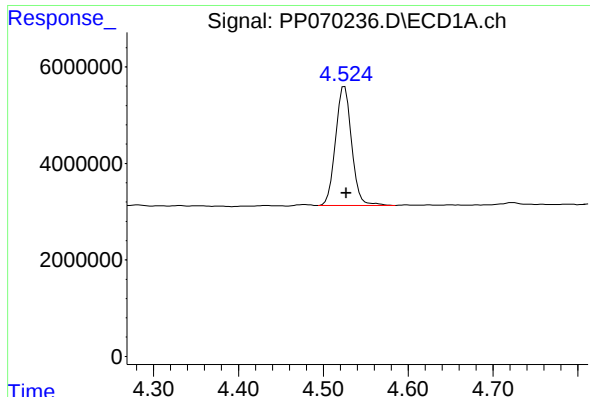

#1 Tetrachloro-m-xylene


R.T.: 4.525 min
Delta R.T.: -0.002 min
Response: 32520690
Conc: 22.16 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-3-WATER-SAMPLE

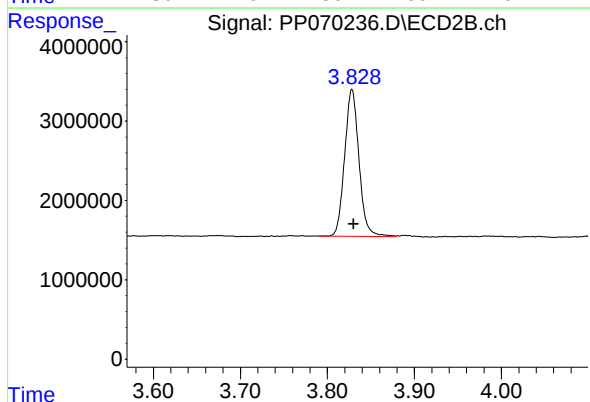


#1 Tetrachloro-m-xylene

R.T.: 3.828 min
Delta R.T.: -0.002 min
Response: 21152137
Conc: 22.12 ng/ml

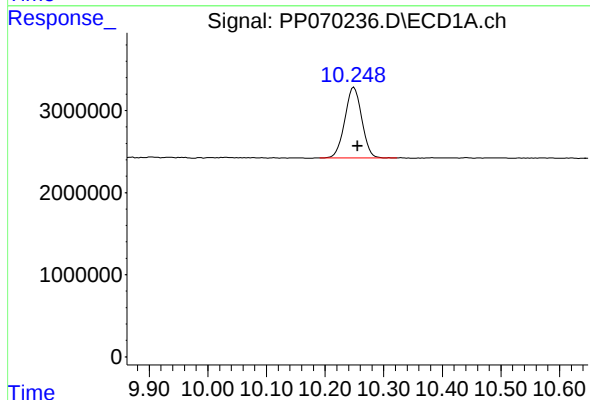

#2 Decachlorobiphenyl

R.T.: 10.249 min
Delta R.T.: -0.007 min
Response: 17273347
Conc: 15.16 ng/ml

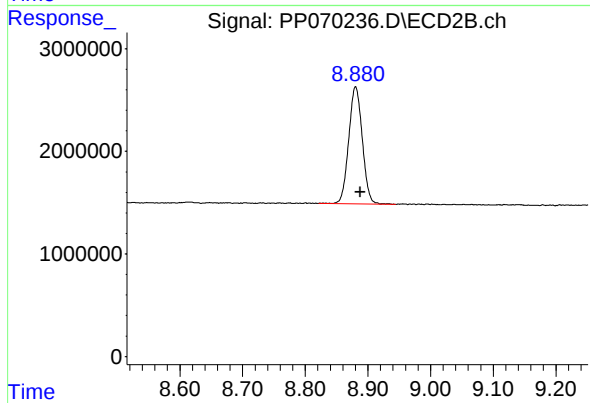

#2 Decachlorobiphenyl

R.T.: 8.880 min
Delta R.T.: -0.008 min
Response: 17164930
Conc: 15.83 ng/ml