

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030521\
 Data File : PP033705.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Mar 2021 15:34
 Operator : DD\AJ
 Sample : M1566-03
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 VEOLIA-72-11977

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 15:48:33 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 05 04:37:34 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.860	4.274	2282050	890521	19.866	22.367
2)	SA Decachlor...	10.793	9.614	1586122	377526	17.528	16.160
Target Compounds							
24)	L5 AR-1248-4	7.111	0.000	67431	0	20.727	N.D. #
26)	L6 AR-1254-1	7.056f	0.000	65623	0	18.863	N.D. #
27)	L6 AR-1254-2	7.313	0.000	43182	0	8.204	N.D. #
28)	L6 AR-1254-3	7.698	0.000	148681	0	26.640	N.D. #
29)	L6 AR-1254-4	7.986	0.000	97354	0	25.375	N.D. #
30)	L6 AR-1254-5	8.436f	7.651	405188	161982	96.650	94.542
31)	L7 AR-1260-1	7.855	0.000	192278	0	46.490	N.D. #
32)	L7 AR-1260-2	8.115	0.000	271766	0	57.104	N.D. #
34)	L7 AR-1260-4	8.688f	0.000	135074	0	30.531	N.D. #
35)	L7 AR-1260-5	9.033	8.196	60554	37482	7.131	14.271 #
36)	L8 AR-1262-1	0.000	7.651	0	161982	N.D.	176.947 #
37)	L8 AR-1262-2	9.033	8.196	60554	37482	6.556	12.691 #
39)	L8 AR-1262-4	9.415	0.000	41418	0	7.493	N.D. #
42)	L9 AR-1268-2	9.415	0.000	41418	0	3.572	N.D. #
45)	L9 AR-1268-5	10.469	0.000	83354	0	2.572	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030521\
Data File : PP033705.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Mar 2021 15:34
Operator : DD\AJ
Sample : M1566-03
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
VEOLIA-72-11977

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 15:48:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030421.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 05 04:37:34 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

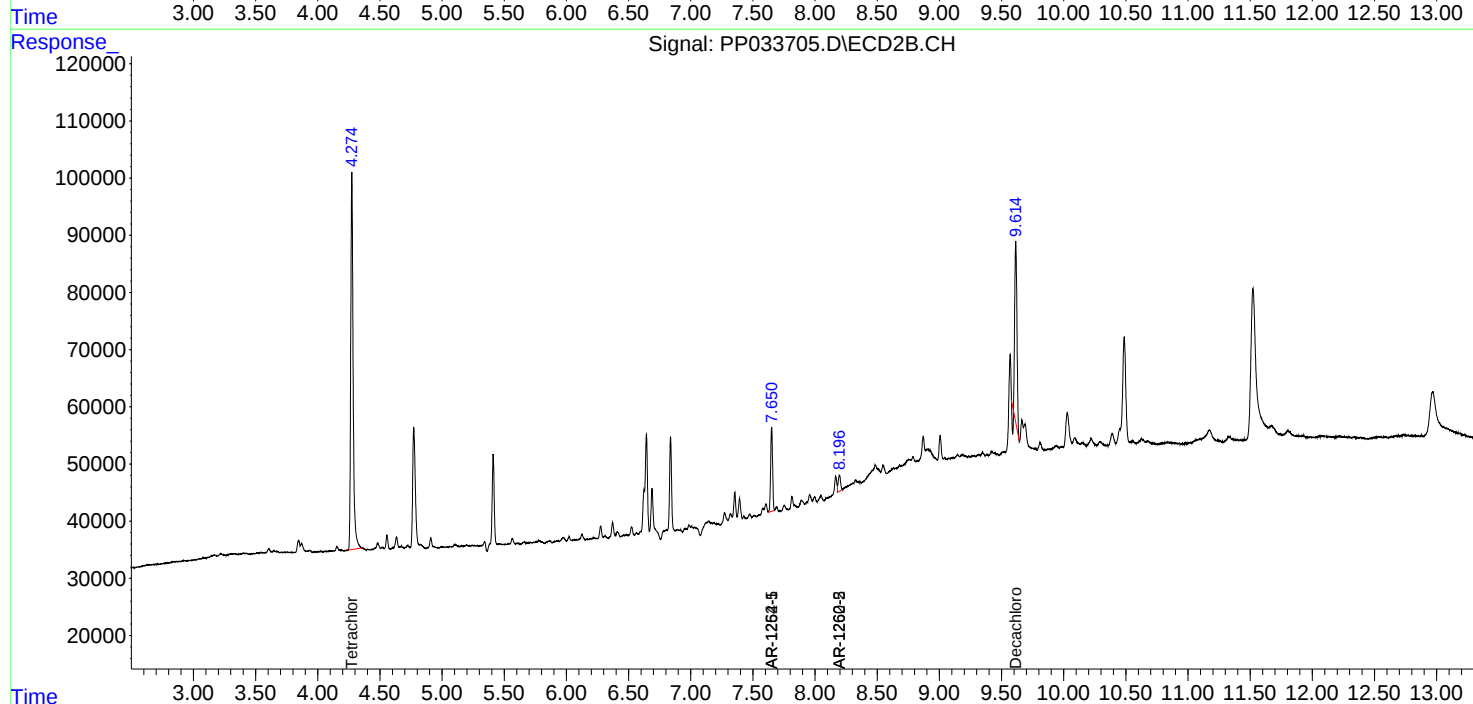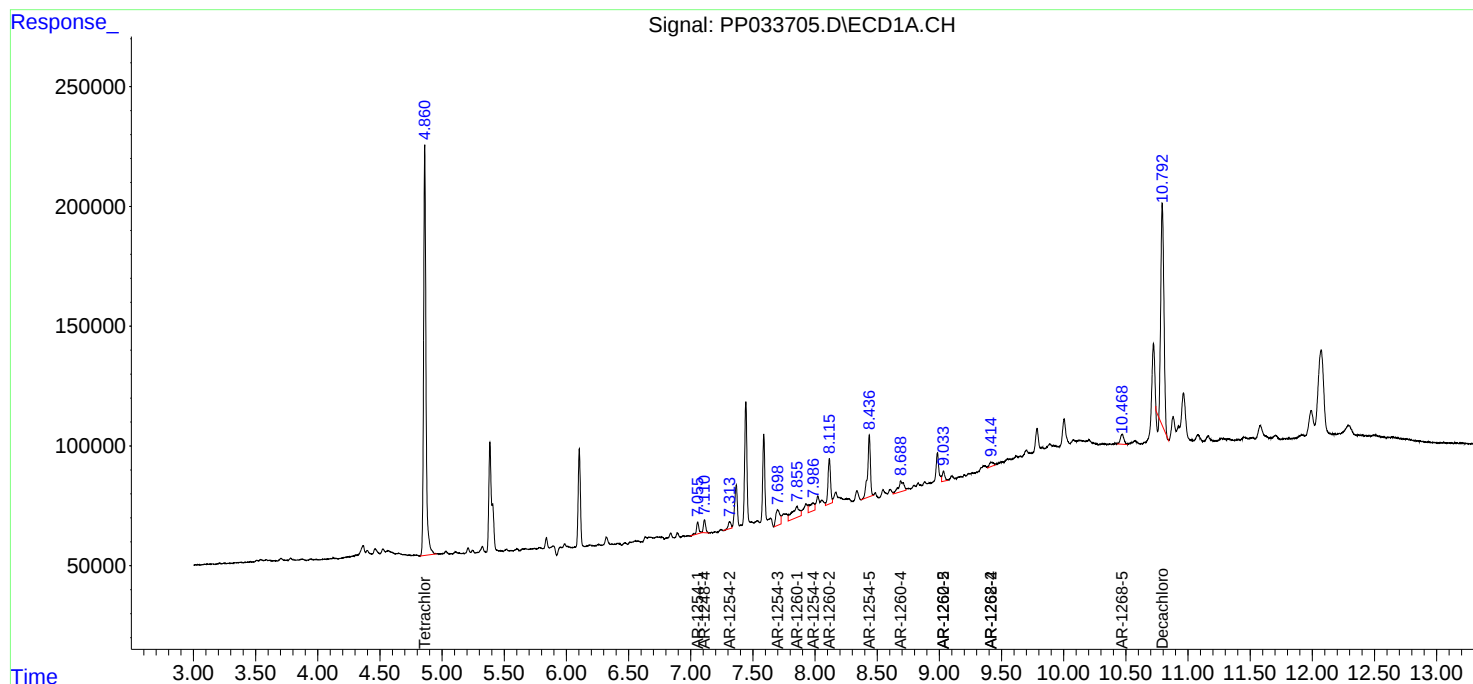


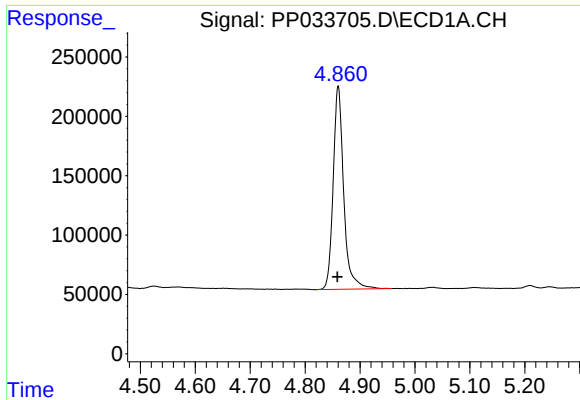

#1 Tetrachloro-m-xylene


R.T.: 4.860 min
Delta R.T.: 0.001 min
Response: 2282050
Conc: 19.87 ng/ml

Instrument :
ECD_P
ClientSampleId :
VEOLIA-72-11977

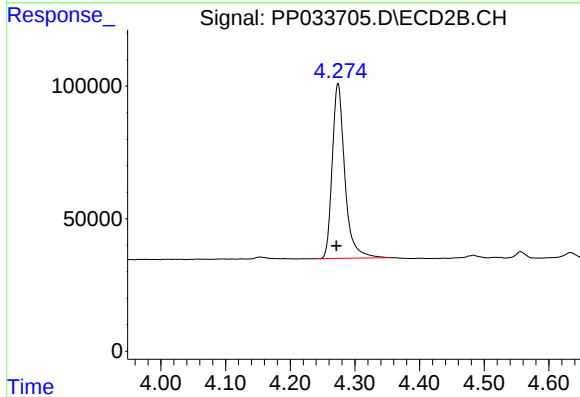


#1 Tetrachloro-m-xylene

R.T.: 4.274 min
Delta R.T.: 0.002 min
Response: 890521
Conc: 22.37 ng/ml

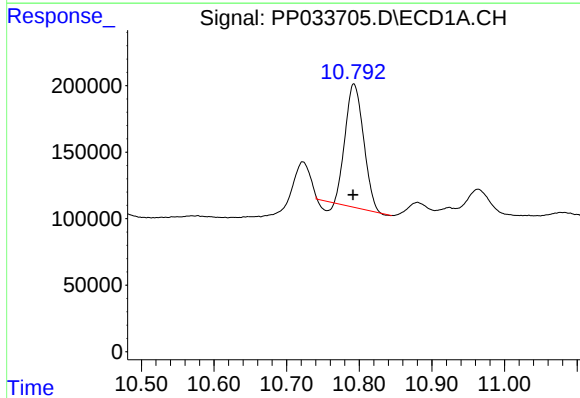


#2 Decachlorobiphenyl

R.T.: 10.793 min
Delta R.T.: 0.000 min
Response: 1586122
Conc: 17.53 ng/ml

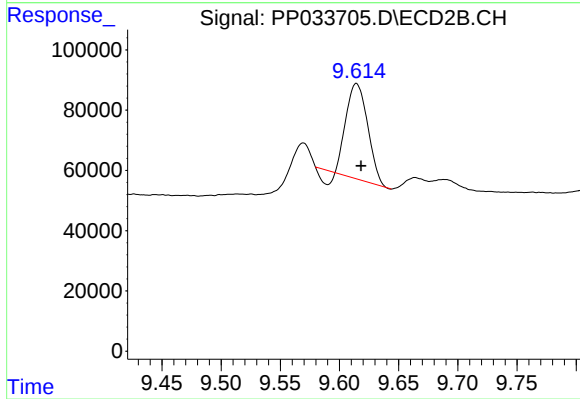

#2 Decachlorobiphenyl


R.T.: 9.614 min
Delta R.T.: -0.004 min
Response: 377526
Conc: 16.16 ng/ml

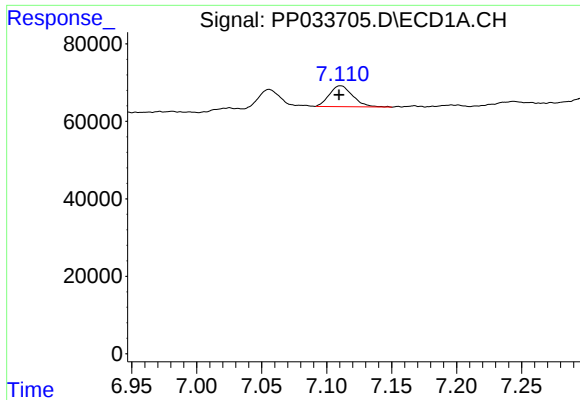

#24 AR-1248-4


R.T.: 7.111 min
Delta R.T.: 0.001 min
Response: 67431
Conc: 20.73 ng/ml

Instrument :
ECD_P
ClientSampleId :
VEOLIA-72-11977

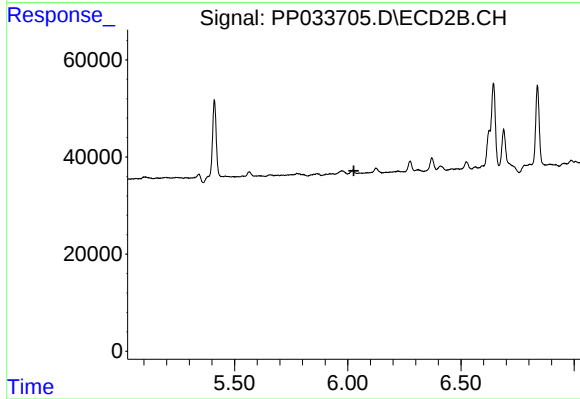


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 6.027 min
Response: 0
Conc: N.D.

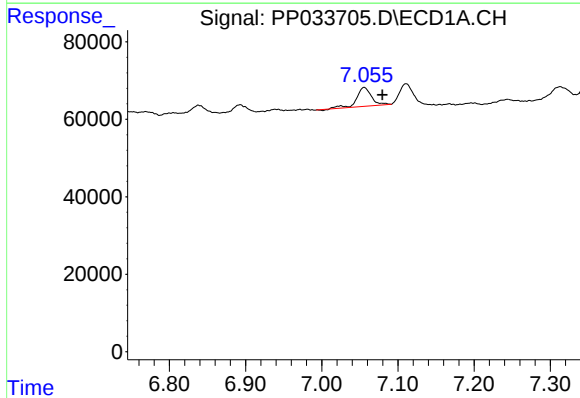


#26 AR-1254-1

R.T.: 7.056 min
Delta R.T.: -0.024 min
Response: 65623
Conc: 18.86 ng/ml

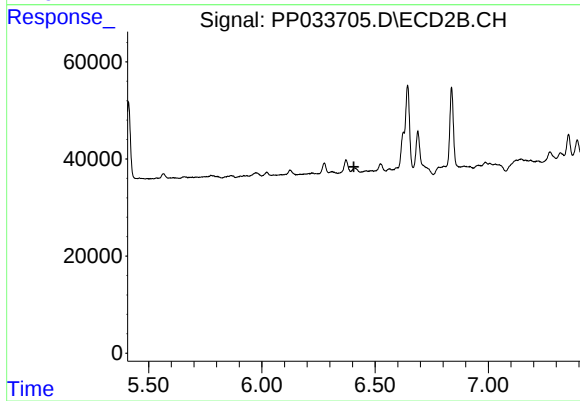

#26 AR-1254-1


R.T.: 0.000 min
Exp R.T. : 6.406 min
Response: 0
Conc: N.D.

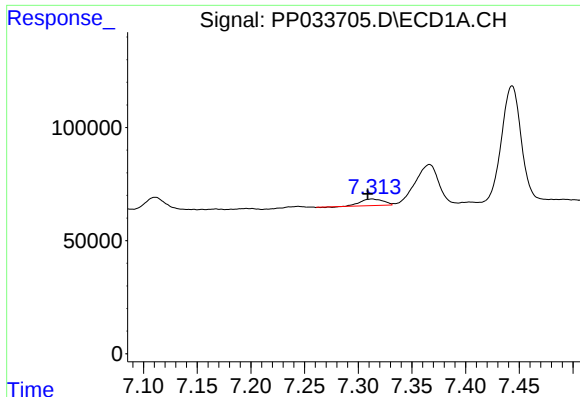

#27 AR-1254-2


R.T.: 7.313 min
Delta R.T.: 0.004 min
Response: 43182
Conc: 8.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
VEOLIA-72-11977

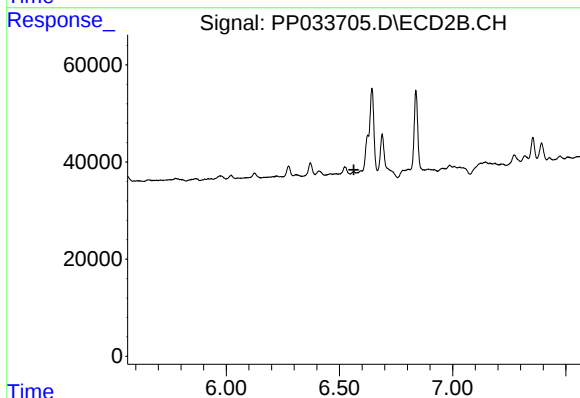


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T. : 6.564 min
Response: 0
Conc: N.D.

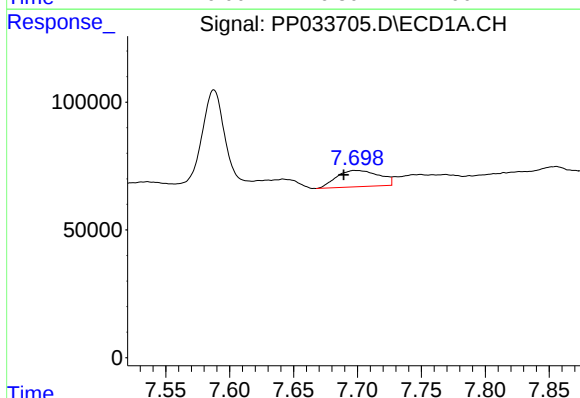


#28 AR-1254-3

R.T.: 7.698 min
Delta R.T.: 0.009 min
Response: 148681
Conc: 26.64 ng/ml

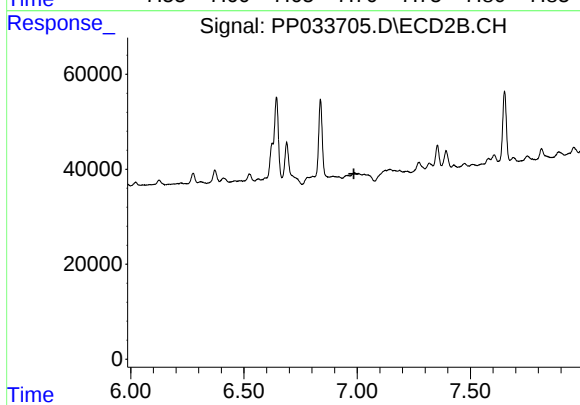

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.986 min
Response: 0
Conc: N.D.

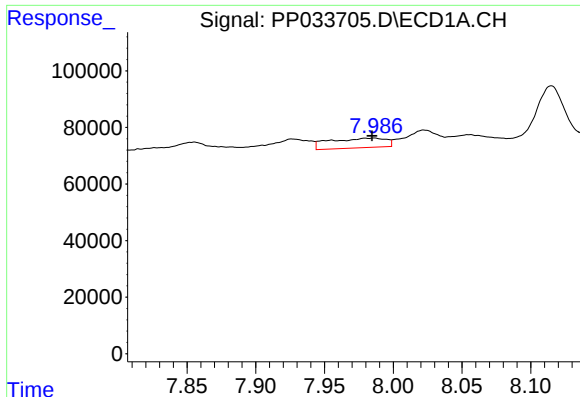

#29 AR-1254-4


R.T.: 7.986 min
Delta R.T.: 0.002 min
Response: 97354
Conc: 25.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
VEOLIA-72-11977

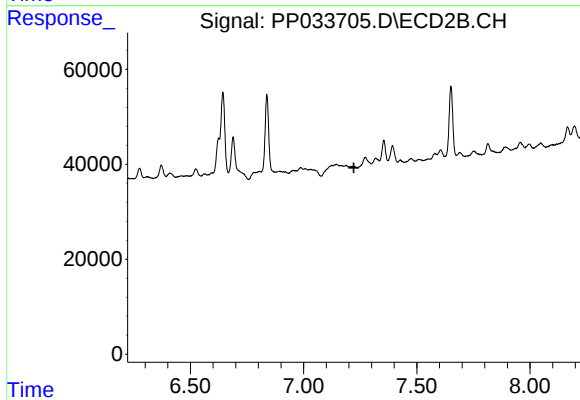


#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 7.222 min
Response: 0
Conc: N.D.

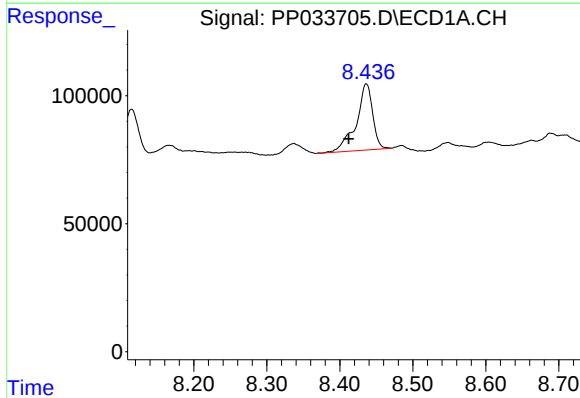


#30 AR-1254-5

R.T.: 8.436 min
Delta R.T.: 0.024 min
Response: 405188
Conc: 96.65 ng/ml

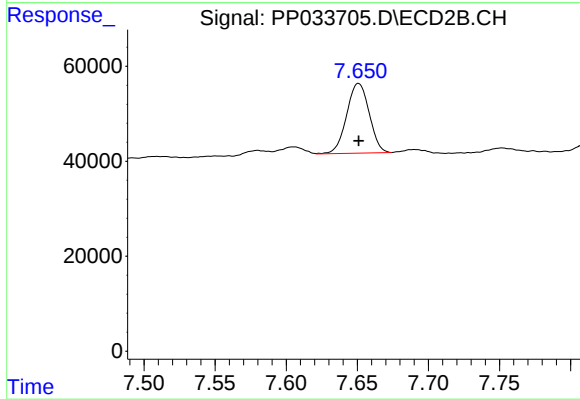

#30 AR-1254-5


R.T.: 7.651 min
Delta R.T.: 0.000 min
Response: 161982
Conc: 94.54 ng/ml

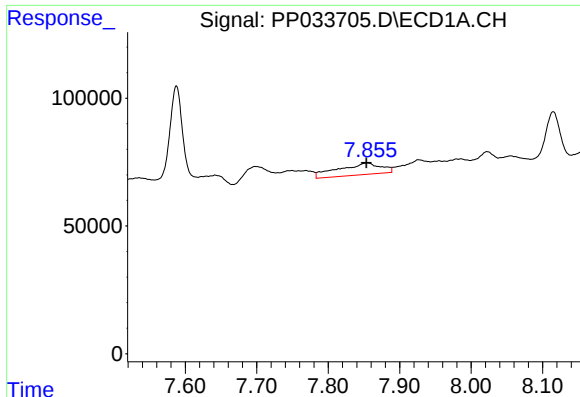

#31 AR-1260-1


R.T.: 7.855 min
Delta R.T.: 0.002 min
Response: 192278
Conc: 46.49 ng/ml

Instrument :
ECD_P
ClientSampleId :
VEOLIA-72-11977

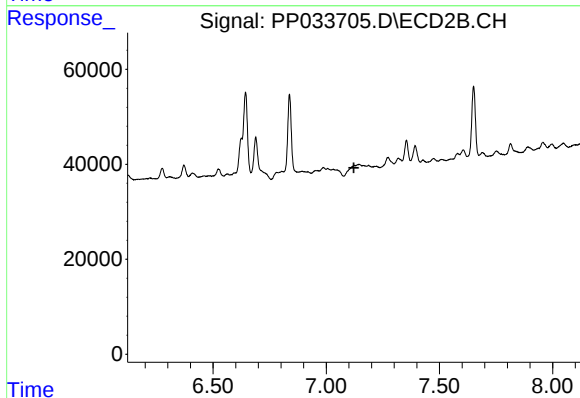


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T. : 7.122 min
Response: 0
Conc: N.D.

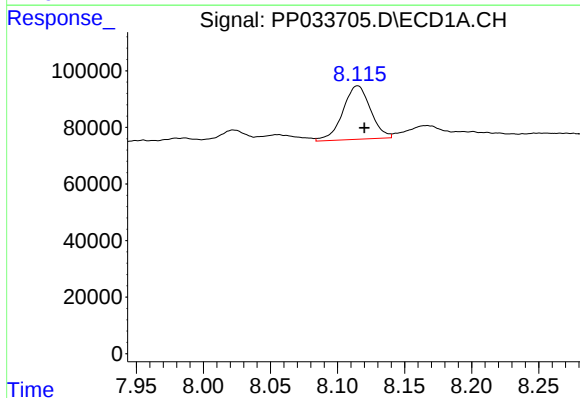


#32 AR-1260-2

R.T.: 8.115 min
Delta R.T.: -0.005 min
Response: 271766
Conc: 57.10 ng/ml

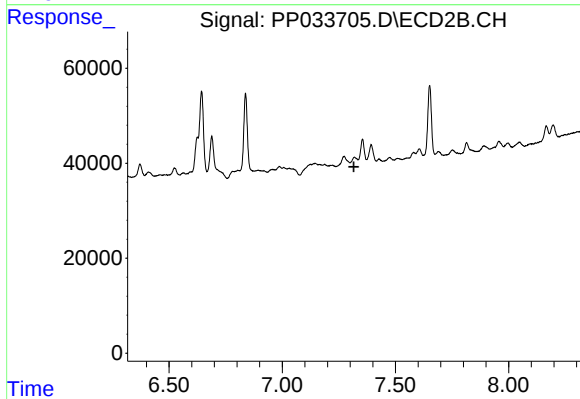

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 7.316 min
Response: 0
Conc: N.D.

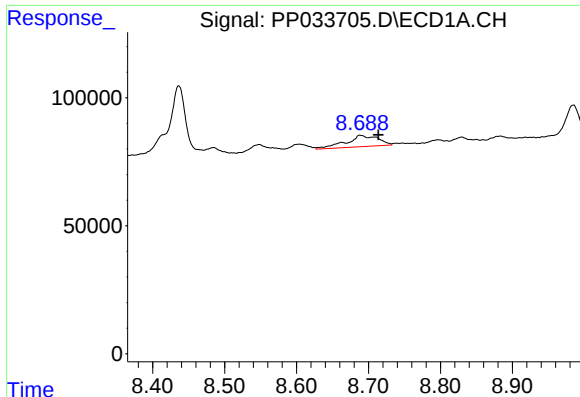

#34 AR-1260-4


R.T.: 8.688 min
Delta R.T.: -0.025 min
Response: 135074
Conc: 30.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
VEOLIA-72-11977

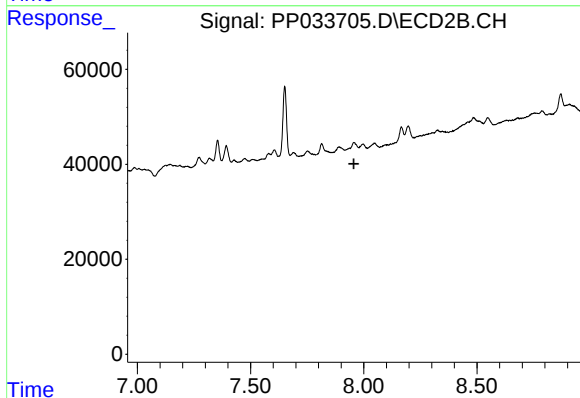


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.956 min
Response: 0
Conc: N.D.

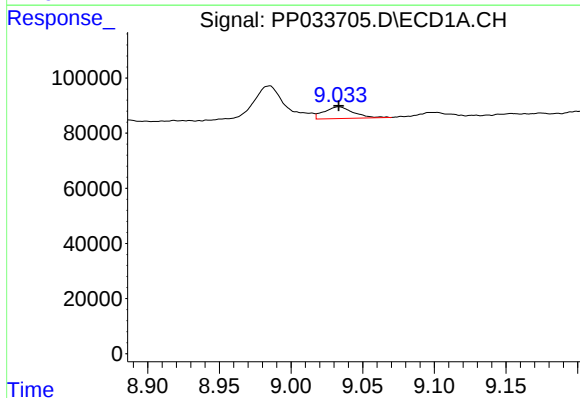


#35 AR-1260-5

R.T.: 9.033 min
Delta R.T.: 0.000 min
Response: 60554
Conc: 7.13 ng/ml

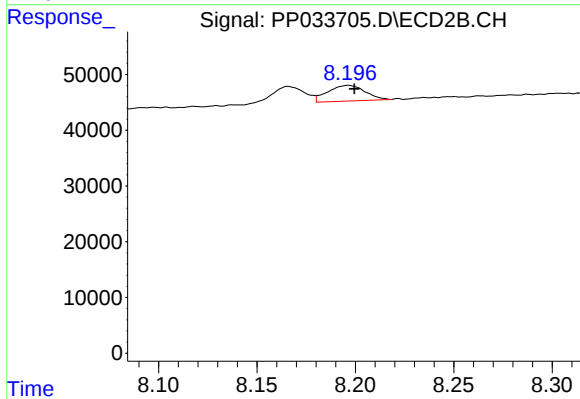

#35 AR-1260-5


R.T.: 8.196 min
Delta R.T.: -0.003 min
Response: 37482
Conc: 14.27 ng/ml

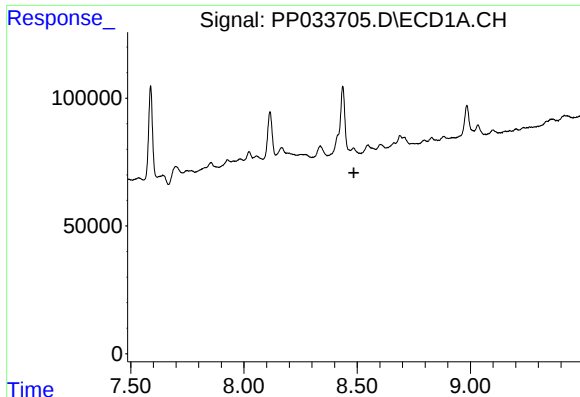

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T.: 8.486 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
VEOLIA-72-11977

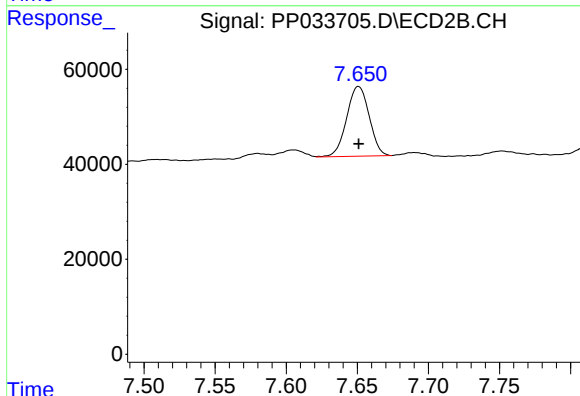


#36 AR-1262-1

R.T.: 7.651 min
Delta R.T.: 0.000 min
Response: 161982
Conc: 176.95 ng/ml

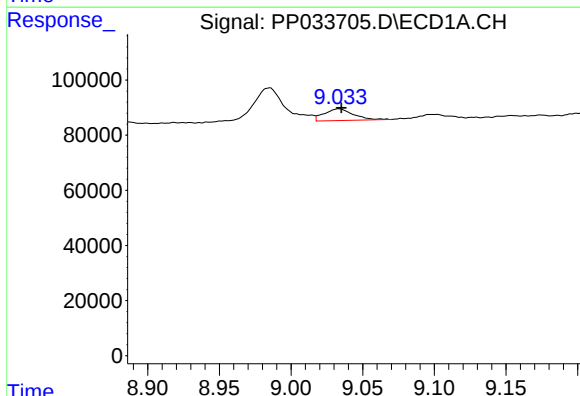


#37 AR-1262-2

R.T.: 9.033 min
Delta R.T.: -0.002 min
Response: 60554
Conc: 6.56 ng/ml

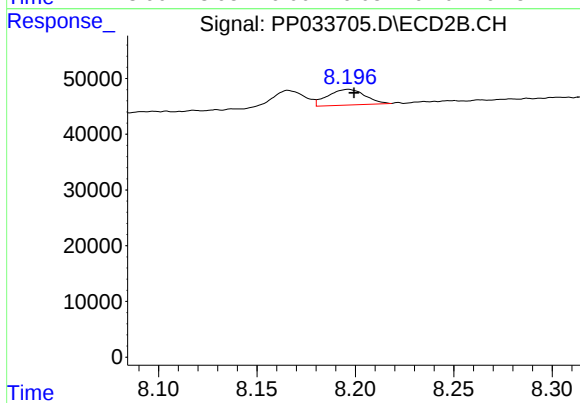

#37 AR-1262-2


R.T.: 8.196 min
Delta R.T.: -0.003 min
Response: 37482
Conc: 12.69 ng/ml

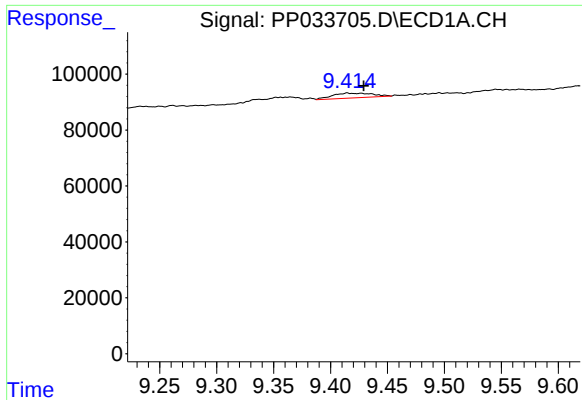

#39 AR-1262-4


R.T.: 9.415 min
Delta R.T.: -0.014 min
Response: 41418
Conc: 7.49 ng/ml

Instrument :
ECD_P
ClientSampleId :
VEOLIA-72-11977

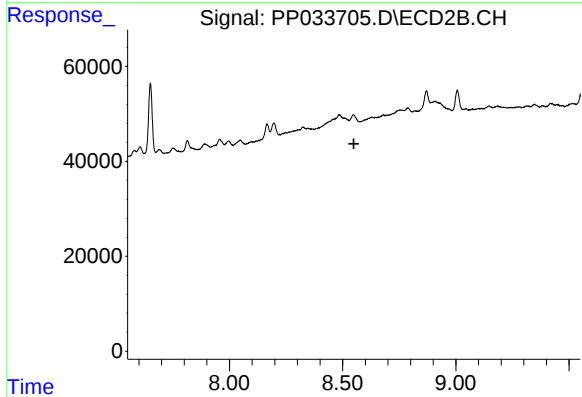


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 8.550 min
Response: 0
Conc: N.D.

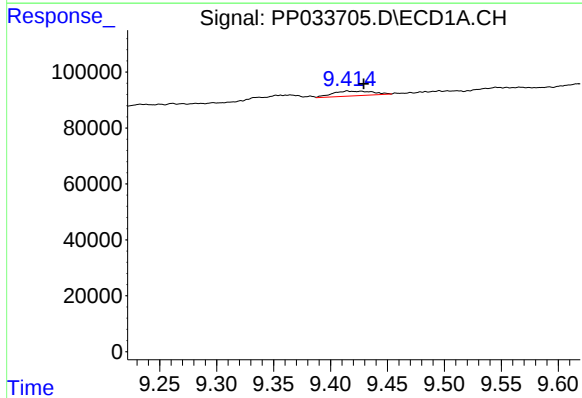


#42 AR-1268-2

R.T.: 9.415 min
Delta R.T.: -0.014 min
Response: 41418
Conc: 3.57 ng/ml

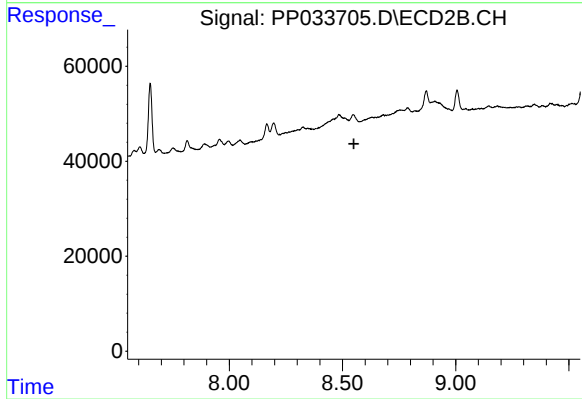

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T. : 8.550 min
Response: 0
Conc: N.D.

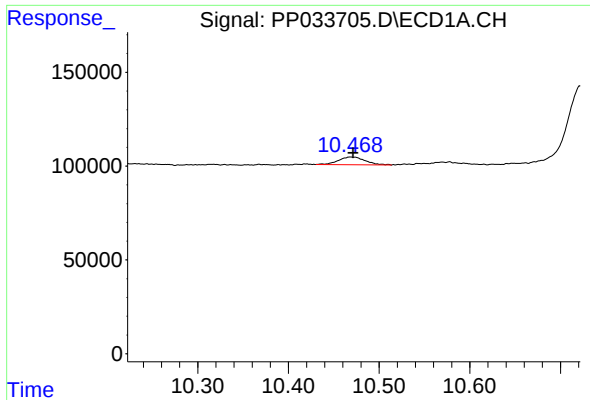

#45 AR-1268-5

R.T.: 10.469 min
Delta R.T.: -0.002 min
Response: 83354
Conc: 2.57 ng/ml

Instrument :
ECD_P
ClientSampleId :
VEOLIA-72-11977

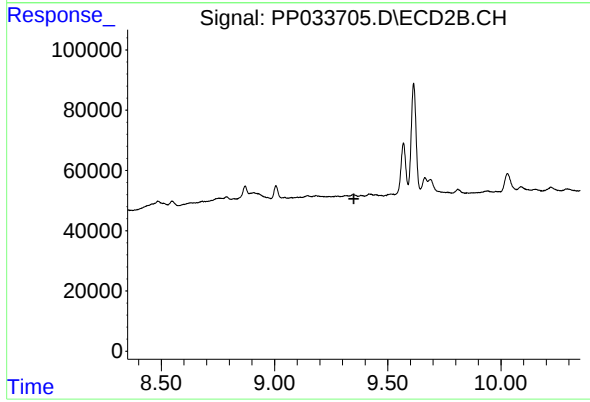

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 9.351 min
Response: 0
Conc: N.D.