

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030521\
 Data File : PP033711.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Mar 2021 17:16
 Operator : DD\AJ
 Sample : M1573-03 20X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 FCA497D-1-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 18:00:28 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 05 04:37:34 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.861	4.274	115831	45666	1.008	1.147
2) SA Decachlor...	10.793	0.000	130195	0	1.439	N.D. #

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030521\
Data File : PP033711.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Mar 2021 17:16
Operator : DD\AJ
Sample : M1573-03 20X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
FCA497D-1-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 18:00:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030421.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 05 04:37:34 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

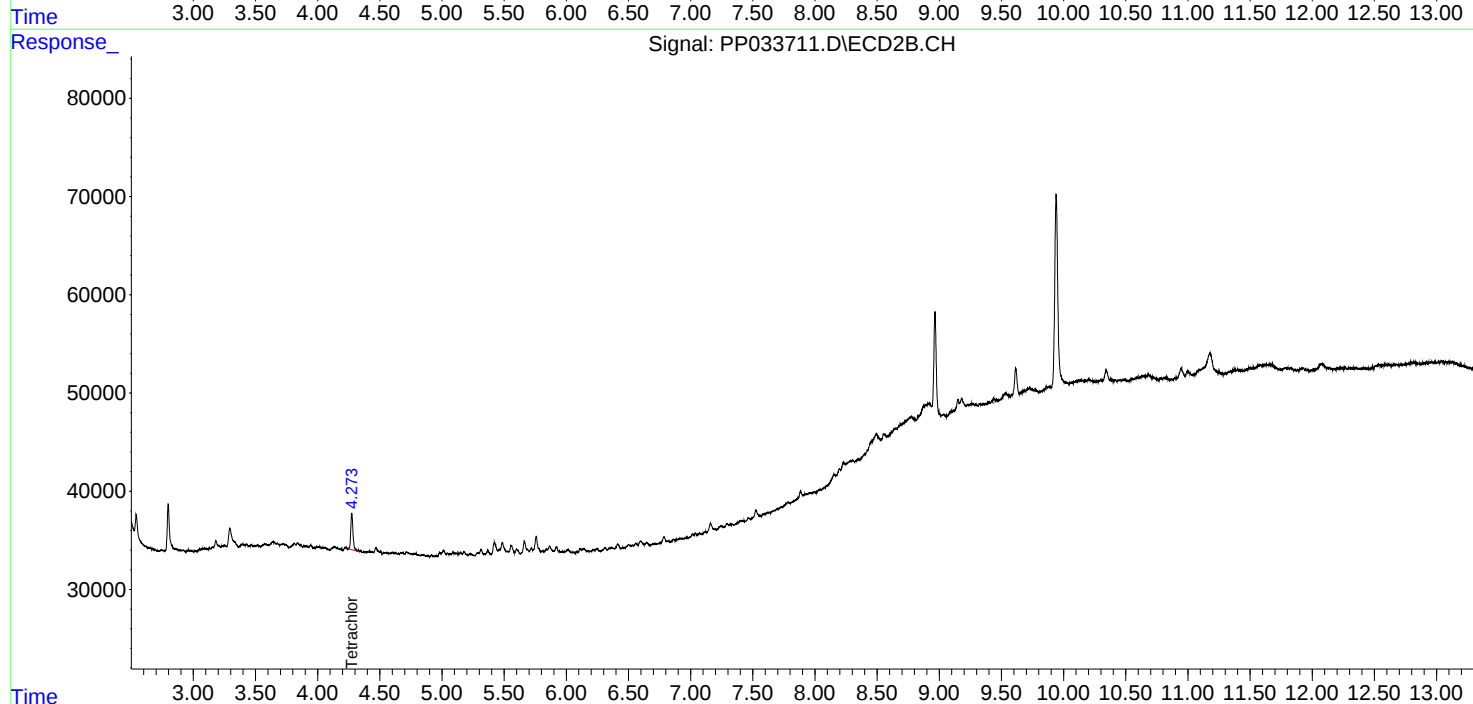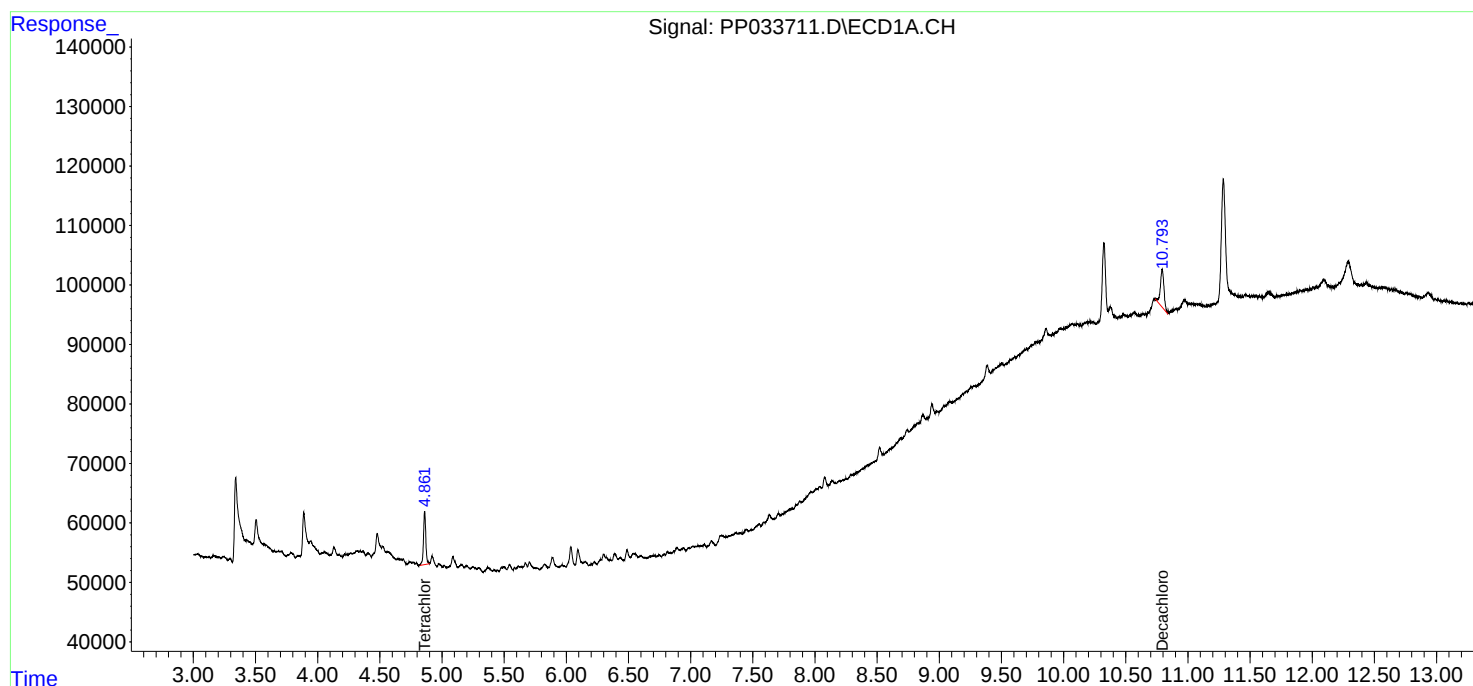


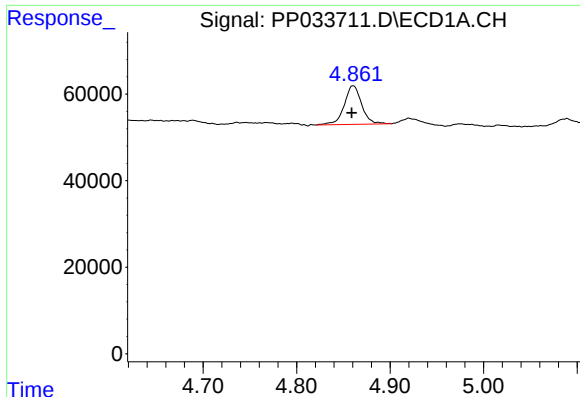

#1 Tetrachloro-m-xylene


R.T.: 4.861 min
Delta R.T.: 0.002 min
Response: 115831
Conc: 1.01 ng/ml

Instrument :
ECD_P
ClientSampleId :
FCA497D-1-1

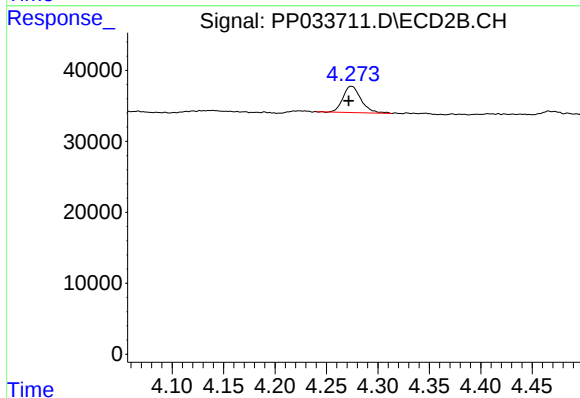


#1 Tetrachloro-m-xylene

R.T.: 4.274 min
Delta R.T.: 0.003 min
Response: 45666
Conc: 1.15 ng/ml

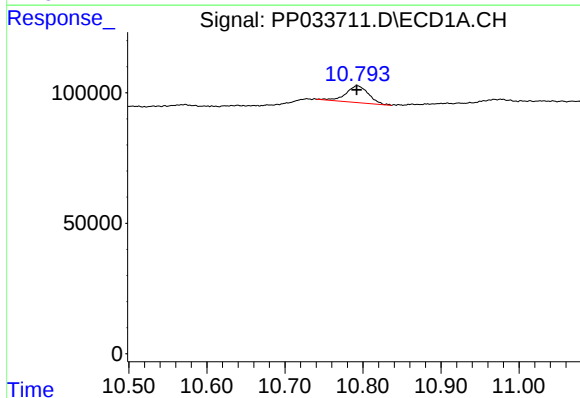

#2 Decachlorobiphenyl

R.T.: 10.793 min
Delta R.T.: 0.002 min
Response: 130195
Conc: 1.44 ng/ml

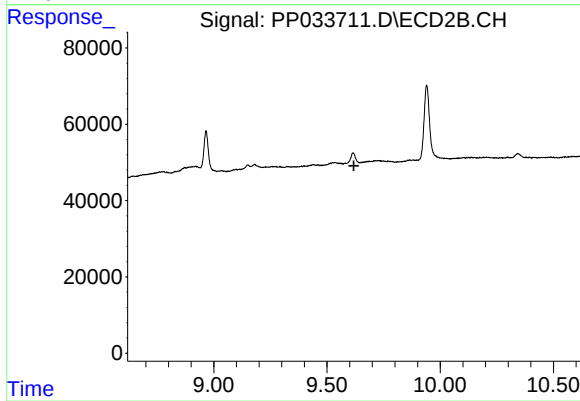

#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.618 min
Response: 0
Conc: N.D.