

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030521\
 Data File : PP033690.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Mar 2021 11:16
 Operator : DD\AJ
 Sample : M1538-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 1-2-TOTES

Manual Integrations
 APPROVED

Ankita
 3/8/2021 12:11:10 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 11:29:30 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 05 04:37:34 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.861	4.275	1193145	403379	10.387	10.132
2) SA Decachlor...	10.791	9.613	1031829	273784	11.403m	11.720

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030521\
Data File : PP033690.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Mar 2021 11:16
Operator : DD\AJ
Sample : M1538-01
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
1-2-TOTES


Manual Integrations
APPROVED

Ankita
3/8/2021 12:11:10 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 11:29:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030421.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 05 04:37:34 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

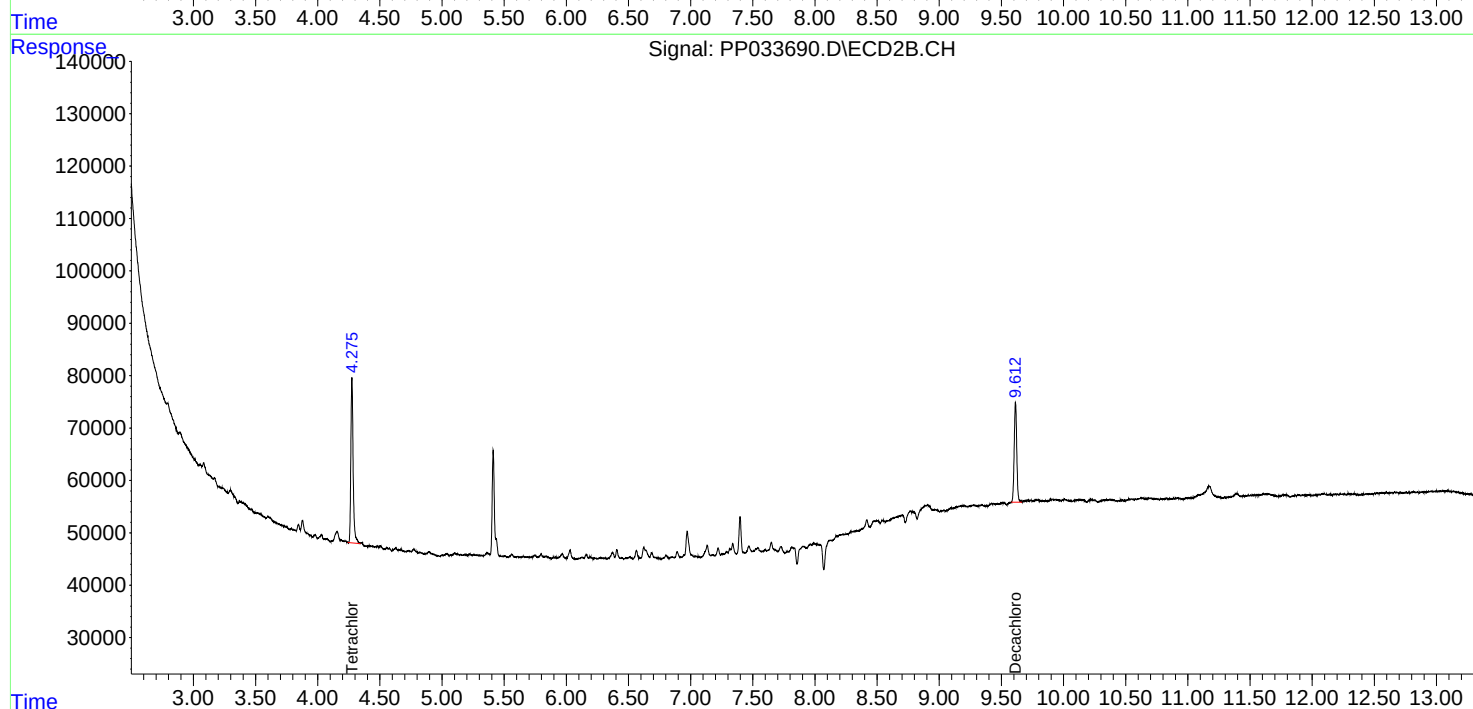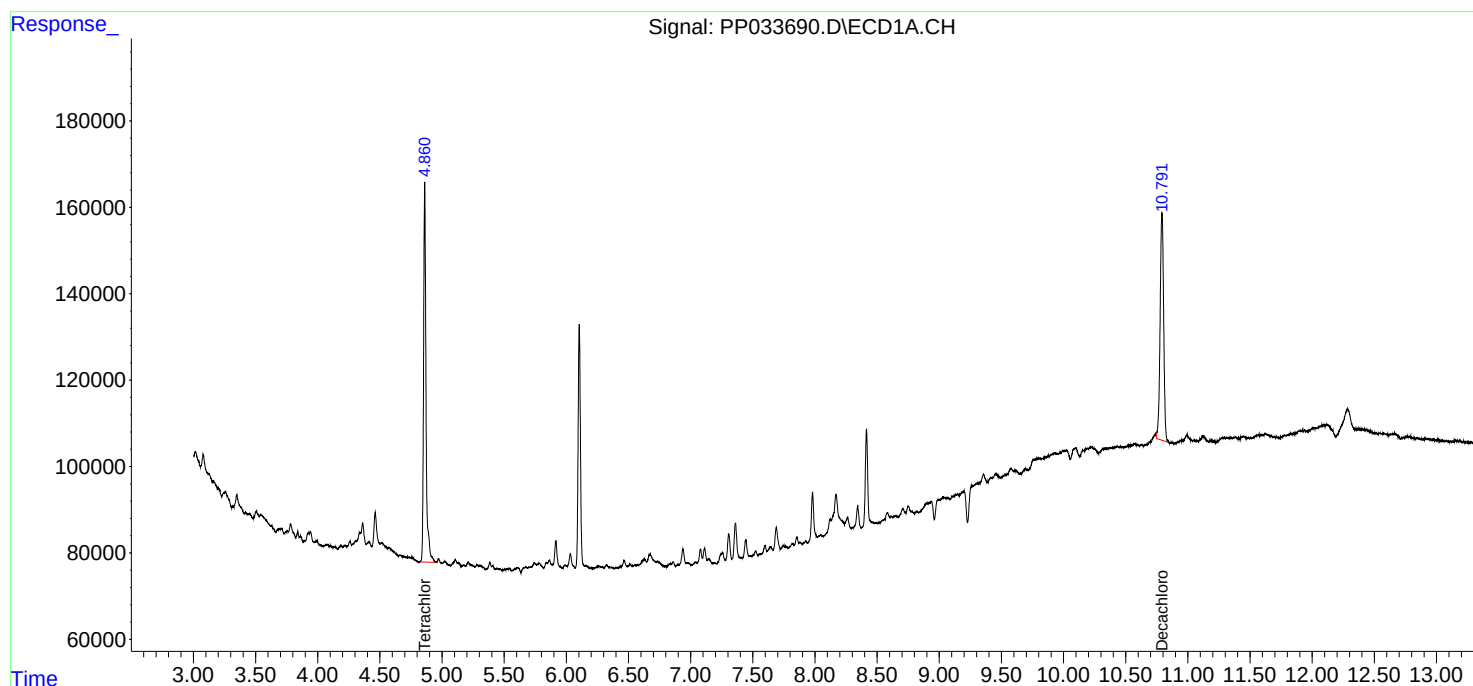

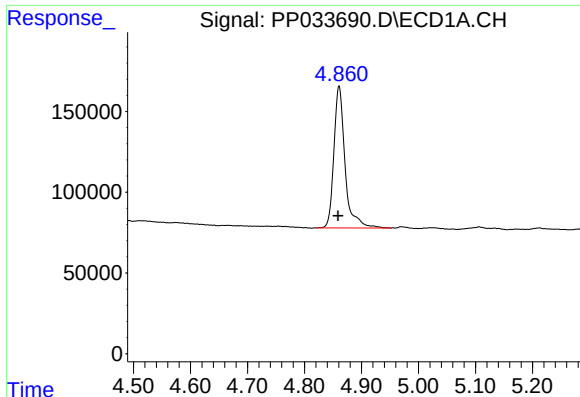


#1 Tetrachloro-m-xylene

R.T.: 4.861 min
Delta R.T.: 0.002 min
Response: 1193145
Conc: 10.39 ng/ml

Instrument :
ECD_P
ClientSampleId :
1-2-TOTES


Manual Integrations
APPROVED

Ankita
3/8/2021 12:11:10 PM

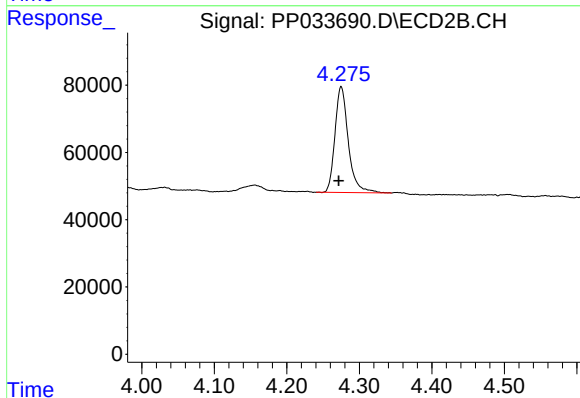


#1 Tetrachloro-m-xylene

R.T.: 4.275 min
Delta R.T.: 0.003 min
Response: 403379
Conc: 10.13 ng/ml

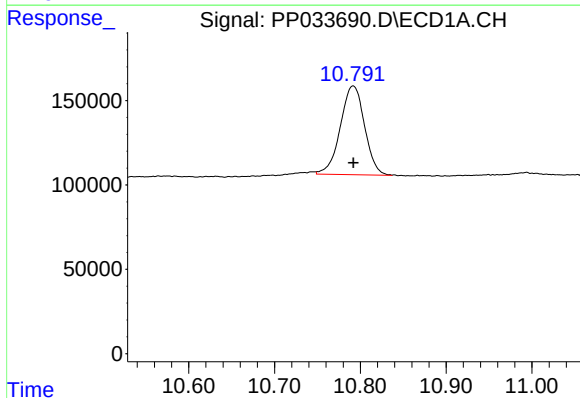

#2 Decachlorobiphenyl

R.T.: 10.791 min
Delta R.T.: 0.000 min
Response: 1031829
Conc: 11.40 ng/ml m

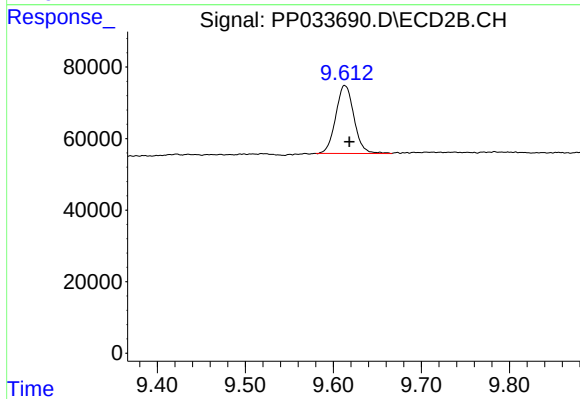

#2 Decachlorobiphenyl

R.T.: 9.613 min
Delta R.T.: -0.005 min
Response: 273784
Conc: 11.72 ng/ml