

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030521\
 Data File : PP033691.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Mar 2021 11:33
 Operator : DD\AJ
 Sample : M1551-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 VEOLIA-VNJ-204

Manual Integrations
 APPROVED

Ankita
 3/8/2021 12:10:25 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 11:58:21 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 05 04:37:34 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.859	4.274	2384665	880301	20.760	22.111
2) SA Decachlor...	10.791	9.614	2468461	663461	27.278	28.400
Target Compounds						
31) L7 AR-1260-1	7.854	7.123	149346	64541	36.110m	47.652m#
32) L7 AR-1260-2	8.117	7.316	380217	76929	79.891	49.705 #
33) L7 AR-1260-3	8.483	7.473	184918	65243	48.432	44.061
34) L7 AR-1260-4	8.710	7.955	185783	55788	41.993m	45.537
35) L7 AR-1260-5	9.033	8.196	346600	125354	40.818	47.728m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030521\
Data File : PP033691.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Mar 2021 11:33
Operator : DD\AJ
Sample : M1551-01
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
VEOLIA-VNJ-204


Manual Integrations
APPROVED

Ankita
3/8/2021 12:10:25 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 11:58:21 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030421.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 05 04:37:34 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

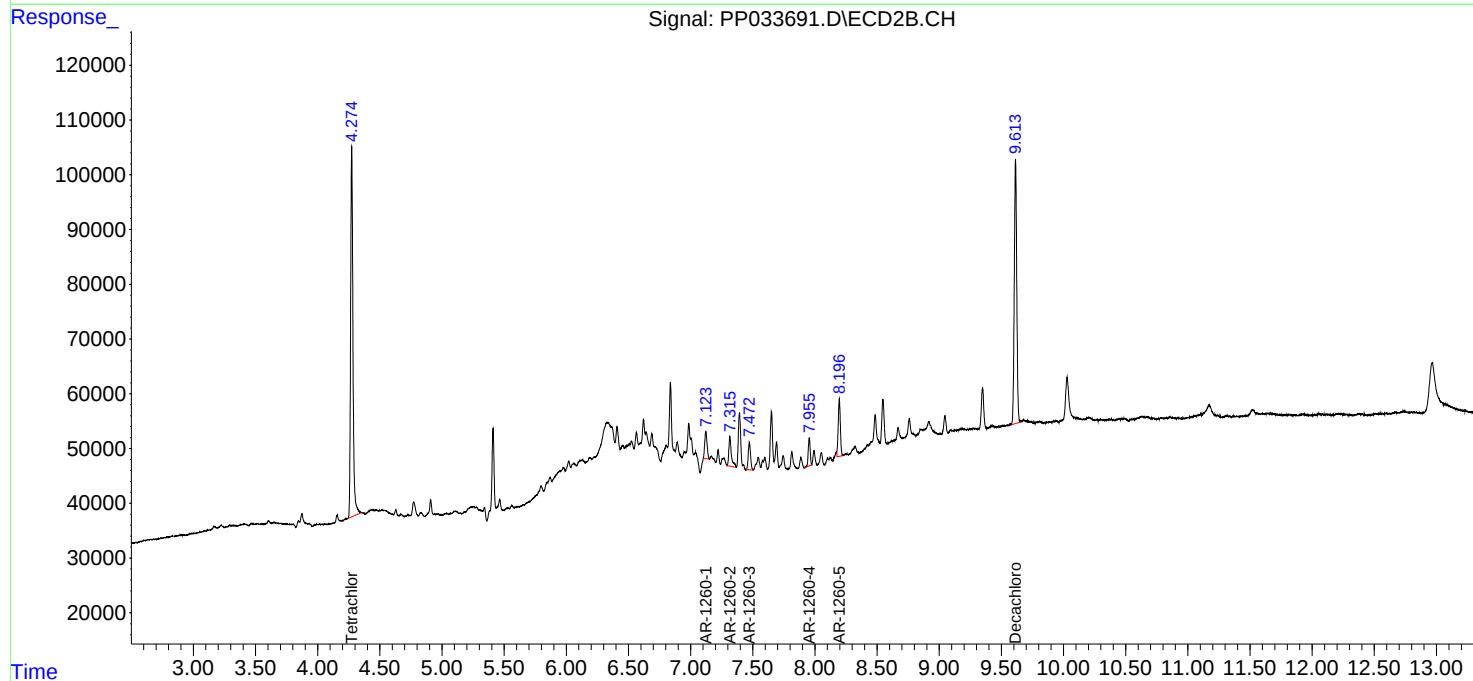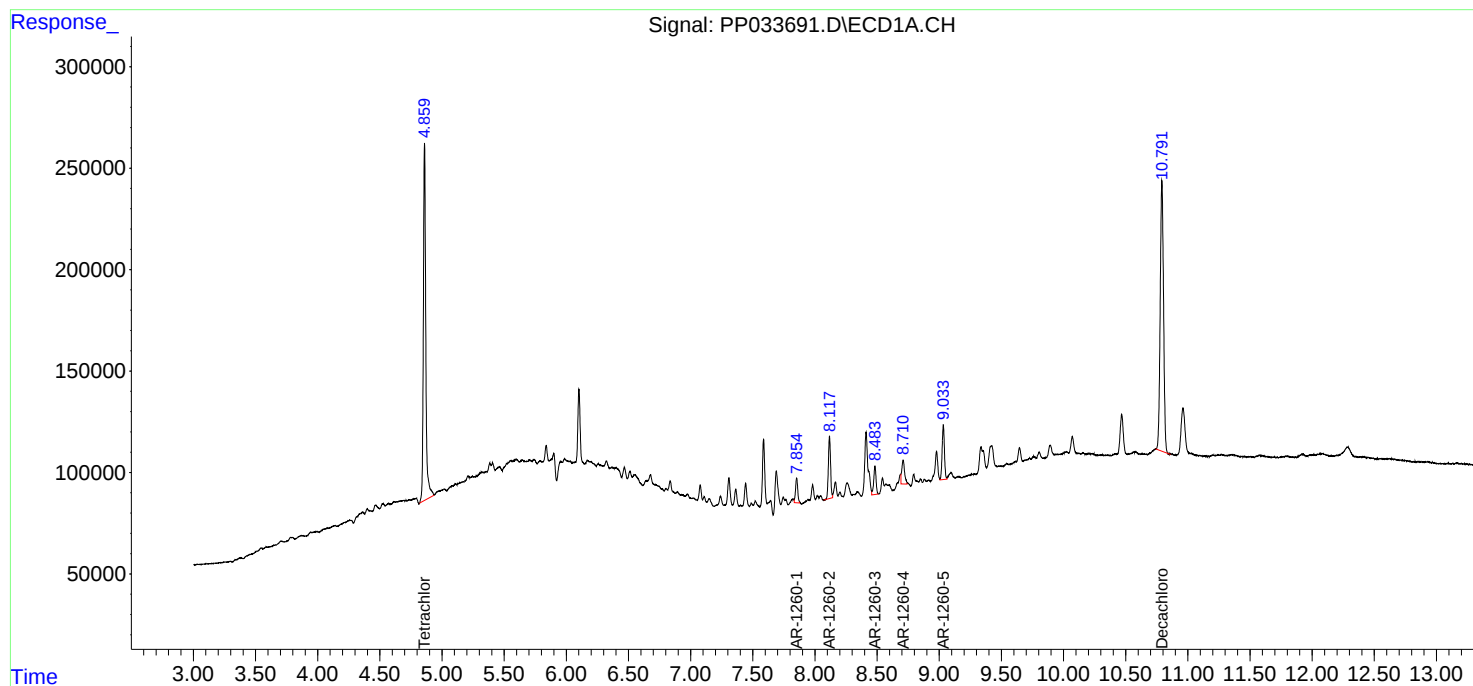

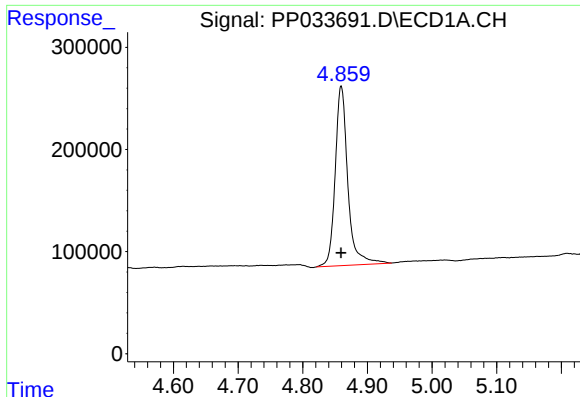


#1 Tetrachloro-m-xylene

R.T.: 4.859 min
Delta R.T.: 0.000 min
Response: 2384665
Conc: 20.76 ng/ml

Instrument :
ECD_P
ClientSampleId :
VEOLIA-VNJ-204


Manual Integrations
APPROVED

Ankita
3/8/2021 12:10:25 PM

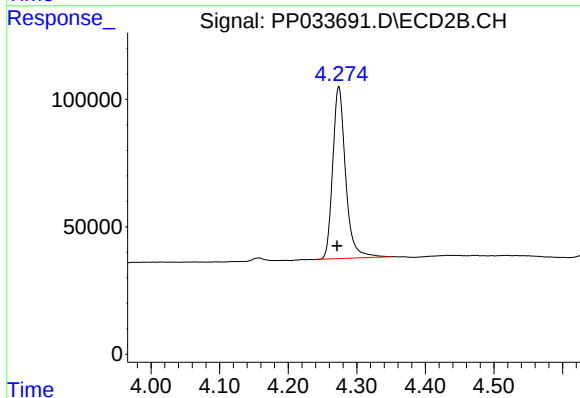


#1 Tetrachloro-m-xylene

R.T.: 4.274 min
Delta R.T.: 0.002 min
Response: 880301
Conc: 22.11 ng/ml

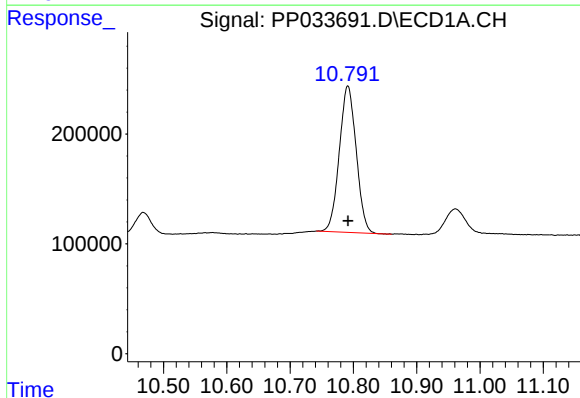


#2 Decachlorobiphenyl

R.T.: 10.791 min
Delta R.T.: 0.000 min
Response: 2468461
Conc: 27.28 ng/ml

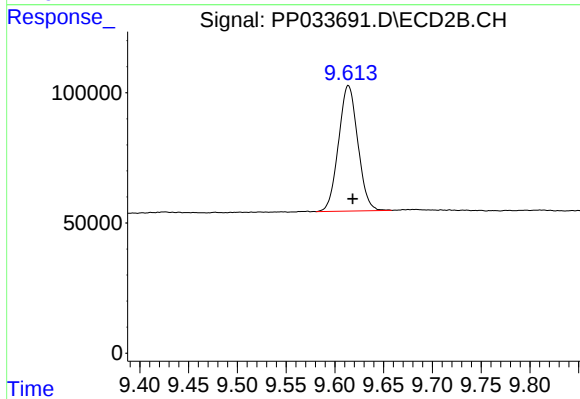

#2 Decachlorobiphenyl

R.T.: 9.614 min
Delta R.T.: -0.004 min
Response: 663461
Conc: 28.40 ng/ml

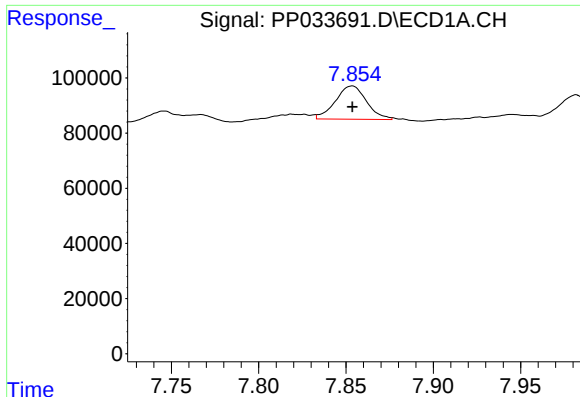


#31 AR-1260-1

R.T.: 7.854 min
Delta R.T.: 0.000 min
Response: 149346
Conc: 36.11 ng/ml m

Instrument :
ECD_P
ClientSampleId :
VEOLIA-VNJ-204


Manual Integrations
APPROVED

Ankita
3/8/2021 12:10:25 PM

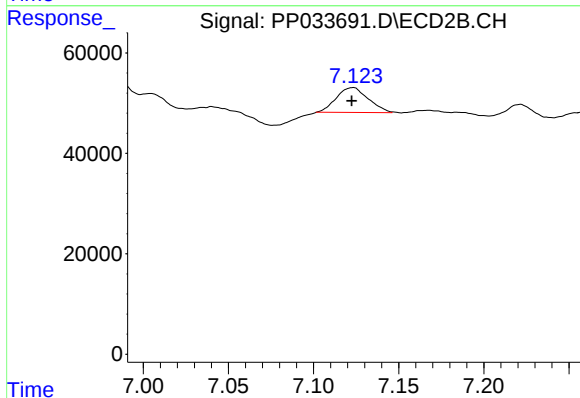


#31 AR-1260-1

R.T.: 7.123 min
Delta R.T.: 0.000 min
Response: 64541
Conc: 47.65 ng/ml m

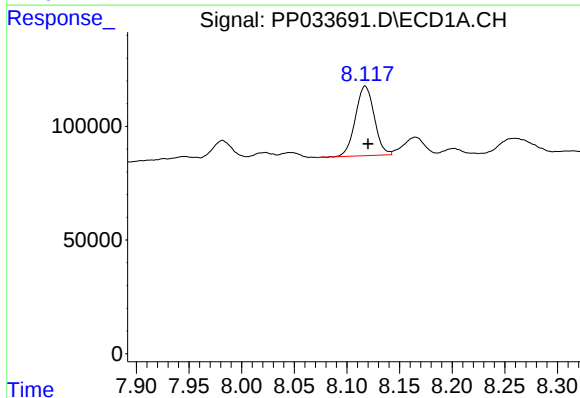


#32 AR-1260-2

R.T.: 8.117 min
Delta R.T.: -0.003 min
Response: 380217
Conc: 79.89 ng/ml

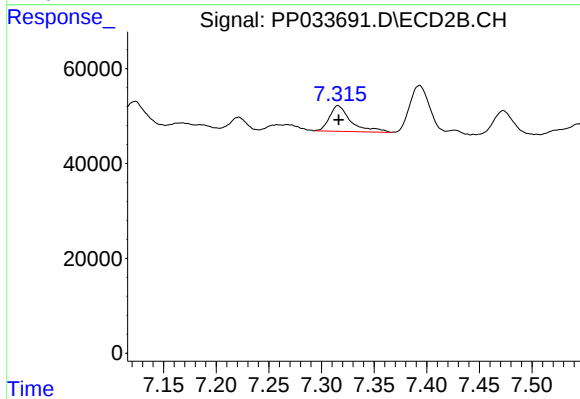

#32 AR-1260-2

R.T.: 7.316 min
Delta R.T.: 0.000 min
Response: 76929
Conc: 49.71 ng/ml

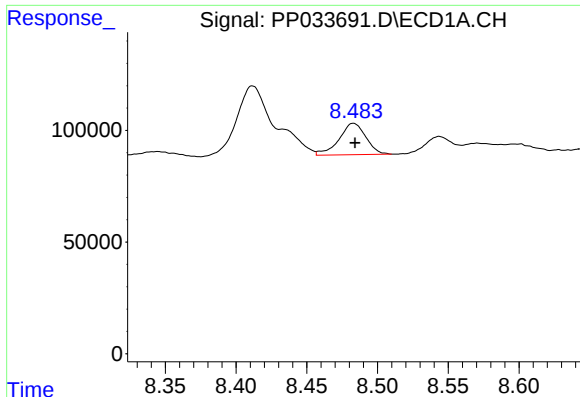


#33 AR-1260-3

R.T.: 8.483 min
Delta R.T.: -0.001 min
Response: 184918
Conc: 48.43 ng/ml

Instrument :
ECD_P
ClientSampleId :
VEOLIA-VNJ-204


Manual Integrations
APPROVED

Ankita
3/8/2021 12:10:25 PM

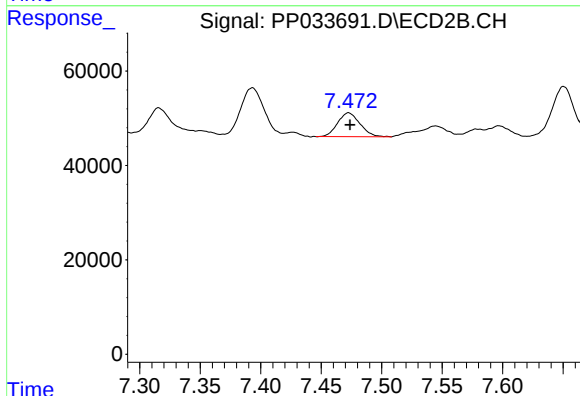


#33 AR-1260-3

R.T.: 7.473 min
Delta R.T.: -0.001 min
Response: 65243
Conc: 44.06 ng/ml

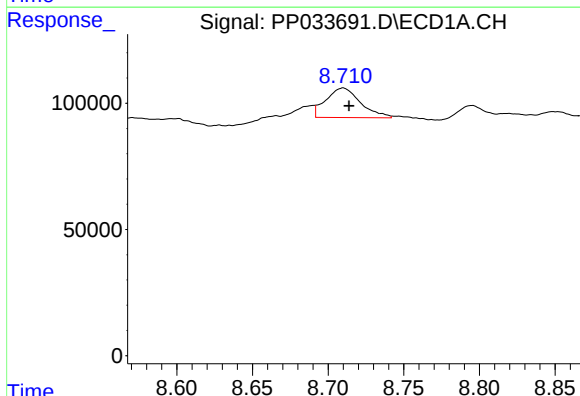


#34 AR-1260-4

R.T.: 8.710 min
Delta R.T.: -0.004 min
Response: 185783
Conc: 41.99 ng/ml m

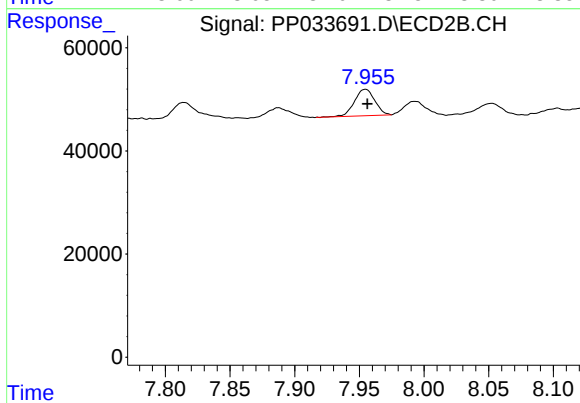

#34 AR-1260-4

R.T.: 7.955 min
Delta R.T.: -0.002 min
Response: 55788
Conc: 45.54 ng/ml

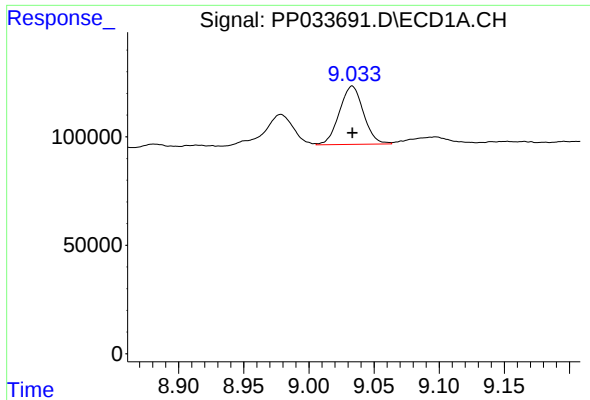


#35 AR-1260-5

R.T.: 9.033 min
Delta R.T.: 0.000 min
Response: 346600
Conc: 40.82 ng/ml

Instrument :
ECD_P
ClientSampleId :
VEOLIA-VNJ-204

Manual Integrations
APPROVED

Ankita
3/8/2021 12:10:25 PM

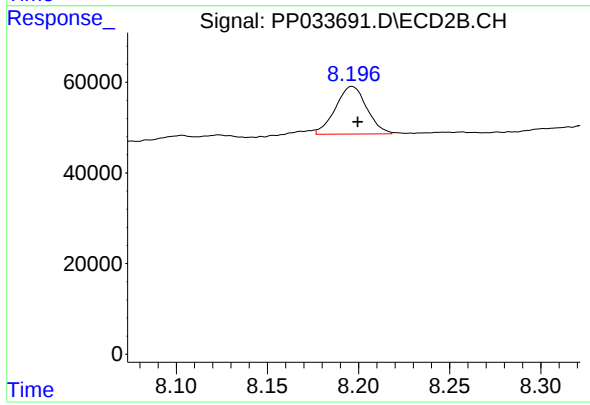

#35 AR-1260-5

R.T.: 8.196 min
Delta R.T.: -0.004 min
Response: 125354
Conc: 47.73 ng/ml m