

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030521\
 Data File : PP033705.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 05 Mar 2021 15:34
 Operator : DD\AJ
 Sample : M1566-03
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 VEOLIA-72-11977

Manual Integrations
 APPROVED

Ankita
 3/8/2021 12:10:48 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 05 15:54:31 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 05 04:37:34 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.860	4.274	2282050	890521	19.866	22.367
2) SA Decachlor...	10.792	9.614	1901725	544374	21.016m	23.302m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030521\
Data File : PP033705.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 05 Mar 2021 15:34
Operator : DD\AJ
Sample : M1566-03
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
VEOLIA-72-11977


Manual Integrations
APPROVED

Ankita
3/8/2021 12:10:48 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 05 15:54:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030421.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 05 04:37:34 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

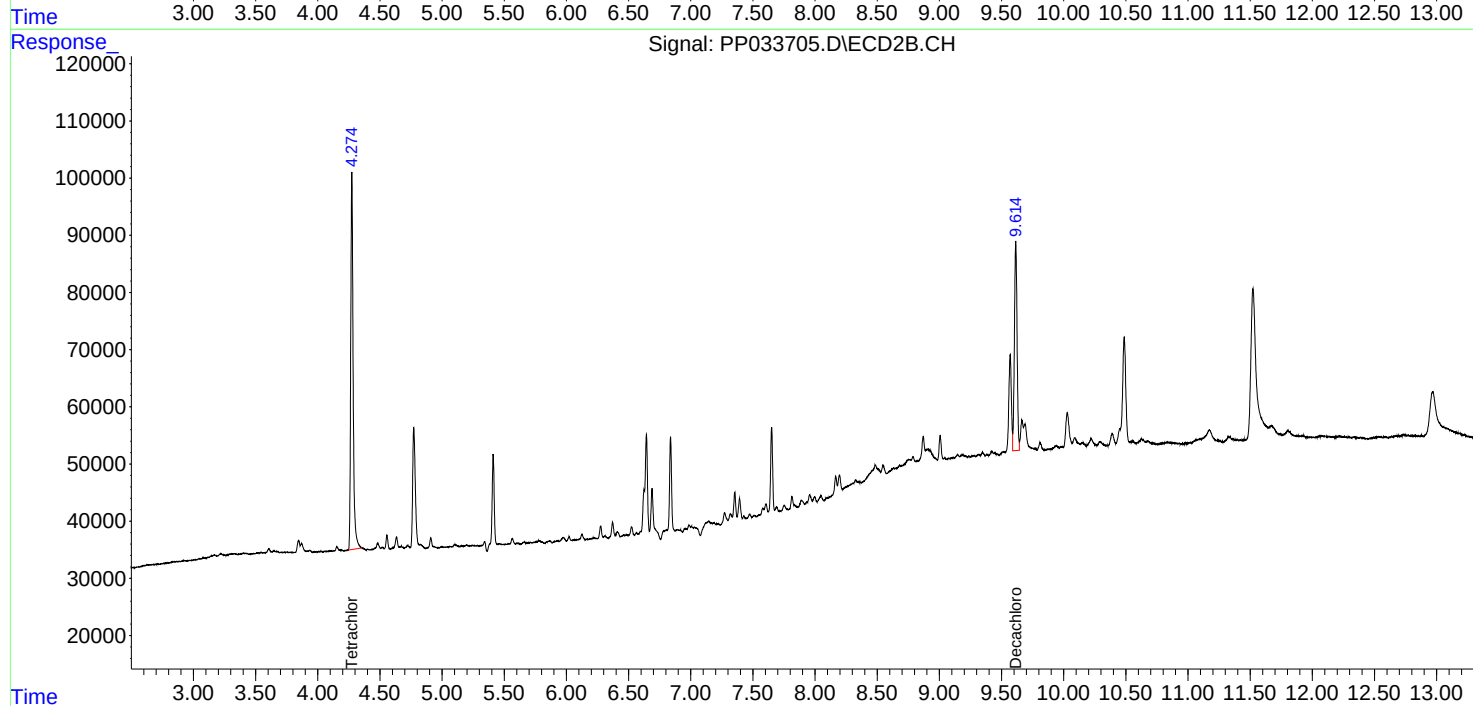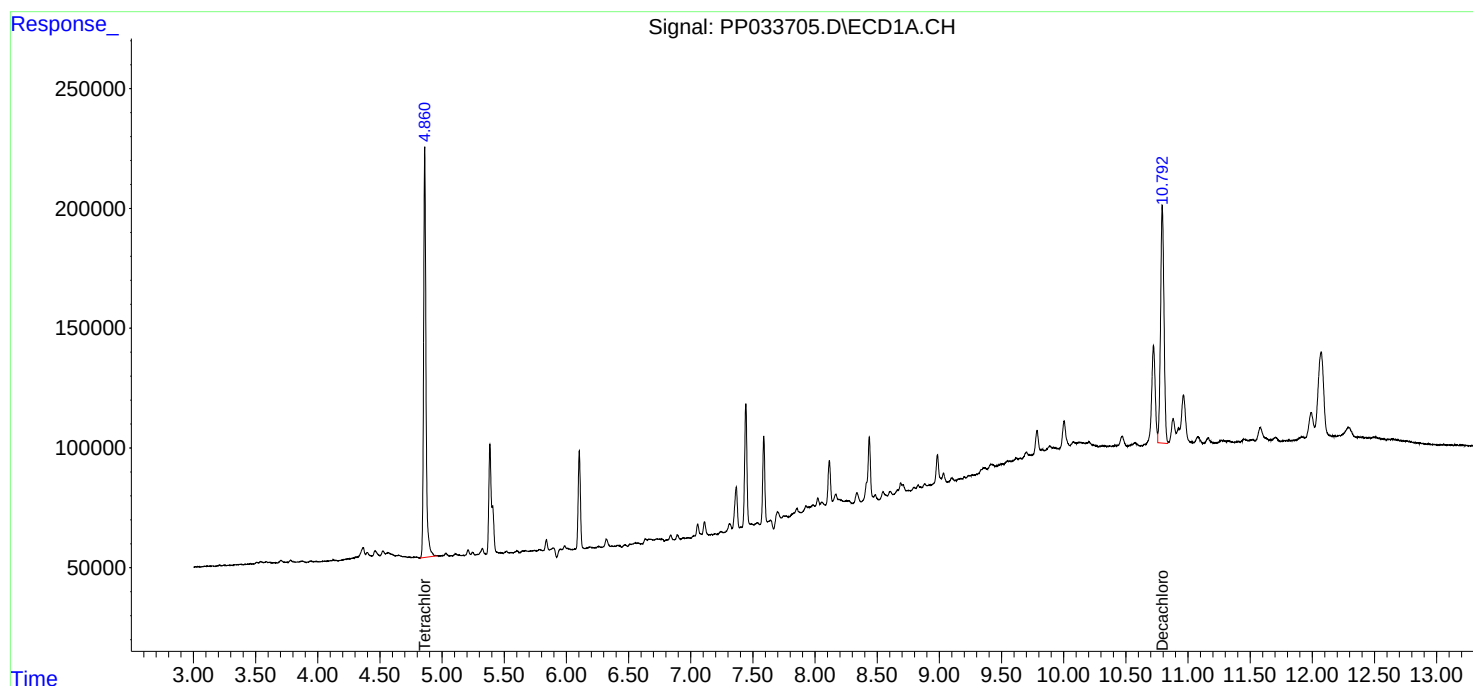

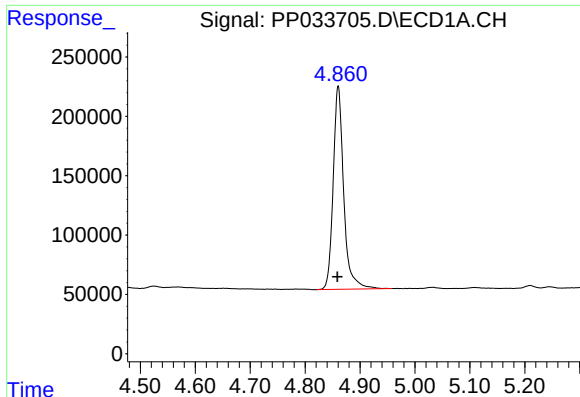


#1 Tetrachloro-m-xylene

R.T.: 4.860 min
Delta R.T.: 0.001 min
Response: 2282050
Conc: 19.87 ng/ml

Instrument :
ECD_P
ClientSampleId :
VEOLIA-72-11977


Manual Integrations
APPROVED

Ankita
3/8/2021 12:10:48 PM

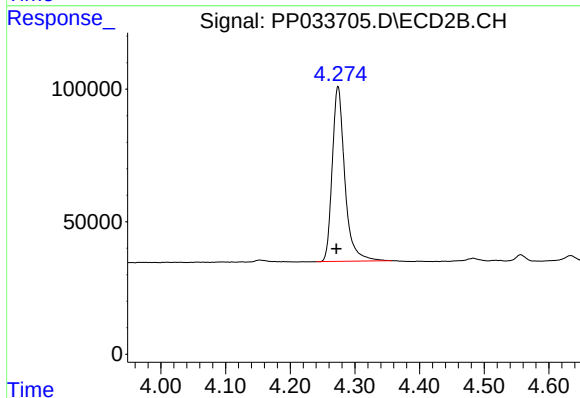


#1 Tetrachloro-m-xylene

R.T.: 4.274 min
Delta R.T.: 0.002 min
Response: 890521
Conc: 22.37 ng/ml

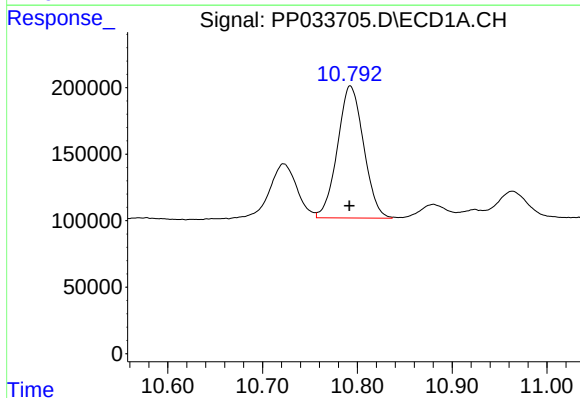

#2 Decachlorobiphenyl

R.T.: 10.792 min
Delta R.T.: 0.000 min
Response: 1901725
Conc: 21.02 ng/ml m

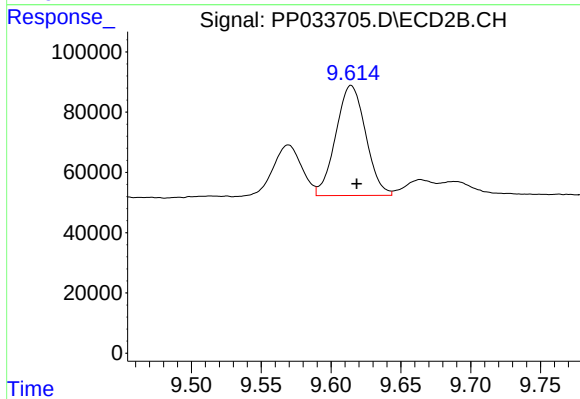

#2 Decachlorobiphenyl

R.T.: 9.614 min
Delta R.T.: -0.005 min
Response: 544374
Conc: 23.30 ng/ml m