

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP030521\  
 Data File : PP033711.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 05 Mar 2021 17:16  
 Operator : DD\AJ  
 Sample : M1573-03 20X  
 Misc :  
 ALS Vial : 22 Sample Multiplier: 1

Instrument :  
 ECD\_P  
 ClientSampleId :  
 FCA497D-1-1

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 05 18:00:28 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP030421.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Fri Mar 05 04:37:34 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

-----

System Monitoring Compounds

Target Compounds

-----



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP030521\  
Data File : PP033711.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 05 Mar 2021 17:16  
Operator : DD\AJ  
Sample : M1573-03 20X  
Misc :  
ALS Vial : 22 Sample Multiplier: 1

Instrument :  
ECD\_P  
ClientSampleId :  
FCA497D-1-1

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Mar 05 18:00:28 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP030421.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Fri Mar 05 04:37:34 2021  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

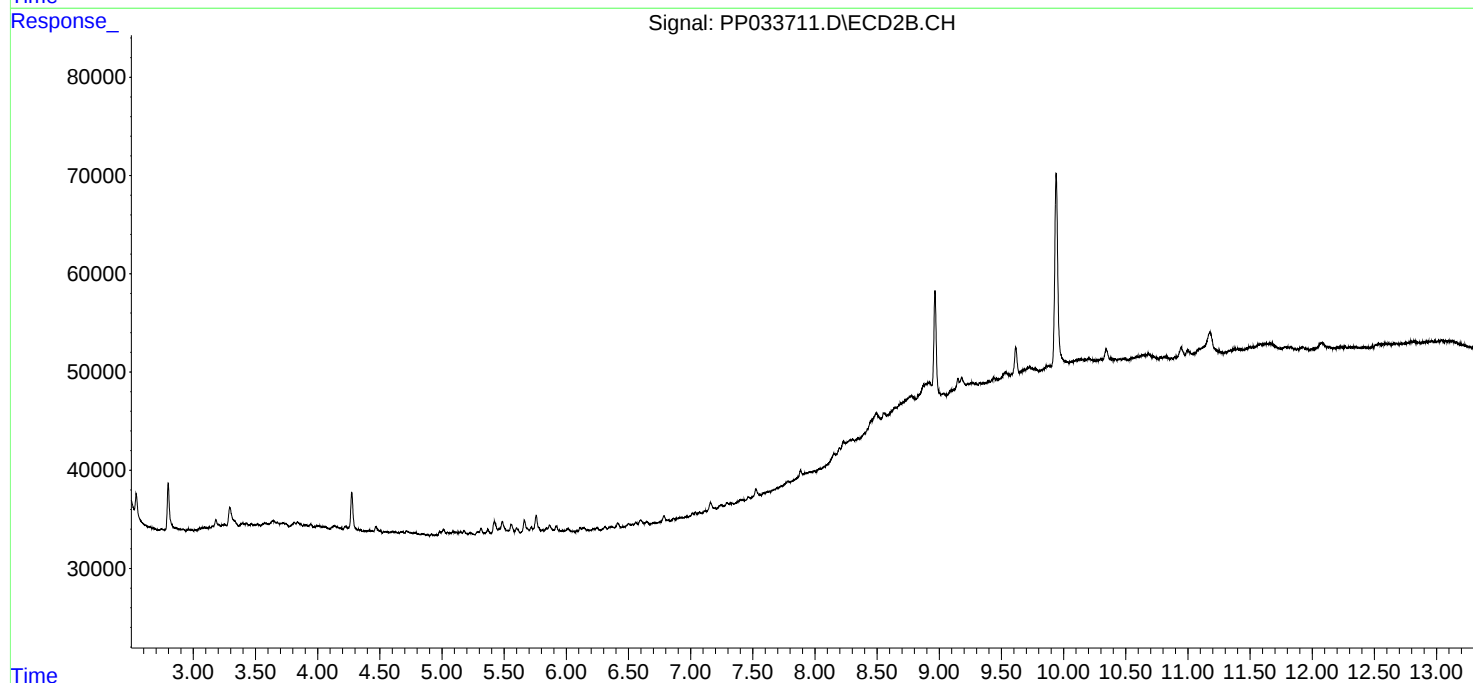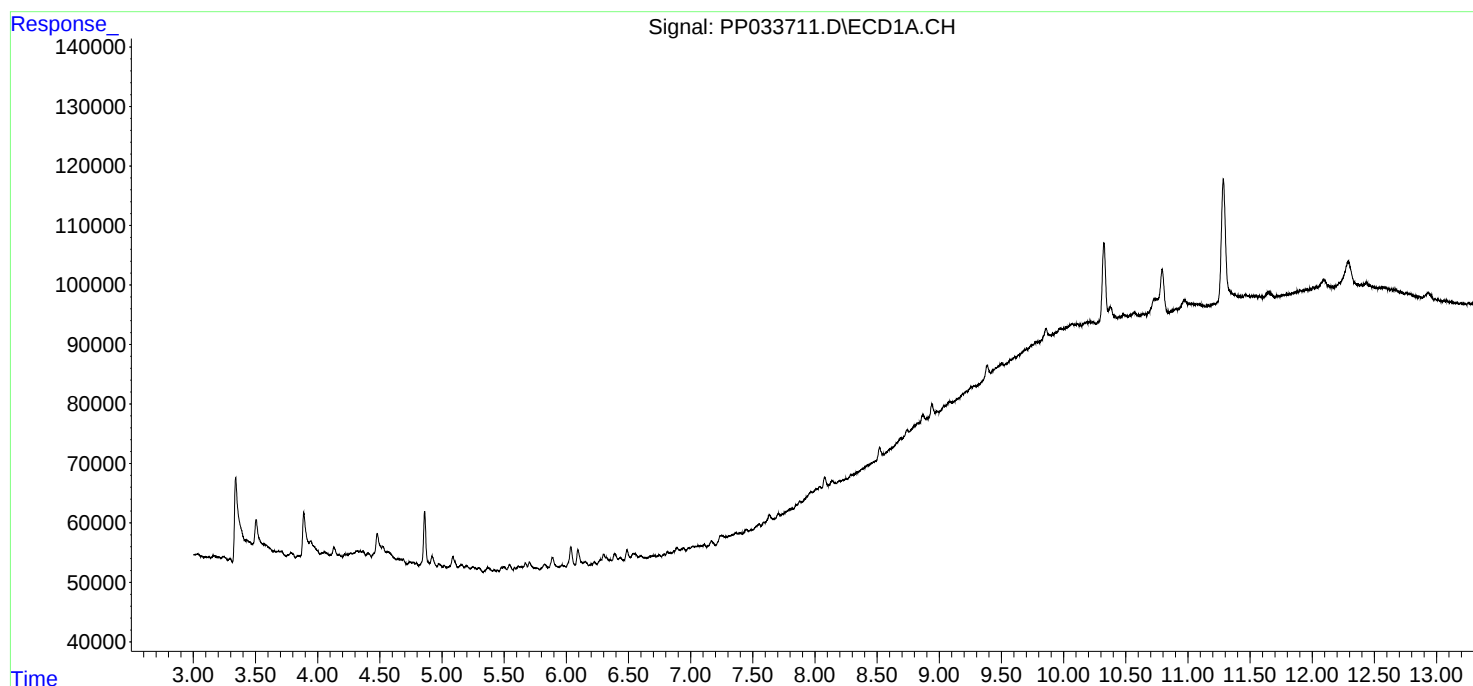


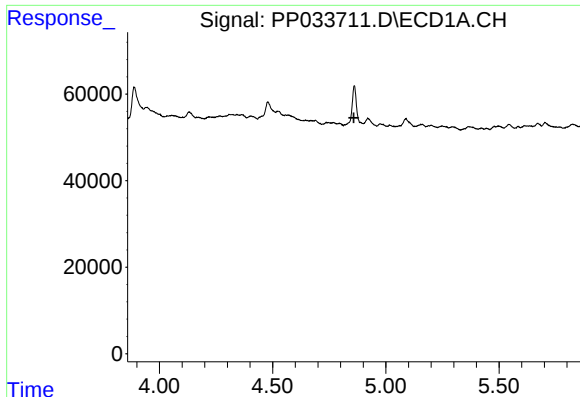

#1 Tetrachloro-m-xylene


R.T.: 0.000 min  
Exp R.T. : 4.859 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_P  
ClientSampleId :  
FCA497D-1-1

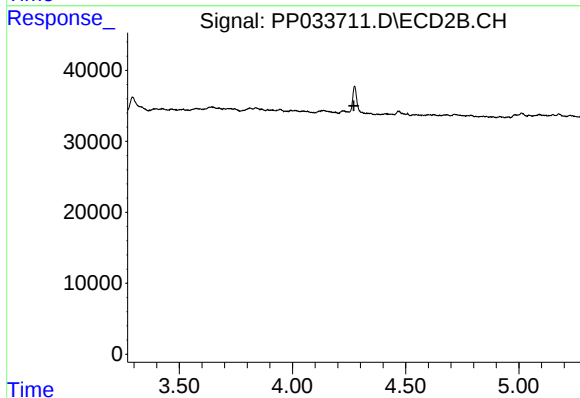


#1 Tetrachloro-m-xylene

R.T.: 0.000 min  
Exp R.T. : 4.272 min  
Response: 0  
Conc: N.D.

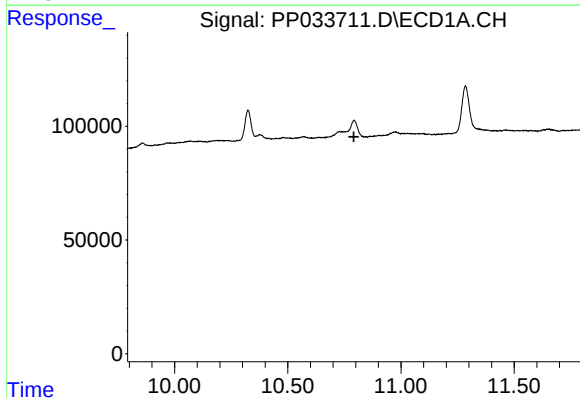

#2 Decachlorobiphenyl

R.T.: 0.000 min  
Exp R.T. : 10.792 min  
Response: 0  
Conc: N.D.

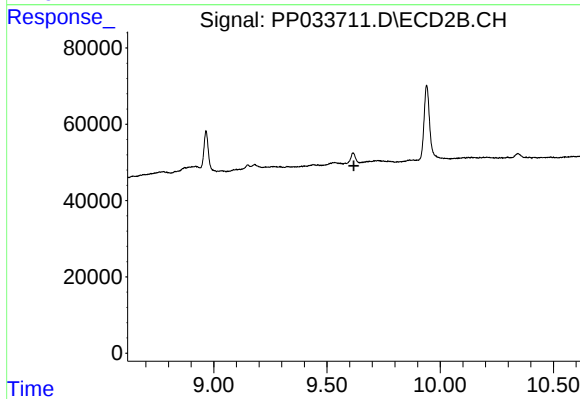

#2 Decachlorobiphenyl

R.T.: 0.000 min  
Exp R.T. : 9.618 min  
Response: 0  
Conc: N.D.