

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030623\
 Data File : PP056216.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Mar 2023 11:45
 Operator : YP\AJ
 Sample : 01763-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
ClientSampleId :
 CM-A-CRUSHED-MASONRY-PILE-1

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/07/2023
 Supervised By :Ankita Jodhani 03/07/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 06 12:15:18 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP021723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 20 05:24:03 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.320	3.563	42890910	32789184	26.620	22.456
2) SA Decachlor...	10.063	8.561	39963352	27122933	19.590	23.907m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030623\
Data File : PP056216.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Mar 2023 11:45
Operator : YP\AJ
Sample : 01763-01
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
CM-A-CRUSHED-MASONRY-PILE-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/07/2023
Supervised By :Ankita Jodhani 03/07/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 06 12:15:18 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP021723.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 20 05:24:03 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

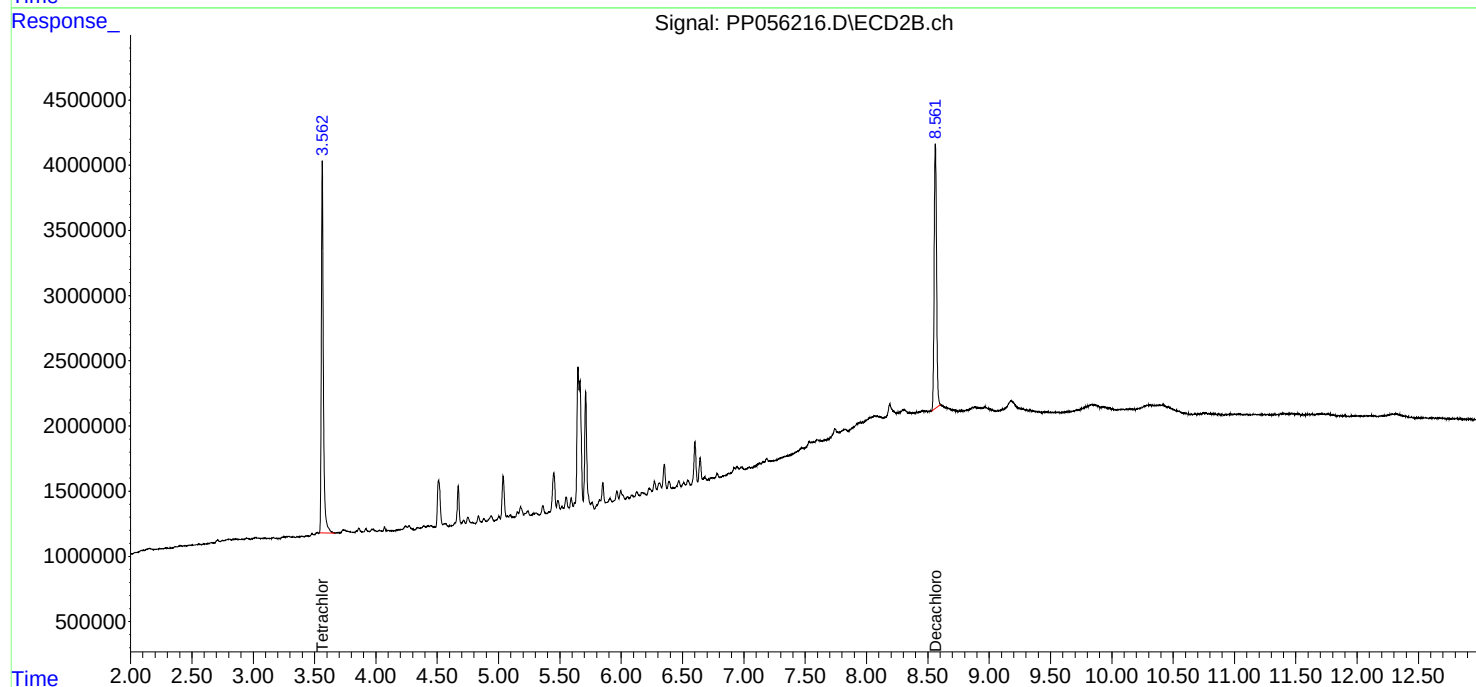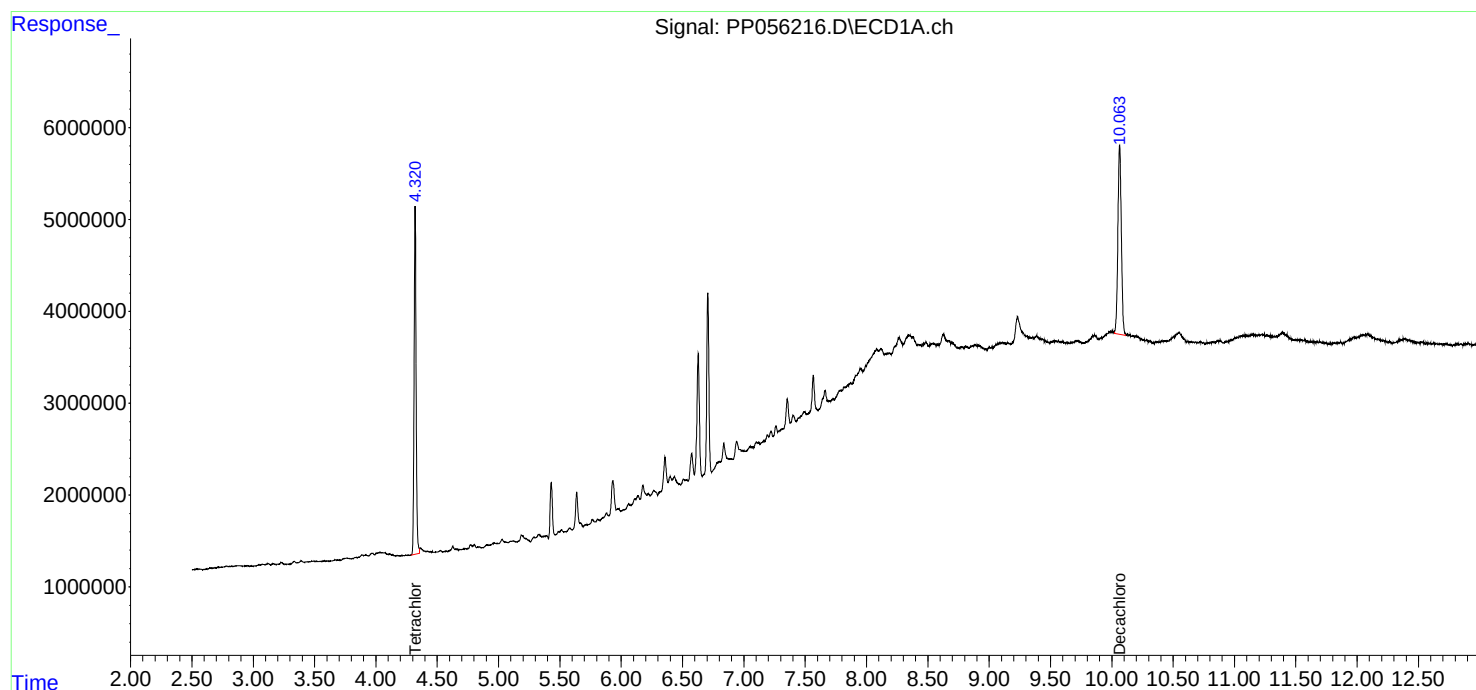

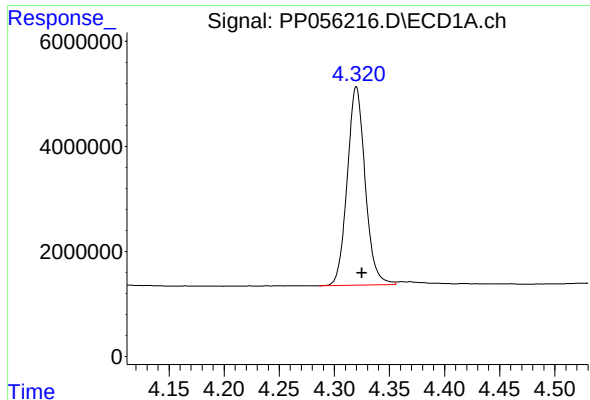

#1 Tetrachloro-m-xylene

R.T.: 4.320 min
Delta R.T.: -0.005 min
Response: 42890910
Conc: 26.62 ng/ml

Instrument :


ECD_P

ClientSampleId :

CM-A-CRUSHED-MASONRY-PILE-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/07/2023
Supervised By :Ankita Jodhani 03/07/2023

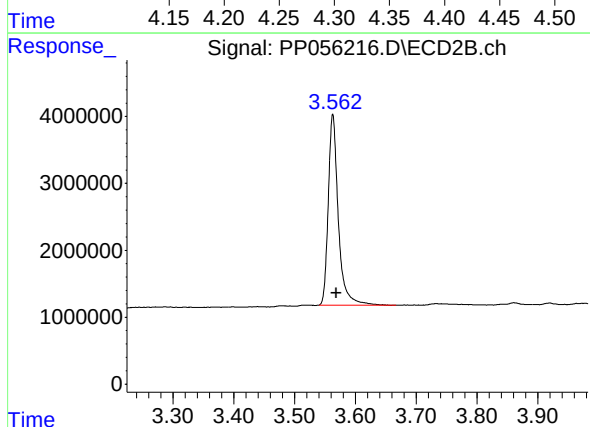


#1 Tetrachloro-m-xylene

R.T.: 3.563 min
Delta R.T.: -0.006 min
Response: 32789184
Conc: 22.46 ng/ml

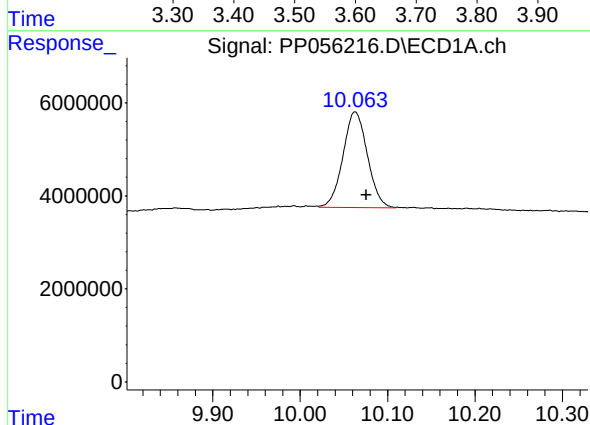

#2 Decachlorobiphenyl

R.T.: 10.063 min
Delta R.T.: -0.013 min
Response: 39963352
Conc: 19.59 ng/ml

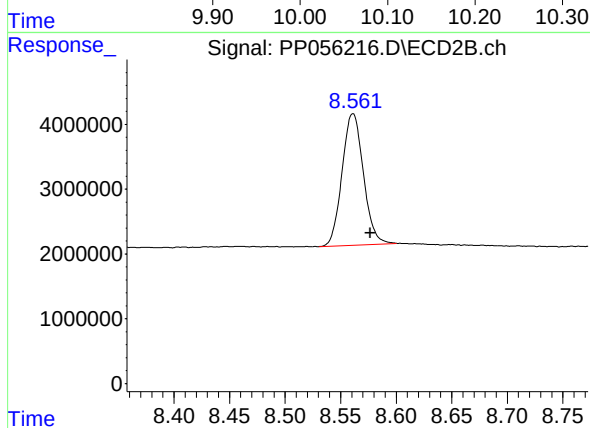

#2 Decachlorobiphenyl

R.T.: 8.561 min
Delta R.T.: -0.016 min
Response: 27122933
Conc: 23.91 ng/ml m