

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030623\
 Data File : PP056245.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Mar 2023 21:12
 Operator : YP\AJ
 Sample : 01820-03
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HR-4-03032023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 06 23:43:52 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP021723.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Feb 20 05:24:03 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.320	3.563	34546343	26439388	21.441	18.107
2) SA Decachlor...	10.068	8.563	30980575	21174930	15.187	18.665

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030623\
Data File : PP056245.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Mar 2023 21:12
Operator : YP\AJ
Sample : 01820-03
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
HR-4-03032023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 06 23:43:52 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP021723.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Feb 20 05:24:03 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

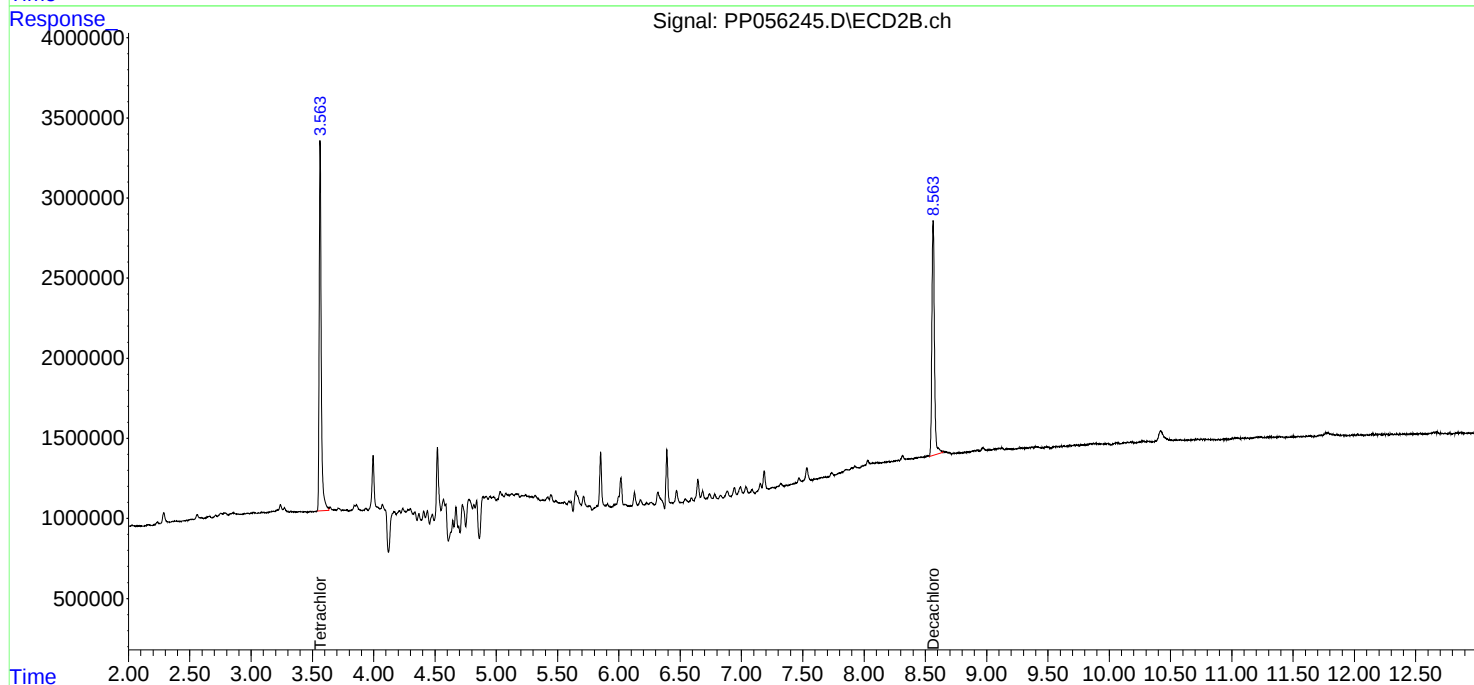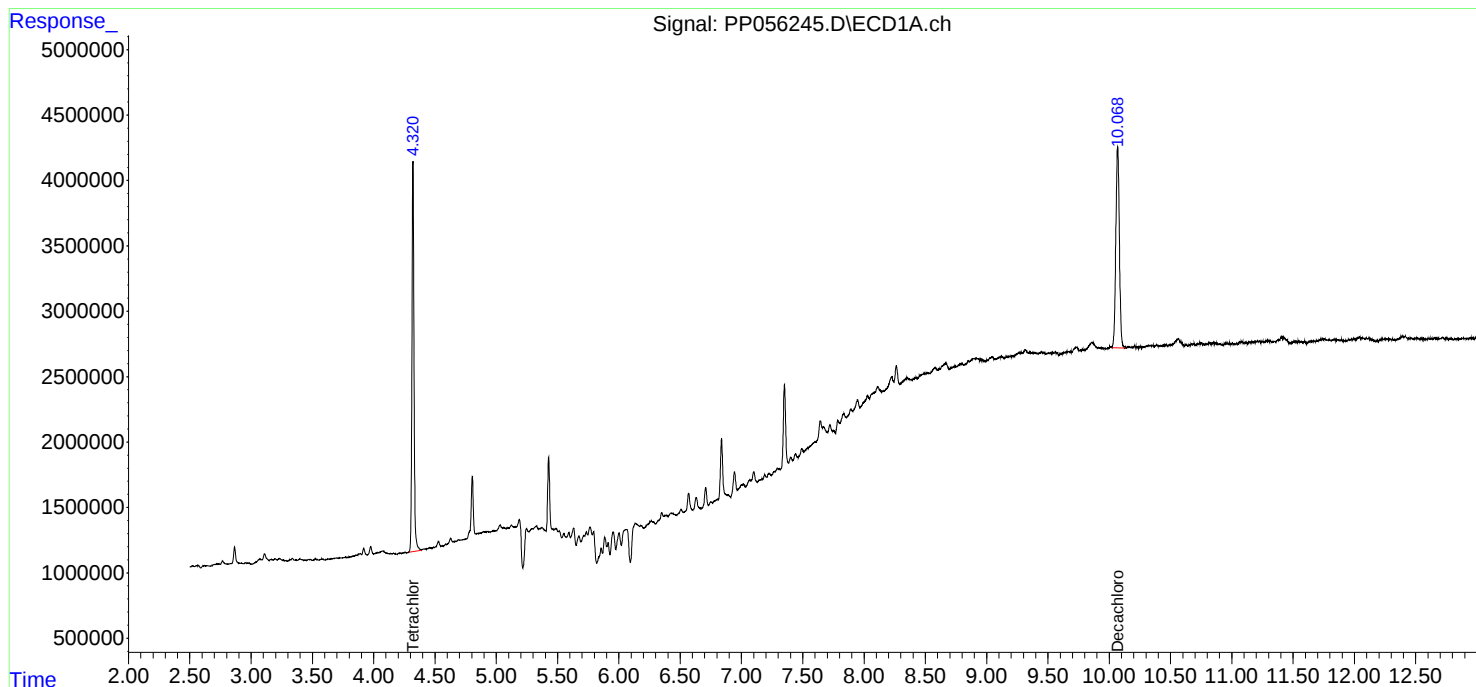


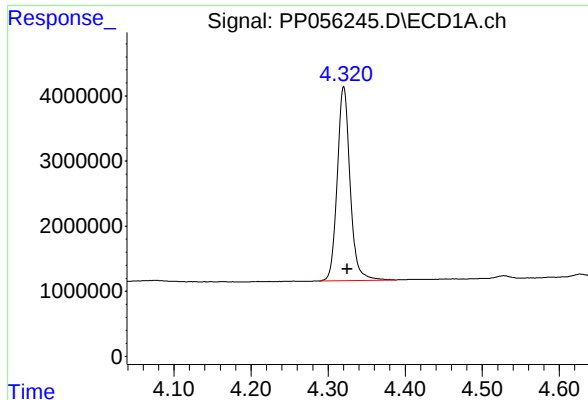

#1 Tetrachloro-m-xylene


R.T.: 4.320 min
Delta R.T.: -0.005 min
Response: 34546343
Conc: 21.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
HR-4-03032023

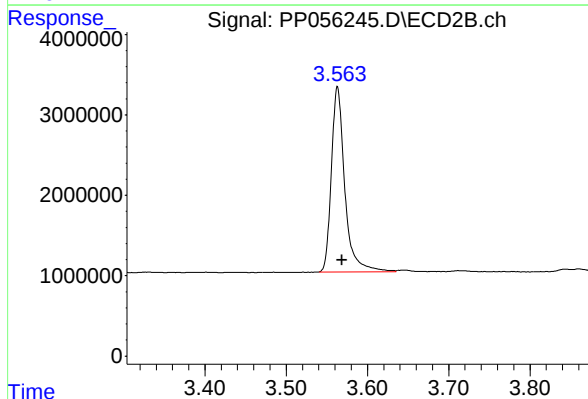


#1 Tetrachloro-m-xylene

R.T.: 3.563 min
Delta R.T.: -0.005 min
Response: 26439388
Conc: 18.11 ng/ml

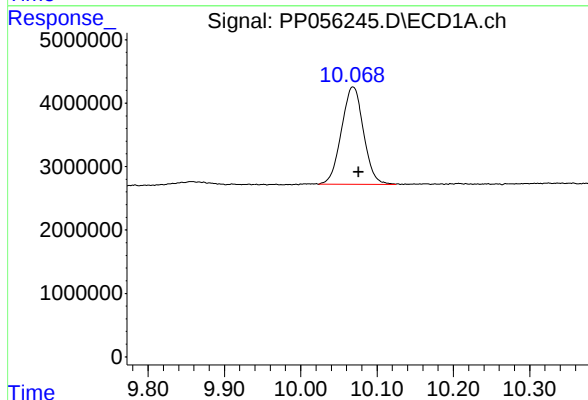

#2 Decachlorobiphenyl

R.T.: 10.068 min
Delta R.T.: -0.008 min
Response: 30980575
Conc: 15.19 ng/ml

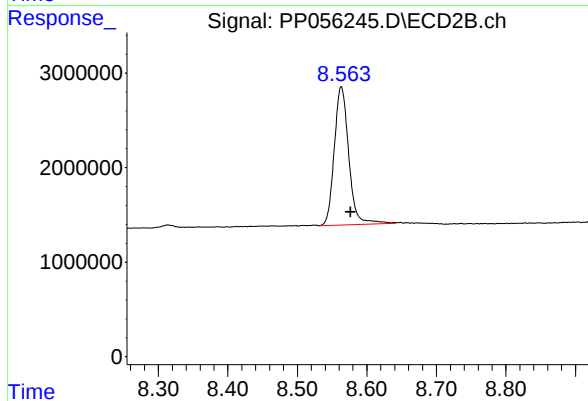

#2 Decachlorobiphenyl

R.T.: 8.563 min
Delta R.T.: -0.013 min
Response: 21174930
Conc: 18.66 ng/ml