

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030722\
 Data File : PP044291.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Mar 2022 15:57
 Operator : YP\AJ
 Sample : N1803-03 10X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 JEH7C3B-END-1-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 08 01:26:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 03 02:21:53 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.912	3.167	1805003	2447029	0.871m	1.399m#
2) SA Decachlor...	10.053	8.535	1662776	1955158	1.208	1.275

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030722\
Data File : PP044291.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Mar 2022 15:57
Operator : YP\AJ
Sample : N1803-03 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
JEH7C3B-END-1-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 08 01:26:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 03 02:21:53 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

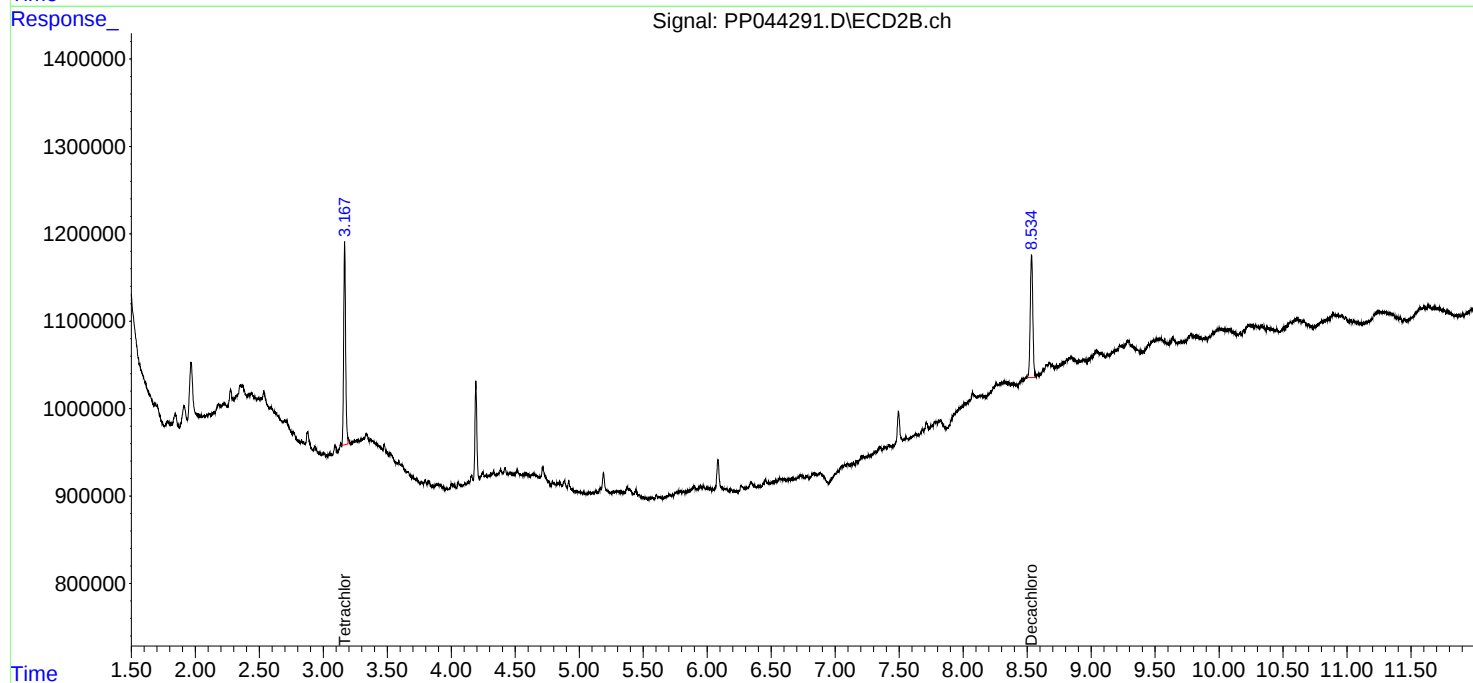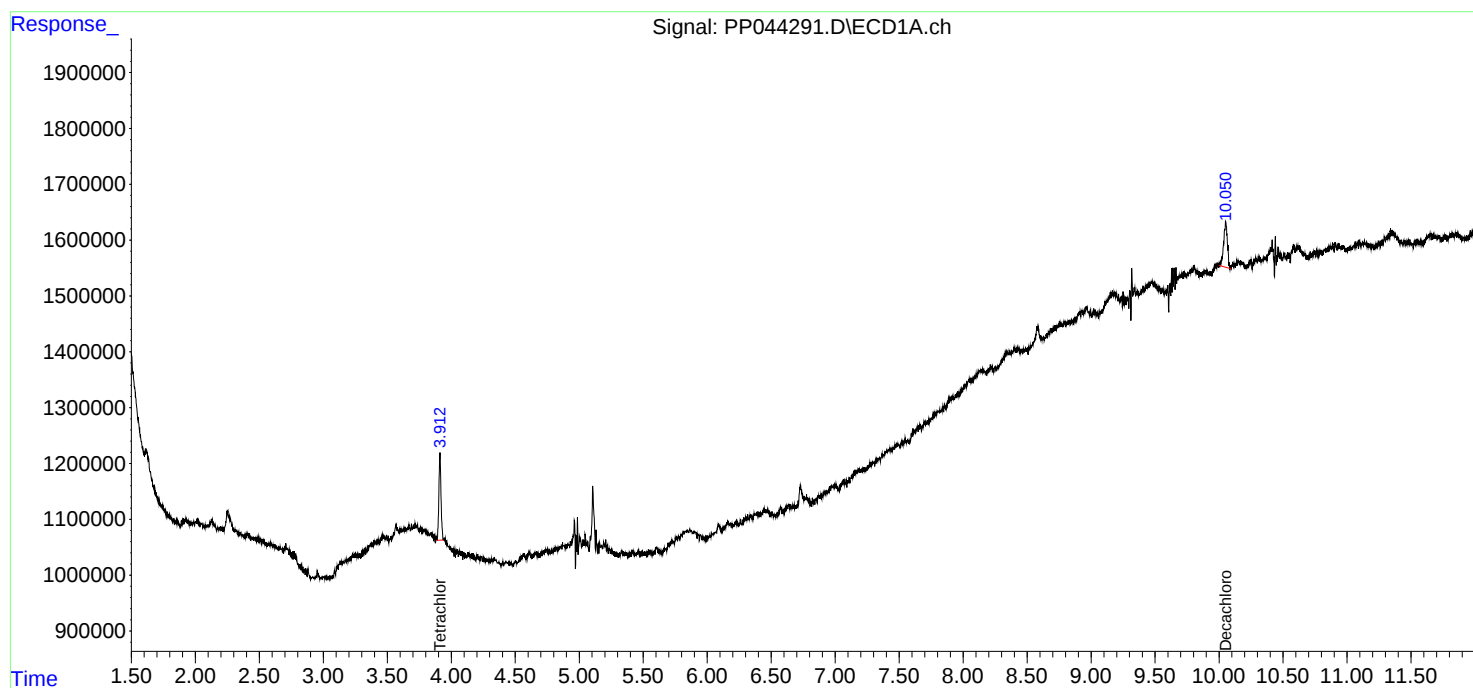


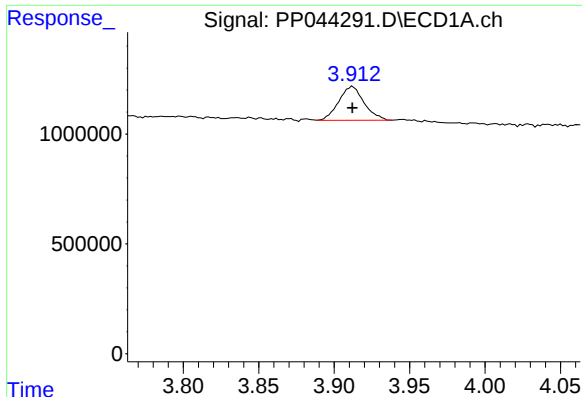

#1 Tetrachloro-m-xylene


R.T.: 3.912 min
Delta R.T.: 0.000 min
Response: 1805003
Conc: 0.87 ng/ml

Instrument :
ECD_P
ClientSampleId :
JEH7C3B-END-1-1

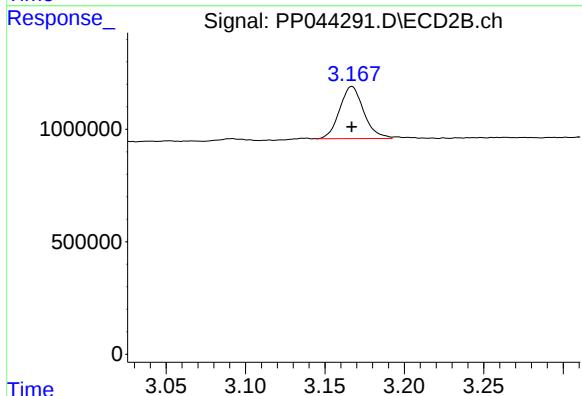


#1 Tetrachloro-m-xylene

R.T.: 3.167 min
Delta R.T.: 0.000 min
Response: 2447029
Conc: 1.40 ng/ml m

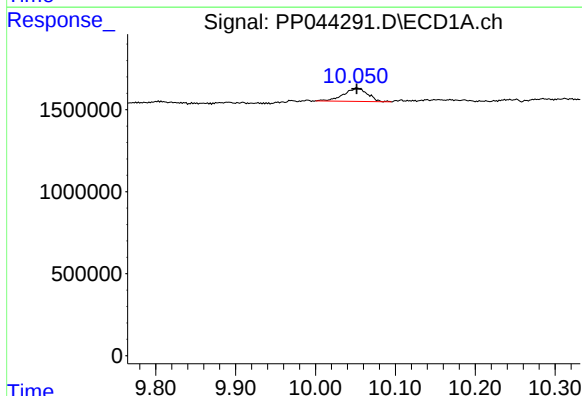

#2 Decachlorobiphenyl

R.T.: 10.053 min
Delta R.T.: 0.000 min
Response: 1662776
Conc: 1.21 ng/ml

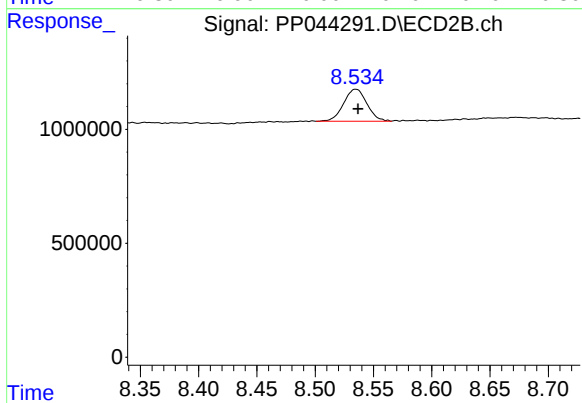

#2 Decachlorobiphenyl

R.T.: 8.535 min
Delta R.T.: -0.002 min
Response: 1955158
Conc: 1.27 ng/ml