

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030725\
 Data File : PP070380.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Mar 2025 22:09
 Operator : YP\AJ
 Sample : Q1516-02
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 GAS-AUD-25-0025

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/10/2025
 Supervised By :Ankita Jodhani 03/10/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 08 00:22:28 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 25 05:10:19 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.521	3.828	25154586	14942282	17.140m	15.629m
2) SA Decachlor...	10.263	8.896	17672547	15258676	15.515m	14.075

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030725\
Data File : PP070380.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Mar 2025 22:09
Operator : YP\AJ
Sample : Q1516-02
Misc :
ALS Vial : 32 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
GAS-AUD-25-0025


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/10/2025
Supervised By :Ankita Jodhani 03/10/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 08 00:22:28 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022425.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 25 05:10:19 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

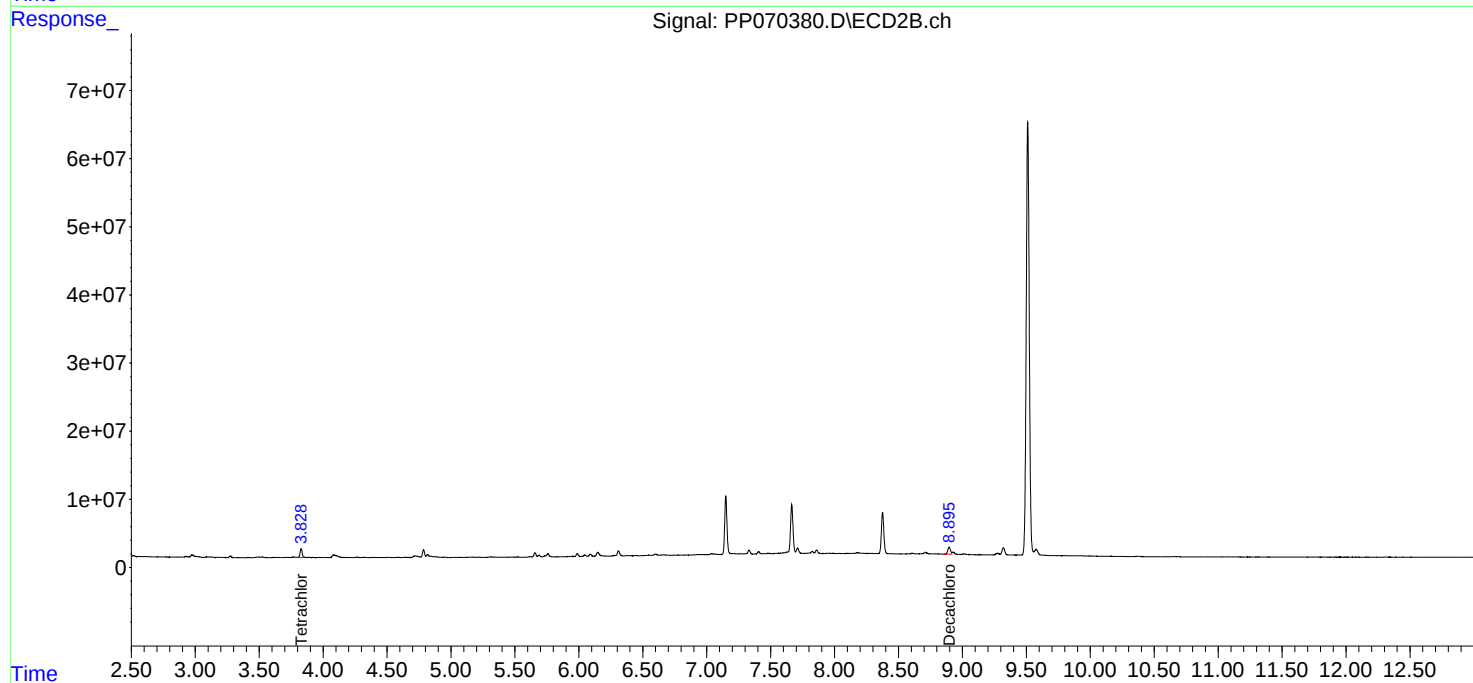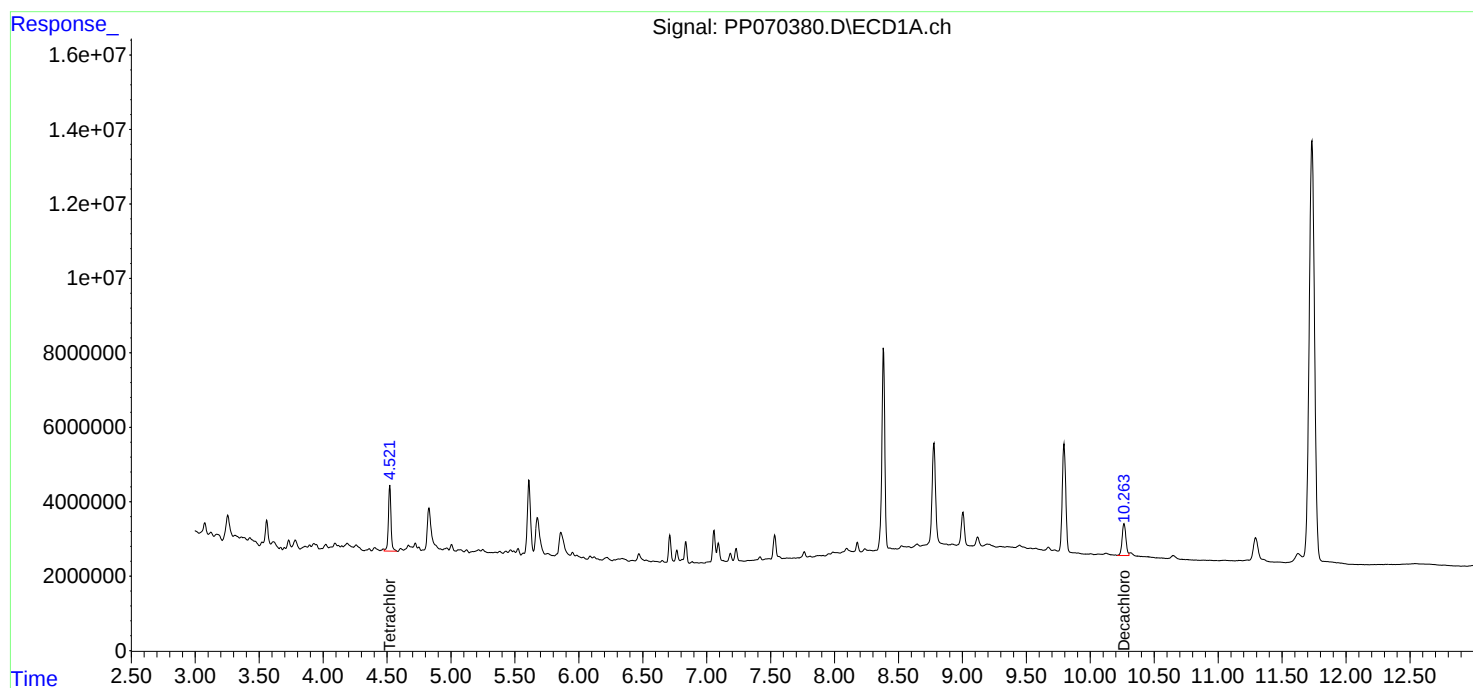

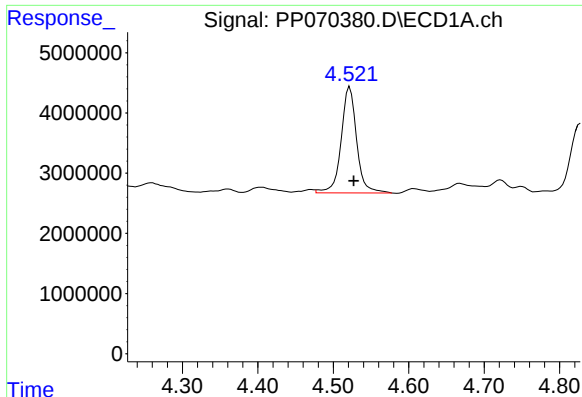


#1 Tetrachloro-m-xylene

R.T.: 4.521 min
Delta R.T.: -0.006 min
Response: 25154586
Conc: 17.14 ng/ml

Instrument :
ECD_P
ClientSampleId :
GAS-AUD-25-0025


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/10/2025
Supervised By :Ankita Jodhani 03/10/2025

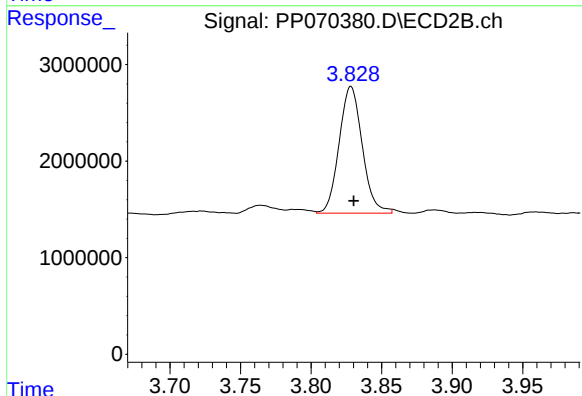


#1 Tetrachloro-m-xylene

R.T.: 3.828 min
Delta R.T.: -0.002 min
Response: 14942282
Conc: 15.63 ng/ml m

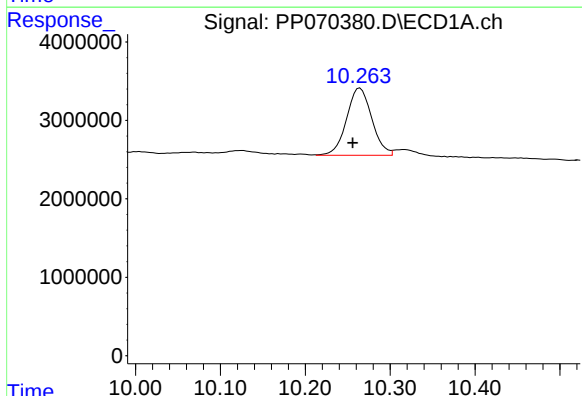

#2 Decachlorobiphenyl

R.T.: 10.263 min
Delta R.T.: 0.007 min
Response: 17672547
Conc: 15.52 ng/ml m

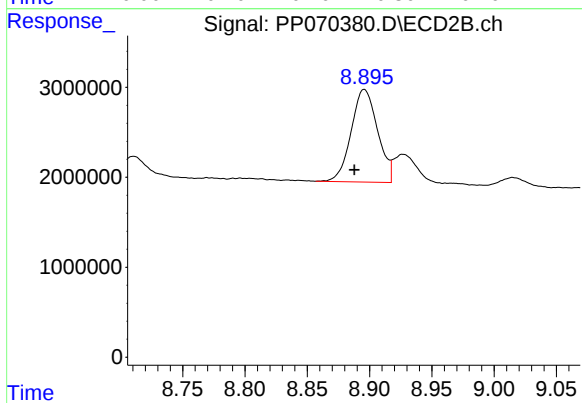

#2 Decachlorobiphenyl

R.T.: 8.896 min
Delta R.T.: 0.008 min
Response: 15258676
Conc: 14.07 ng/ml