

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030725\
 Data File : PP070383.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Mar 2025 22:58
 Operator : YP\AJ
 Sample : Q1510-02 10X
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 FMC-25-0006

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/10/2025
 Supervised By :Ankita Jodhani 03/10/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 08 00:23:28 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022425.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Feb 25 05:10:19 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.519	3.828	4218394	2001875	2.874m	2.094 #
2) SA Decachlor...	10.253	8.883	3416034	3576534	2.999	3.299

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030725\
Data File : PP070383.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Mar 2025 22:58
Operator : YP\AJ
Sample : Q1510-02 10X
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
FMC-25-0006


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/10/2025
Supervised By :Ankita Jodhani 03/10/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 08 00:23:28 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP022425.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Feb 25 05:10:19 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

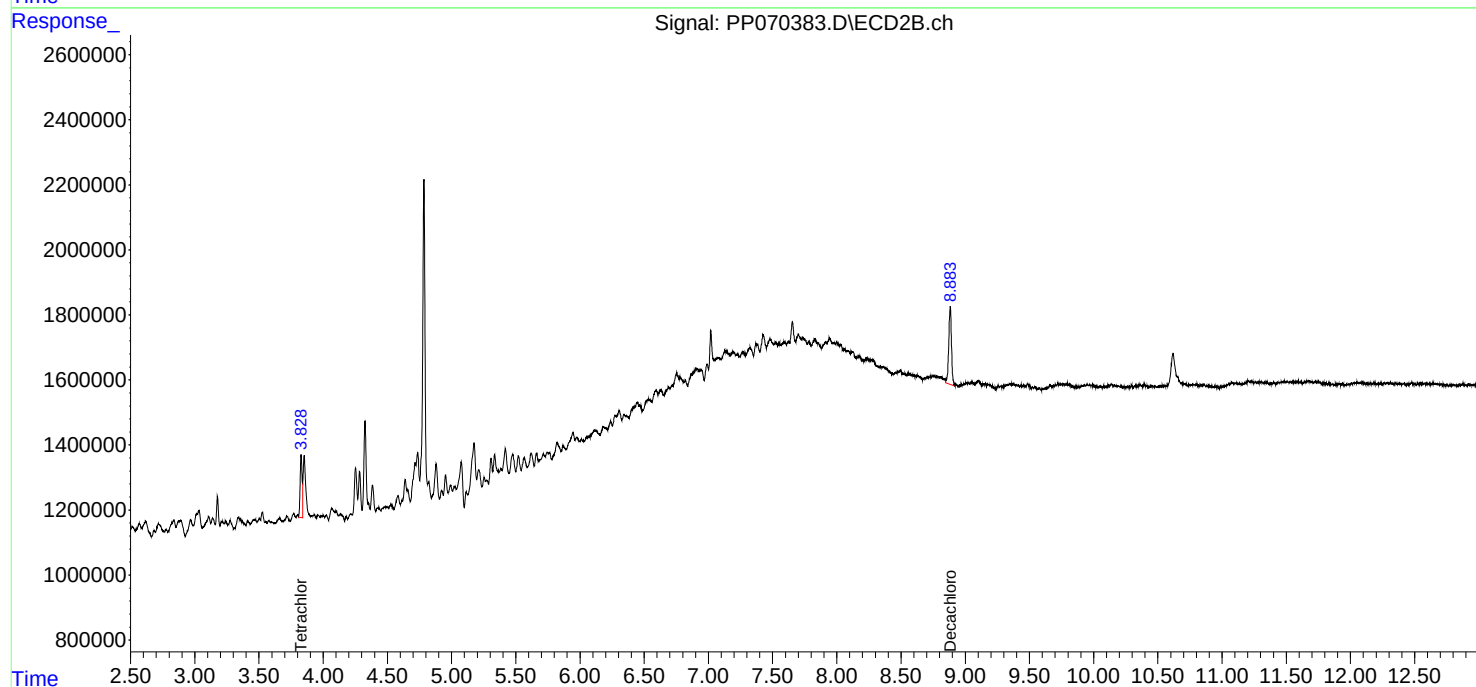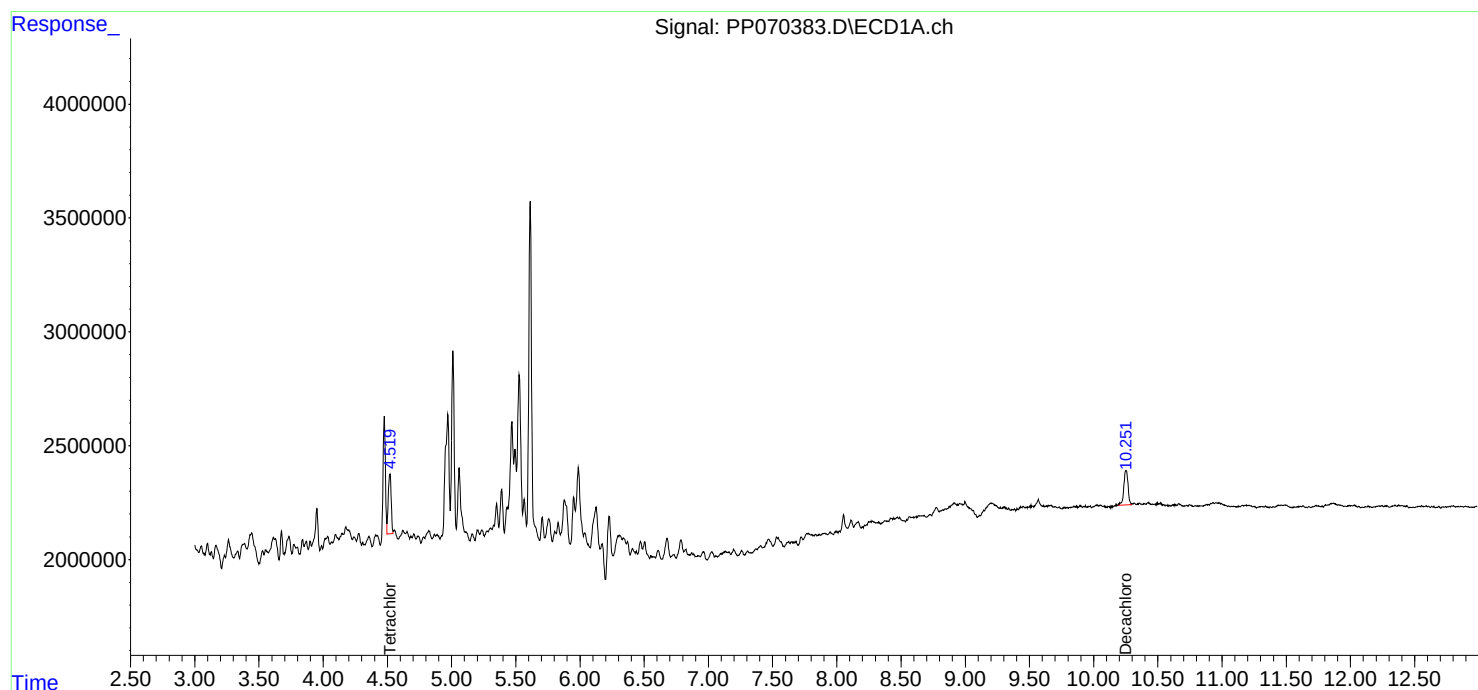

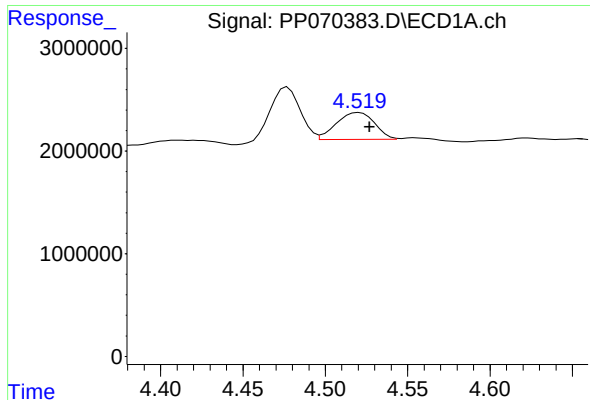


#1 Tetrachloro-m-xylene

R.T.: 4.519 min
Delta R.T.: -0.008 min
Response: 4218394
Conc: 2.87 ng/ml

Instrument :
ECD_P
ClientSampleId :
FMC-25-0006


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/10/2025
Supervised By :Ankita Jodhani 03/10/2025

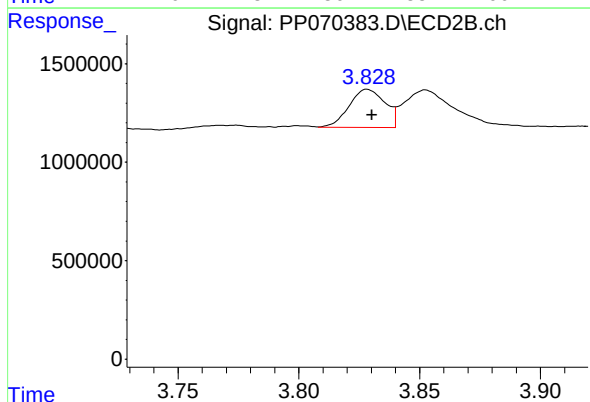


#1 Tetrachloro-m-xylene

R.T.: 3.828 min
Delta R.T.: -0.002 min
Response: 2001875
Conc: 2.09 ng/ml

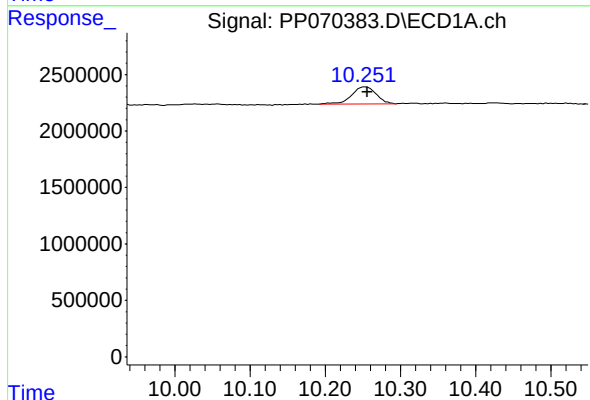

#2 Decachlorobiphenyl

R.T.: 10.253 min
Delta R.T.: -0.003 min
Response: 3416034
Conc: 3.00 ng/ml

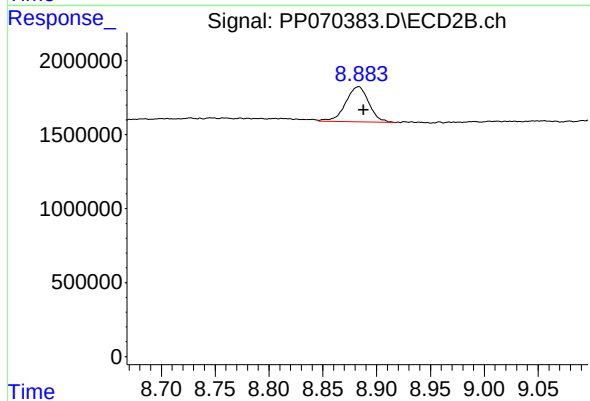

#2 Decachlorobiphenyl

R.T.: 8.883 min
Delta R.T.: -0.005 min
Response: 3576534
Conc: 3.30 ng/ml