

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030821\
 Data File : PP033730.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Mar 2021 14:58
 Operator : DD\AJ
 Sample : M1582-07
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 VEOLIA-72-11991

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 09 05:02:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 05 04:37:34 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.858	4.272	1707272	742970	14.863	18.661 #
2) SA Decachlor...	10.785	9.604	894454	274305	9.884	11.742

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030821\
Data File : PP033730.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Mar 2021 14:58
Operator : DD\AJ
Sample : M1582-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
VEOLIA-72-11991

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 09 05:02:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030421.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 05 04:37:34 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

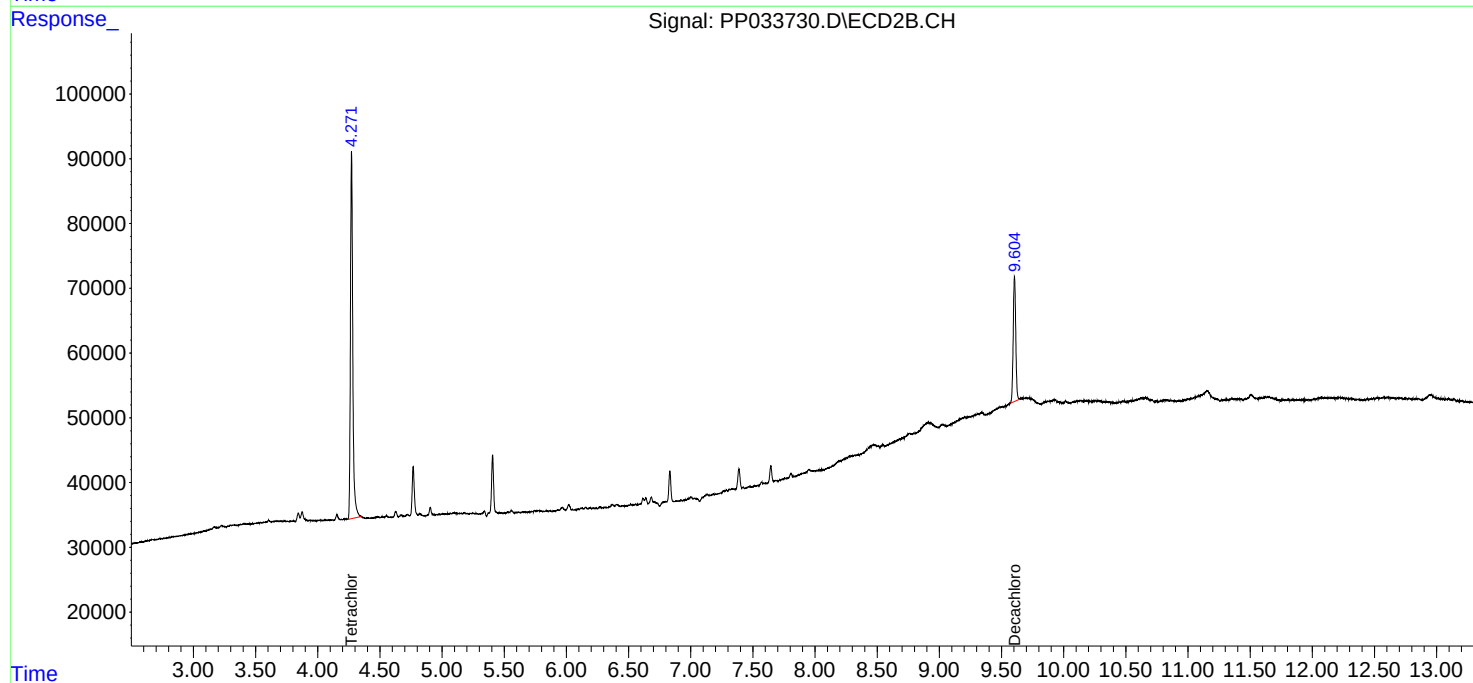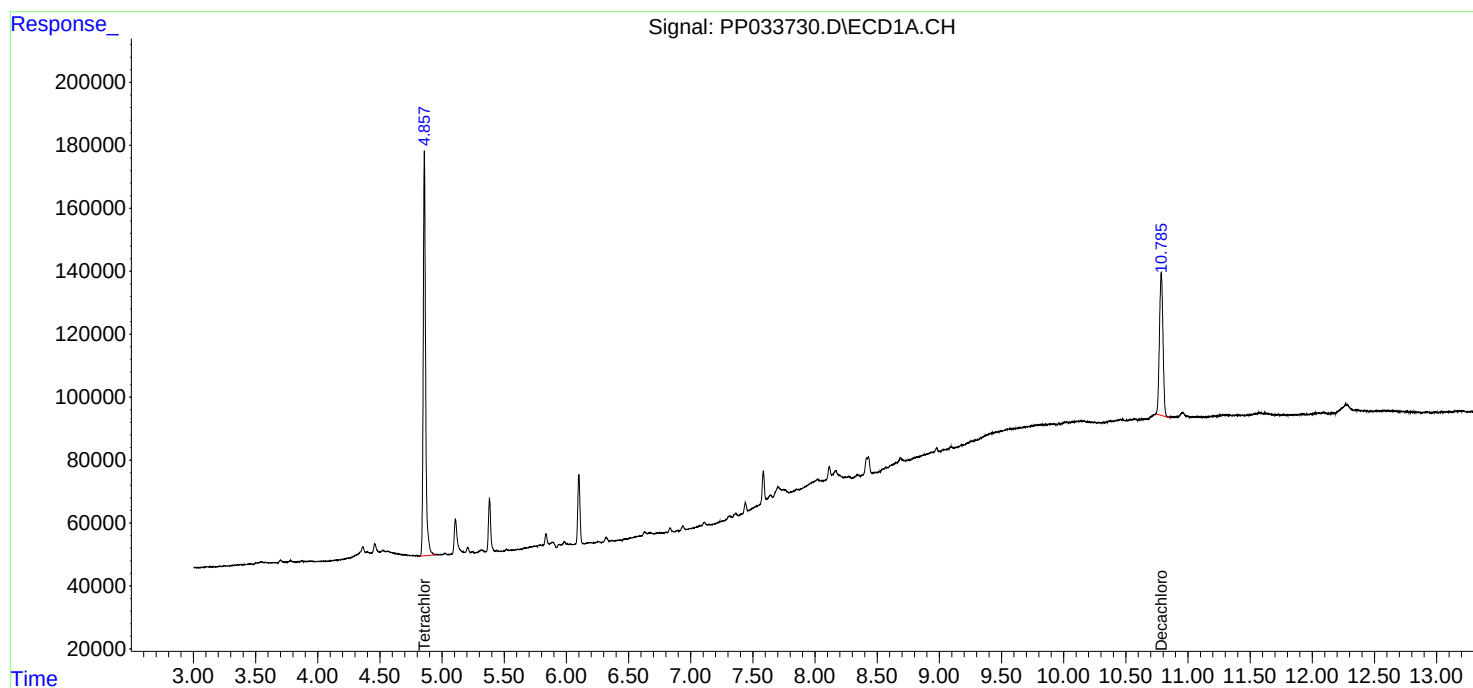


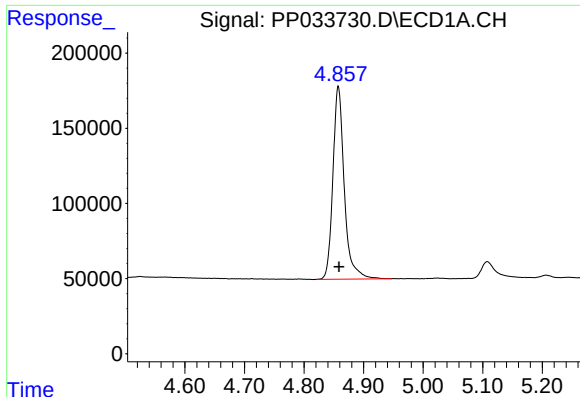

#1 Tetrachloro-m-xylene


R.T.: 4.858 min
Delta R.T.: -0.001 min
Response: 1707272
Conc: 14.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
VEOLIA-72-11991

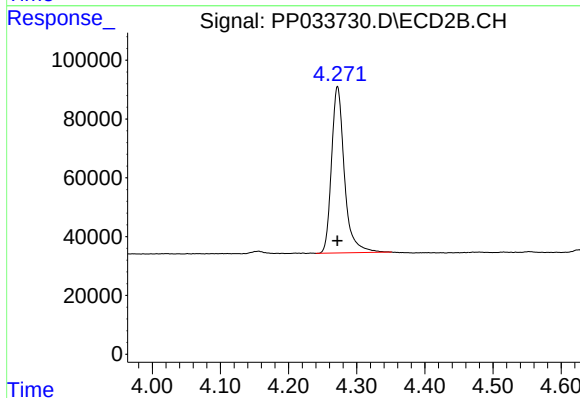


#1 Tetrachloro-m-xylene

R.T.: 4.272 min
Delta R.T.: 0.000 min
Response: 742970
Conc: 18.66 ng/ml

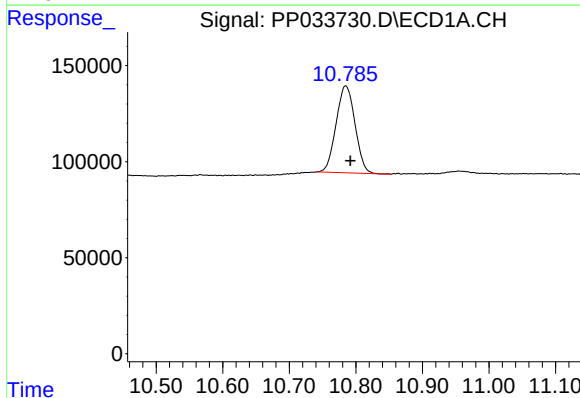

#2 Decachlorobiphenyl

R.T.: 10.785 min
Delta R.T.: -0.007 min
Response: 894454
Conc: 9.88 ng/ml

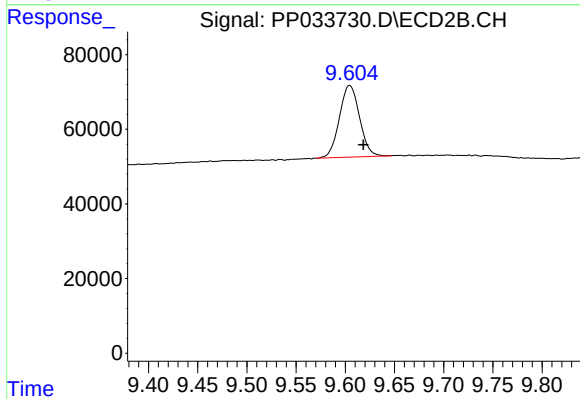

#2 Decachlorobiphenyl

R.T.: 9.604 min
Delta R.T.: -0.014 min
Response: 274305
Conc: 11.74 ng/ml