

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030821\
 Data File : PP033732.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Mar 2021 15:32
 Operator : DD\AJ
 Sample : M1577-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 72-11939-VNJ-229

Manual Integrations
 APPROVED

Ankita
 3/9/2021 1:05:30 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 09 04:09:38 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Mar 05 04:37:34 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.859	4.273	1835918	843140	15.983	21.177 #
2) SA Decachlor...	10.785	9.606	1765260	569147	19.507	24.363
Target Compounds						
26) L6 AR-1254-1	7.076	6.402	47918	37232	13.774	23.658m#
27) L6 AR-1254-2	7.307	6.561	242756	35667	46.121	26.034m#
28) L6 AR-1254-3	7.695	6.981	283761	54516	50.844m	25.426m#
29) L6 AR-1254-4	7.981	7.217	119335	40149	31.104m	36.335m
30) L6 AR-1254-5	8.407	7.645	136180	60378	32.483m	35.240m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030821\
Data File : PP033732.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Mar 2021 15:32
Operator : DD\AJ
Sample : M1577-01
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
72-11939-VNJ-229


Manual Integrations
APPROVED

Ankita
3/9/2021 1:05:30 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 09 04:09:38 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030421.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Mar 05 04:37:34 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

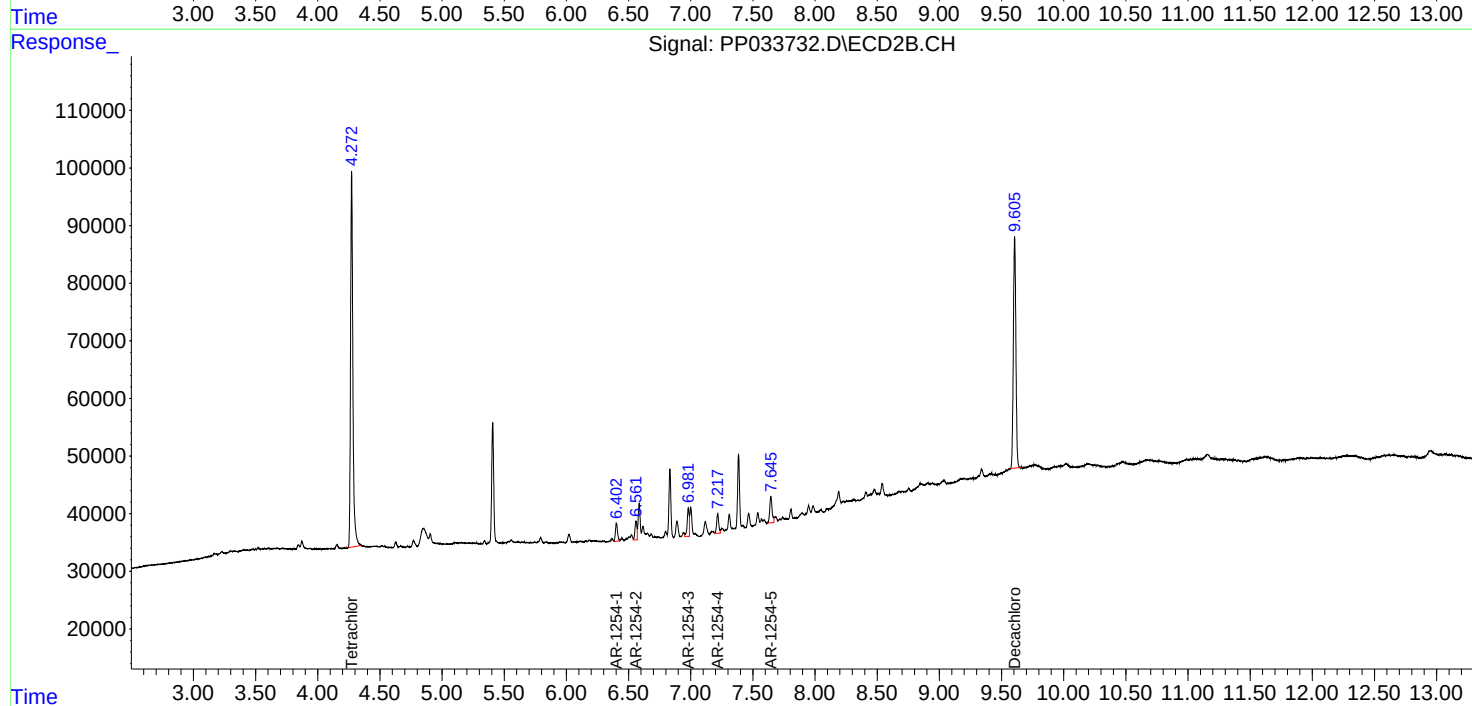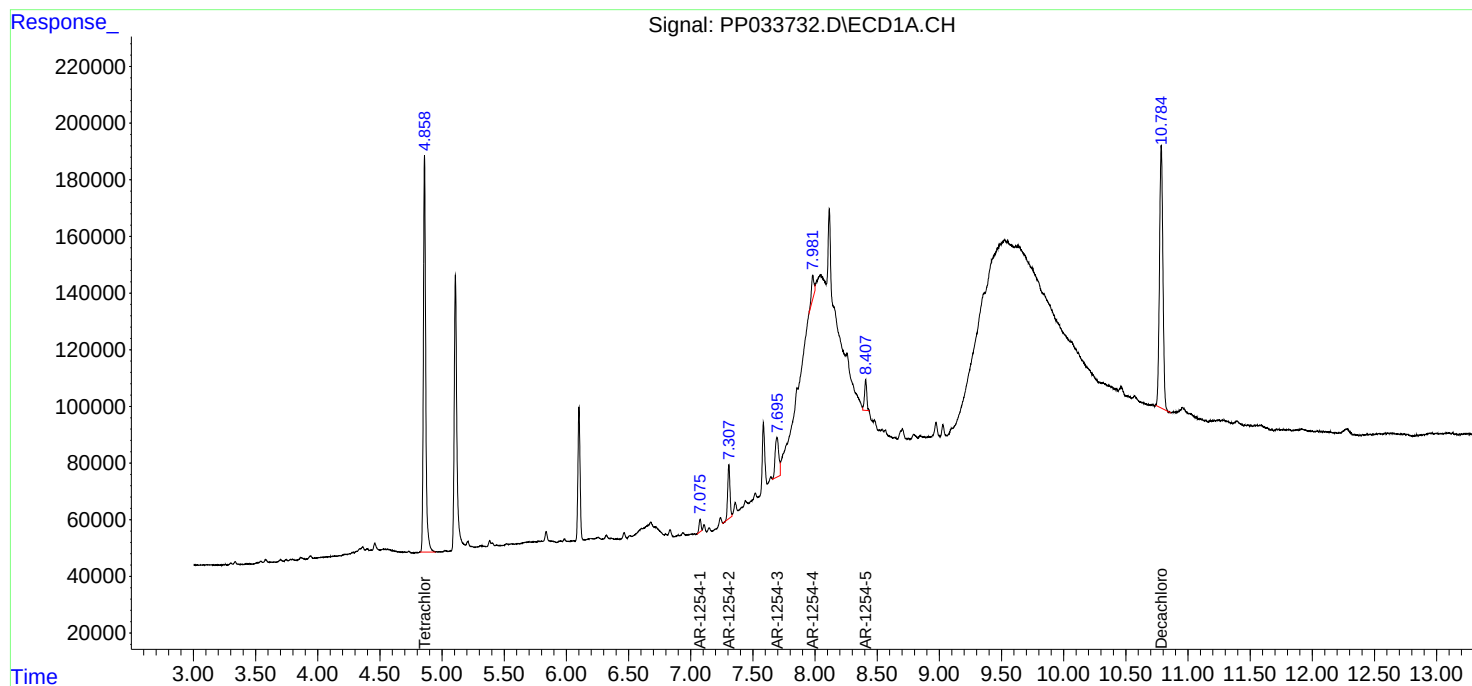

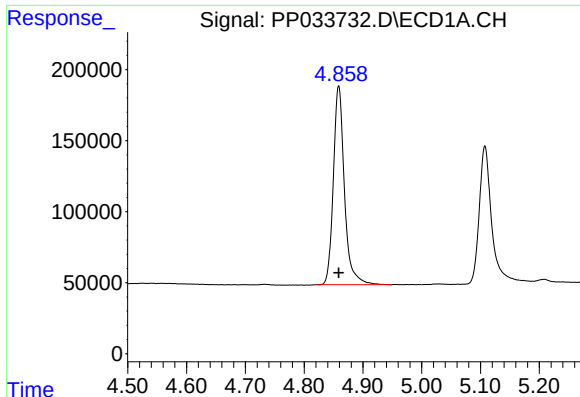


#1 Tetrachloro-m-xylene

R.T.: 4.859 min
Delta R.T.: 0.000 min
Response: 1835918
Conc: 15.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
72-11939-VNJ-229


Manual Integrations
APPROVED

Ankita
3/9/2021 1:05:30 PM

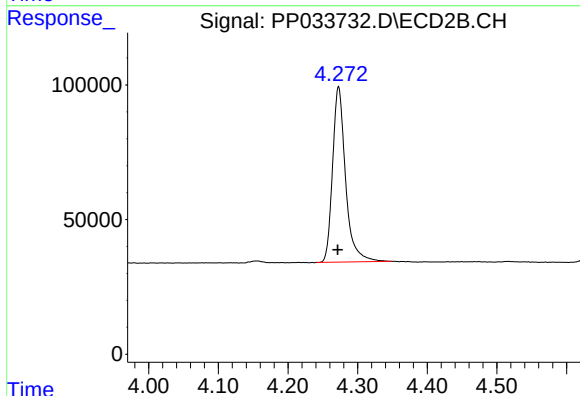


#1 Tetrachloro-m-xylene

R.T.: 4.273 min
Delta R.T.: 0.001 min
Response: 843140
Conc: 21.18 ng/ml

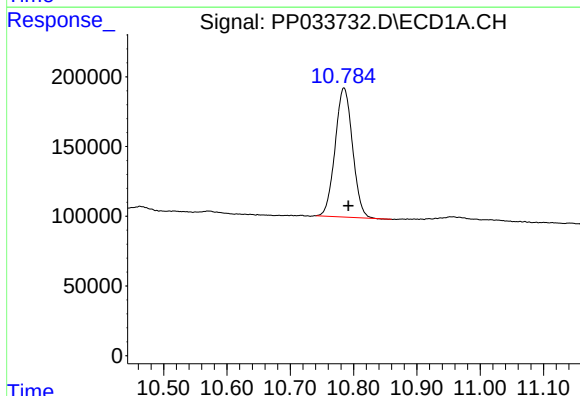


#2 Decachlorobiphenyl

R.T.: 10.785 min
Delta R.T.: -0.007 min
Response: 1765260
Conc: 19.51 ng/ml

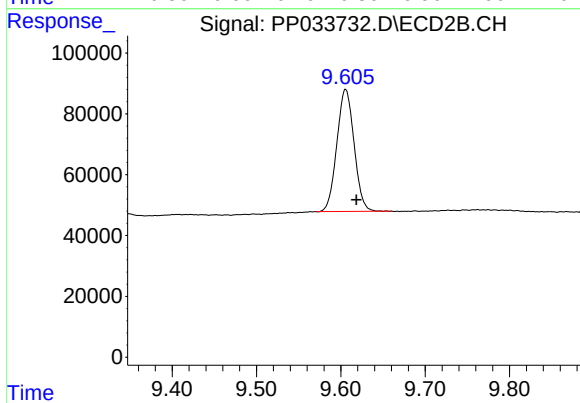

#2 Decachlorobiphenyl

R.T.: 9.606 min
Delta R.T.: -0.013 min
Response: 569147
Conc: 24.36 ng/ml

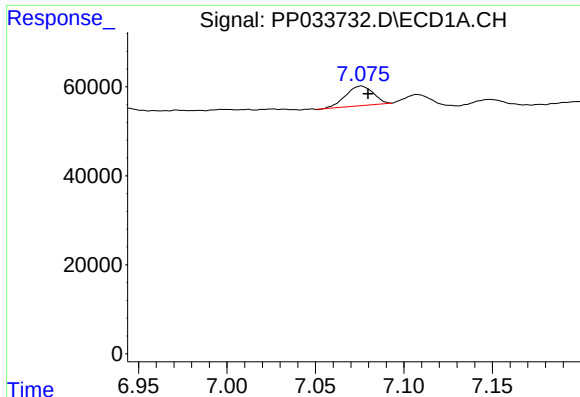

#26 AR-1254-1

R.T.: 7.076 min
Delta R.T.: -0.004 min
Response: 47918
Conc: 13.77 ng/ml

Instrument :
ECD_P
ClientSampleId :
72-11939-VNJ-229

Manual Integrations
APPROVED

Ankita
3/9/2021 1:05:30 PM

#26 AR-1254-1


R.T.: 6.402 min
Delta R.T.: -0.004 min
Response: 37232
Conc: 23.66 ng/ml m

#27 AR-1254-2

R.T.: 7.307 min
Delta R.T.: -0.001 min
Response: 242756
Conc: 46.12 ng/ml

#27 AR-1254-2

R.T.: 6.561 min
Delta R.T.: -0.003 min
Response: 35667
Conc: 26.03 ng/ml m

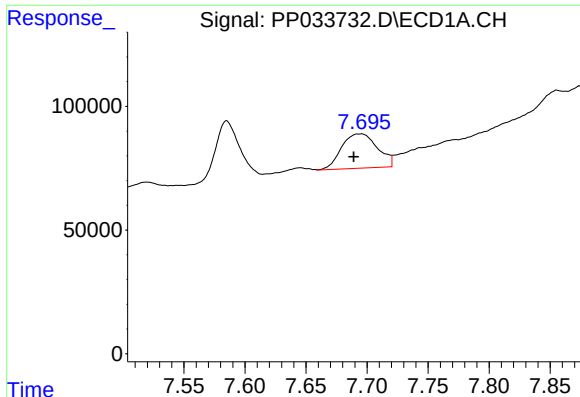


#28 AR-1254-3

R.T.: 7.695 min
Delta R.T.: 0.006 min
Response: 283761
Conc: 50.84 ng/ml m

Instrument :
ECD_P
ClientSampleId :
72-11939-VNJ-229


Manual Integrations
APPROVED

Ankita
3/9/2021 1:05:30 PM

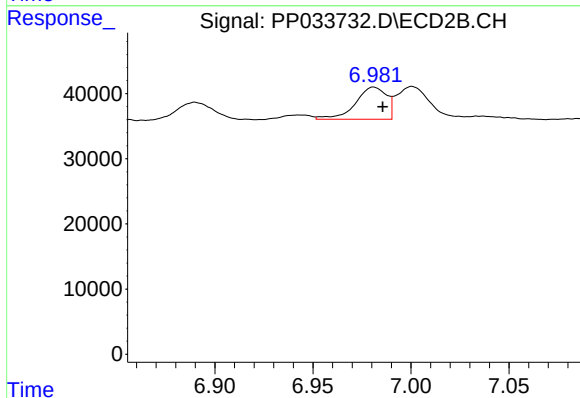


#28 AR-1254-3

R.T.: 6.981 min
Delta R.T.: -0.005 min
Response: 54516
Conc: 25.43 ng/ml m

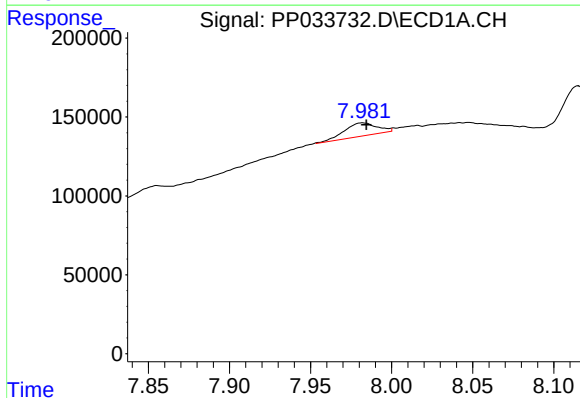


#29 AR-1254-4

R.T.: 7.981 min
Delta R.T.: -0.003 min
Response: 119335
Conc: 31.10 ng/ml m

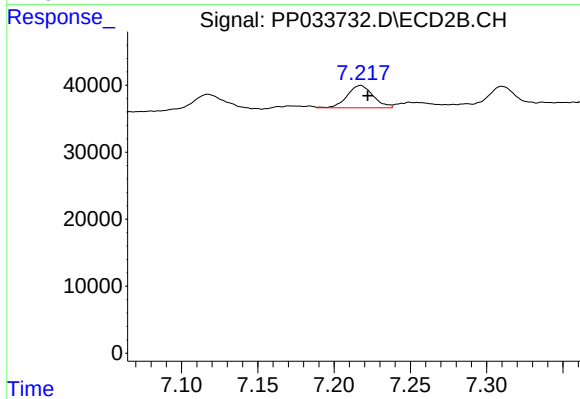

#29 AR-1254-4

R.T.: 7.217 min
Delta R.T.: -0.005 min
Response: 40149
Conc: 36.34 ng/ml m

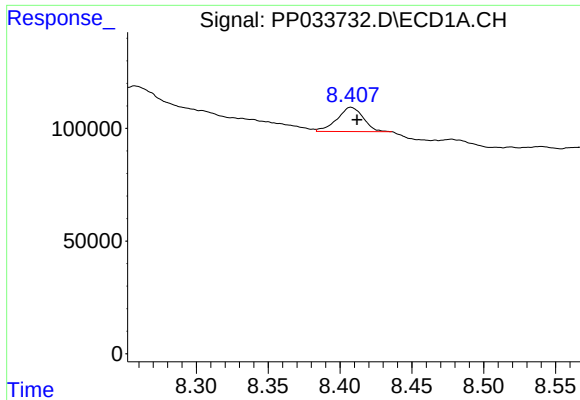


#30 AR-1254-5

R.T.: 8.407 min
Delta R.T.: -0.005 min
Response: 136180
Conc: 32.48 ng/ml m

Instrument :
ECD_P
ClientSampleId :
72-11939-VNJ-229

Manual Integrations
APPROVED

Ankita
3/9/2021 1:05:30 PM

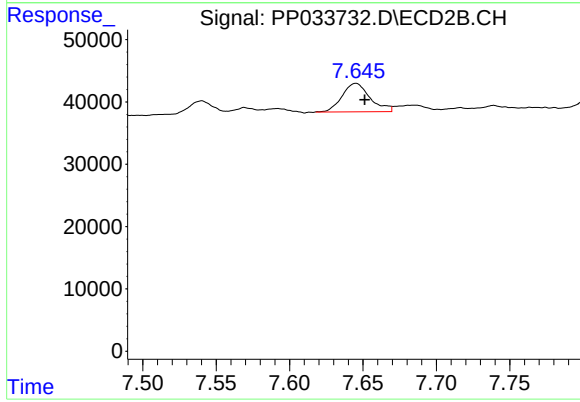

#30 AR-1254-5

R.T.: 7.645 min
Delta R.T.: -0.006 min
Response: 60378
Conc: 35.24 ng/ml m