

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030822\
 Data File : PP044369.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Mar 2022 05:33
 Operator : YP\AJ
 Sample : N1827-03 10X
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CLI-2022-24A

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/09/2022
 Supervised By :Ankita Jodhani 03/09/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 09 07:58:30 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 03 02:21:53 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.912	3.166	3588433	4277264	1.732m	2.445 #
2) SA Decachlor...	10.051	8.536	3392276	3484552	2.465	2.272
Target Compounds						
26) L6 AR-1254-1	6.090	5.164	80577751	108.9E6	1074.399	1317.241
27) L6 AR-1254-2	6.330	5.325	161.5E6	115.6E6	1437.226	1607.610
28) L6 AR-1254-3	6.729	5.756	227.2E6	242.6E6	1941.898	2105.510
29) L6 AR-1254-4	7.044	6.007	190.7E6	184.1E6	2372.276	2444.903
30) L6 AR-1254-5	7.505	6.458	262.0E6	321.7E6	3009.610	2952.191

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030822\
Data File : PP044369.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Mar 2022 05:33
Operator : YP\AJ
Sample : N1827-03 10X
Misc :
ALS Vial : 41 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
CLI-2022-24A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/09/2022
Supervised By :Ankita Jodhani 03/09/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 09 07:58:30 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 03 02:21:53 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

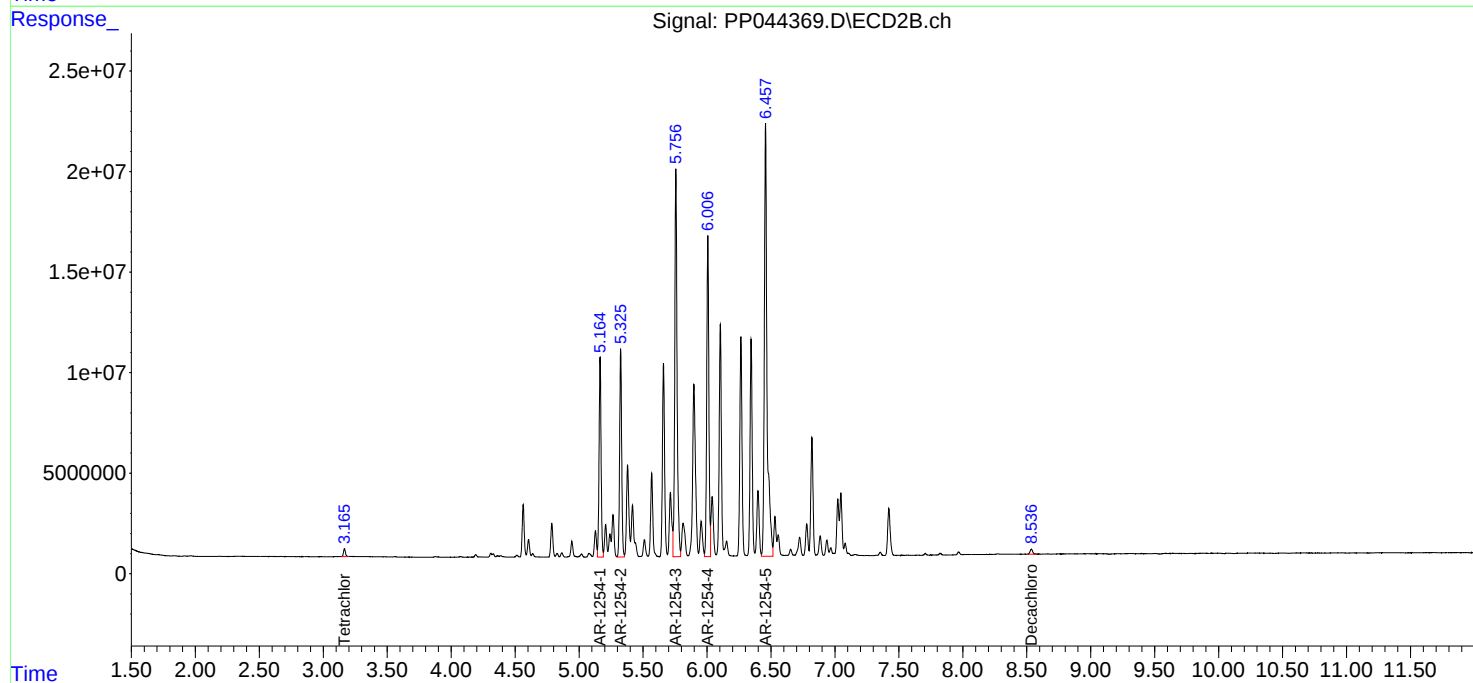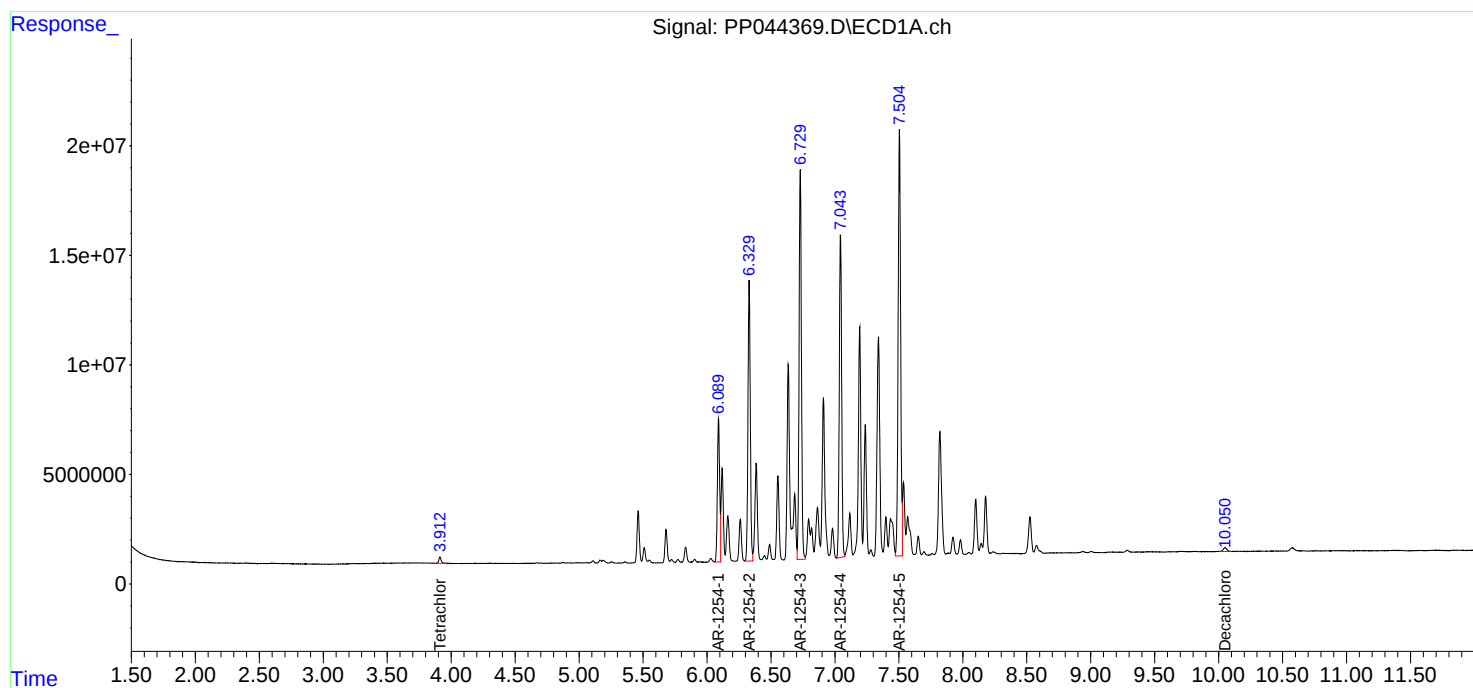

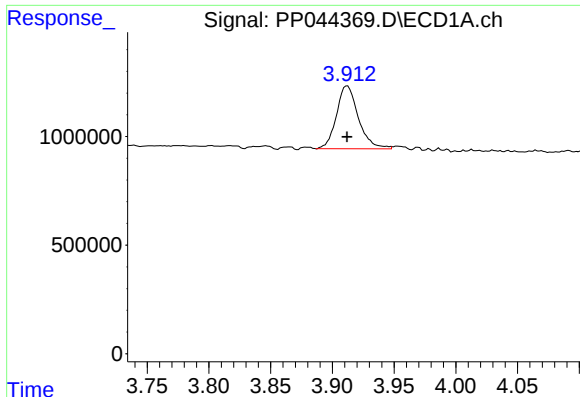


#1 Tetrachloro-m-xylene

R.T.: 3.912 min
Delta R.T.: 0.000 min
Response: 3588433
Conc: 1.73 ng/ml

Instrument :
ECD_P
ClientSampleId :
CLI-2022-24A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/09/2022
Supervised By :Ankita Jodhani 03/09/2022

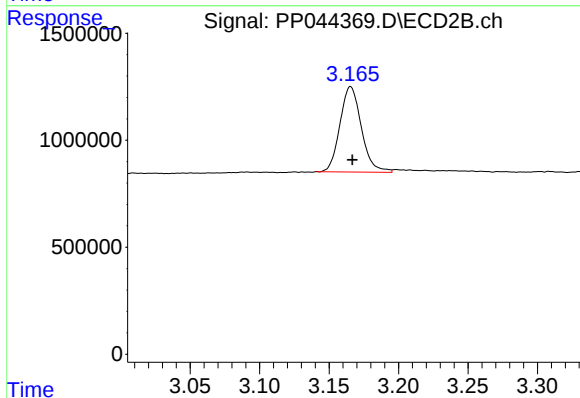


#1 Tetrachloro-m-xylene

R.T.: 3.166 min
Delta R.T.: -0.001 min
Response: 4277264
Conc: 2.44 ng/ml

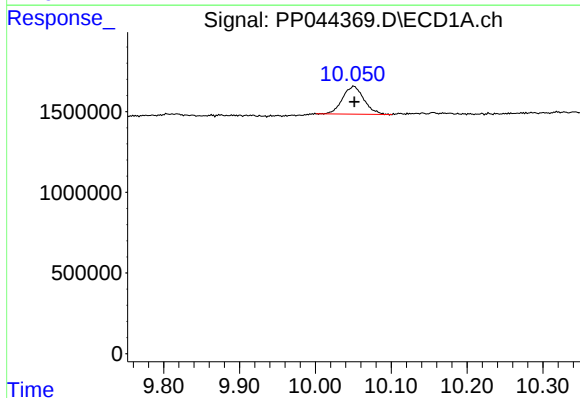


#2 Decachlorobiphenyl

R.T.: 10.051 min
Delta R.T.: 0.000 min
Response: 3392276
Conc: 2.46 ng/ml

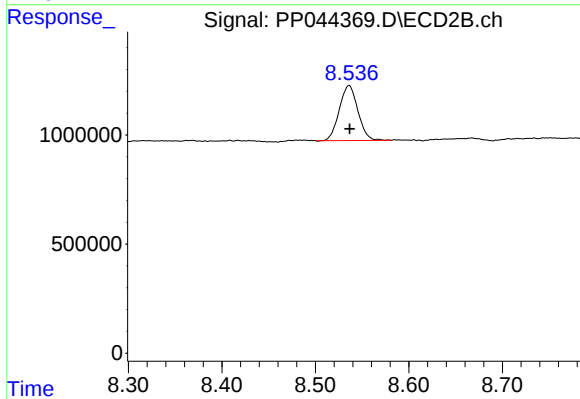

#2 Decachlorobiphenyl

R.T.: 8.536 min
Delta R.T.: 0.000 min
Response: 3484552
Conc: 2.27 ng/ml

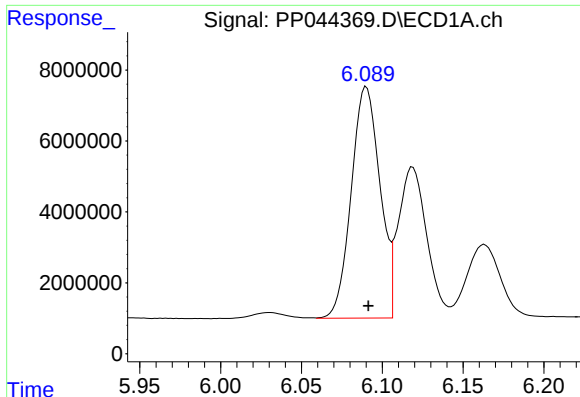


#26 AR-1254-1

R.T.: 6.090 min
Delta R.T.: -0.001 min
Response: 80577751
Conc: 1074.40 ng/ml

Instrument :
ECD_P
ClientSampleId :
CLI-2022-24A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/09/2022
Supervised By :Ankita Jodhani 03/09/2022

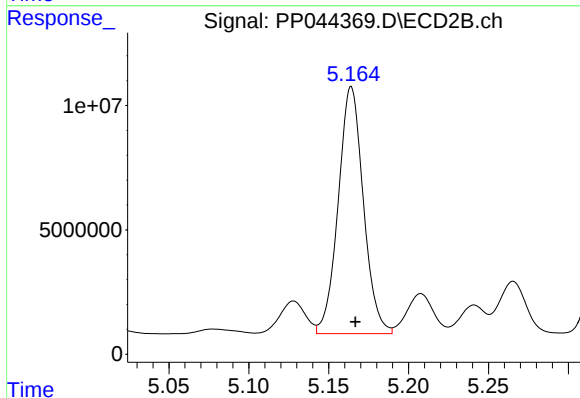


#26 AR-1254-1

R.T.: 5.164 min
Delta R.T.: -0.003 min
Response: 108901017
Conc: 1317.24 ng/ml

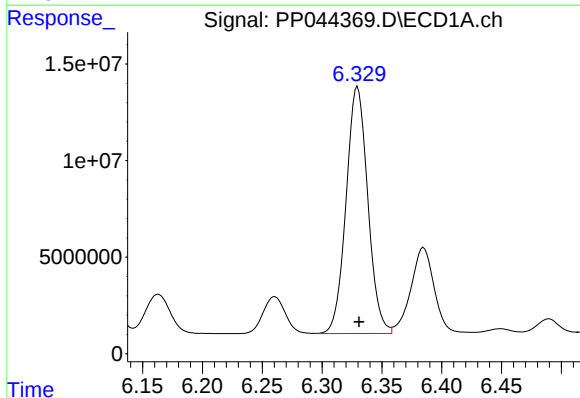


#27 AR-1254-2

R.T.: 6.330 min
Delta R.T.: -0.001 min
Response: 161492192
Conc: 1437.23 ng/ml

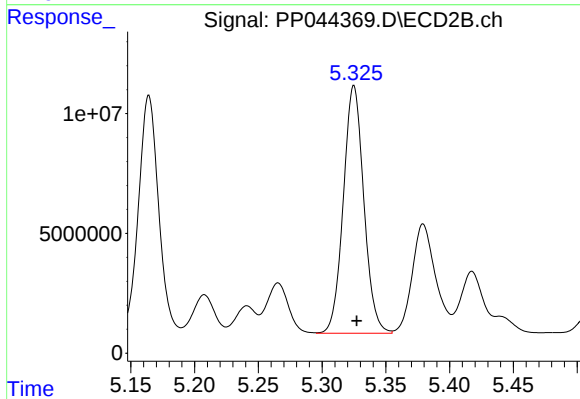

#27 AR-1254-2

R.T.: 5.325 min
Delta R.T.: -0.002 min
Response: 115649311
Conc: 1607.61 ng/ml

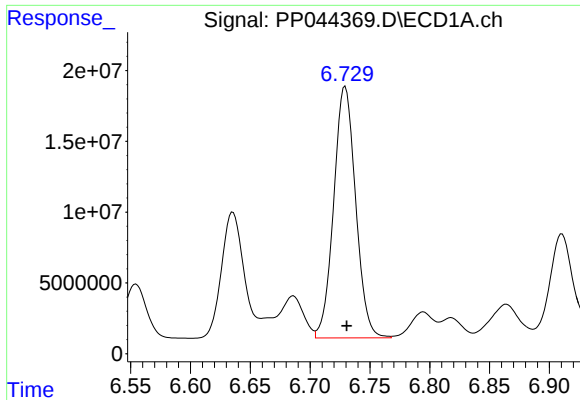


#28 AR-1254-3

R.T.: 6.729 min
Delta R.T.: -0.001 min
Response: 227233704
Conc: 1941.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
CLI-2022-24A


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/09/2022
Supervised By :Ankita Jodhani 03/09/2022

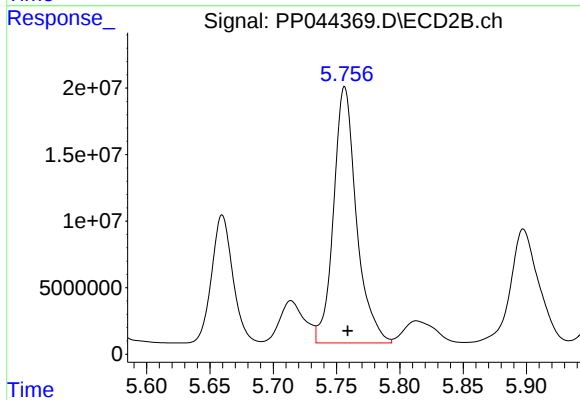


#28 AR-1254-3

R.T.: 5.756 min
Delta R.T.: -0.002 min
Response: 242581308
Conc: 2105.51 ng/ml

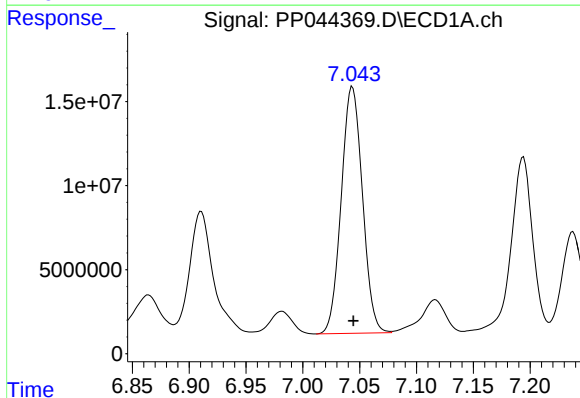


#29 AR-1254-4

R.T.: 7.044 min
Delta R.T.: 0.000 min
Response: 190733647
Conc: 2372.28 ng/ml

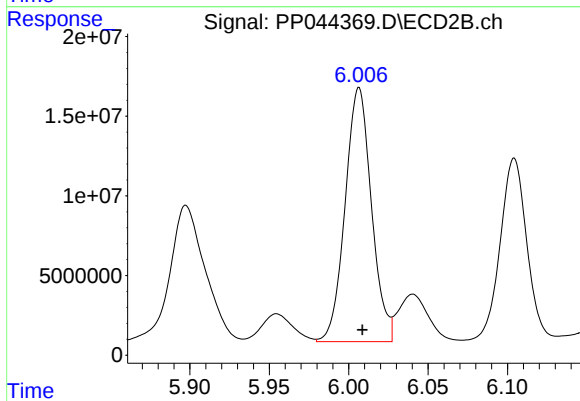

#29 AR-1254-4

R.T.: 6.007 min
Delta R.T.: -0.002 min
Response: 184060084
Conc: 2444.90 ng/ml

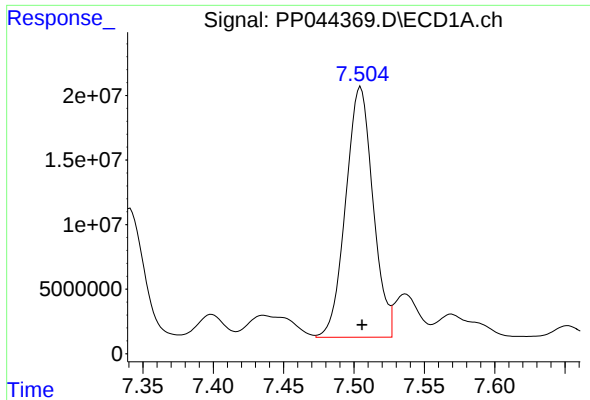


#30 AR-1254-5

R.T.: 7.505 min
Delta R.T.: -0.001 min
Response: 261972844
Conc: 3009.61 ng/ml

Instrument :
ECD_P
ClientSampleId :
CLI-2022-24A

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/09/2022
Supervised By :Ankita Jodhani 03/09/2022

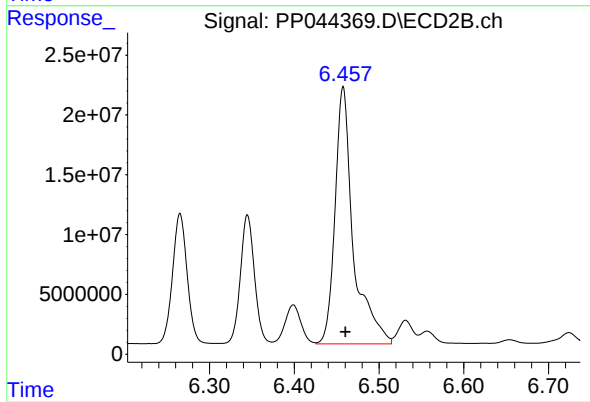

#30 AR-1254-5

R.T.: 6.458 min
Delta R.T.: -0.003 min
Response: 321731214
Conc: 2952.19 ng/ml