

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030921\
 Data File : PP033788.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Mar 2021 3:48
 Operator : DD\AJ
 Sample : M1458-07
 Misc : AR1221 LOD 40 PPB
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 10 06:00:26 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 10 03:01:34 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.857	4.270	1462556	693175	16.903	17.062
2) SA Decachlor...	10.782	9.598	1503087	493440	17.798	18.491
Target Compounds						
8) L2 AR-1221-1	5.108	4.528	59727	16256	64.724	38.177 #
9) L2 AR-1221-2	5.204	4.626	42665	18754	60.718	57.959
10) L2 AR-1221-3	5.290	4.716	109295	39431	51.926	40.227



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030921\
Data File : PP033788.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Mar 2021 3:48
Operator : DD\AJ
Sample : M1458-07
Misc : AR1221 LOD 40 PPB
ALS Vial : 44 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 10 06:00:26 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 10 03:01:34 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

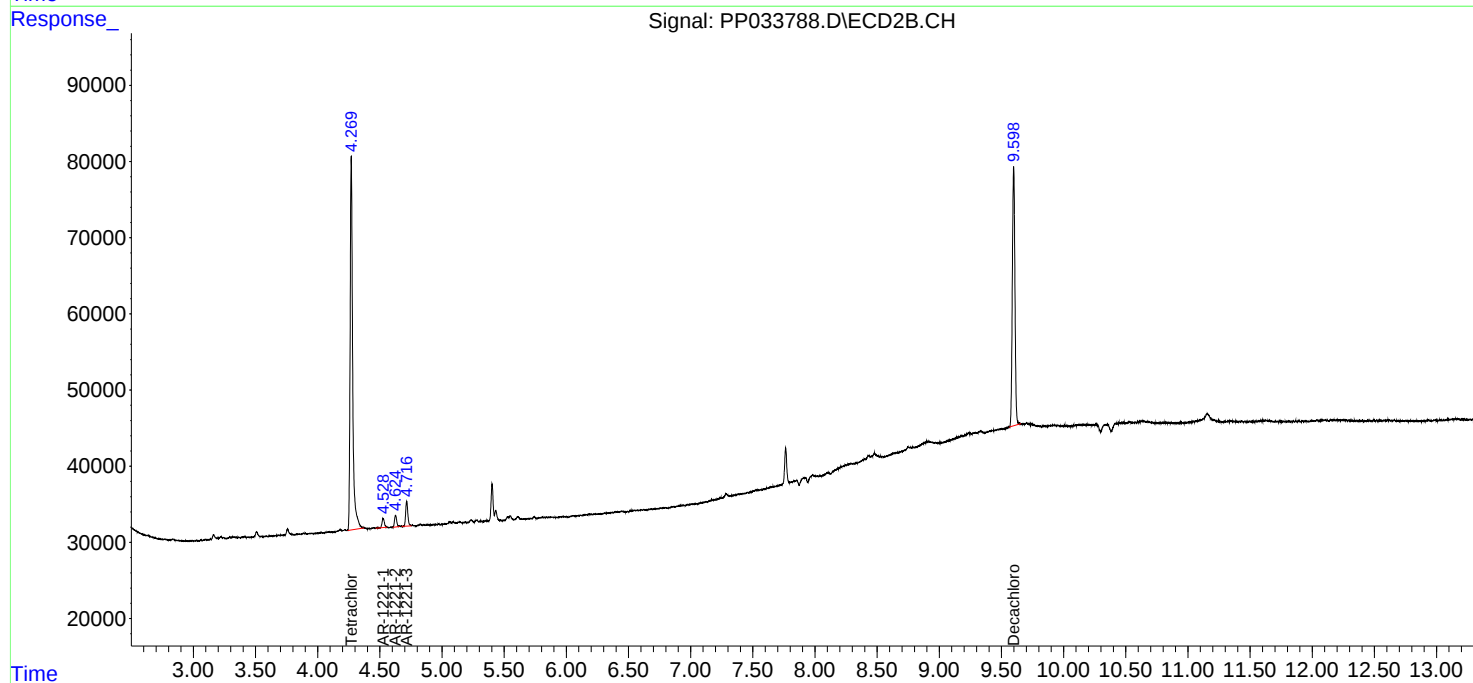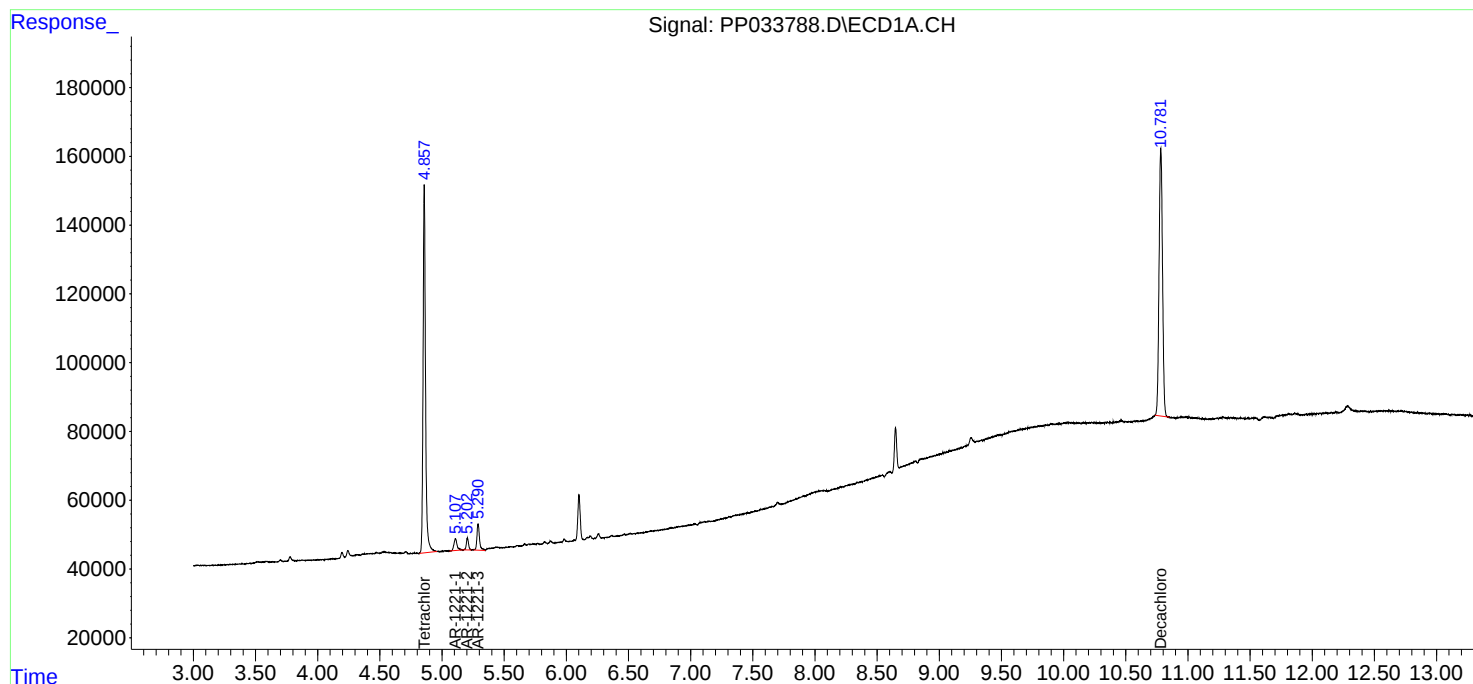


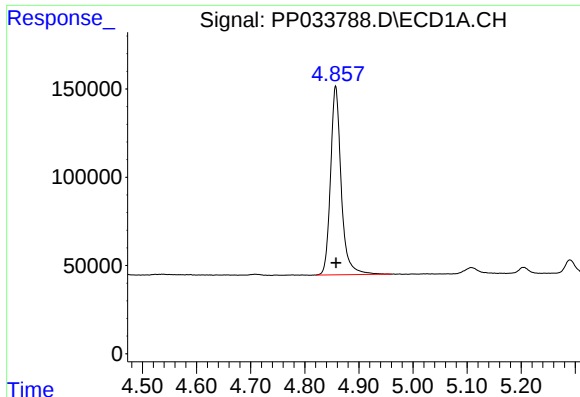

#1 Tetrachloro-m-xylene


R.T.: 4.857 min
Delta R.T.: 0.000 min
Response: 1462556
Conc: 16.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

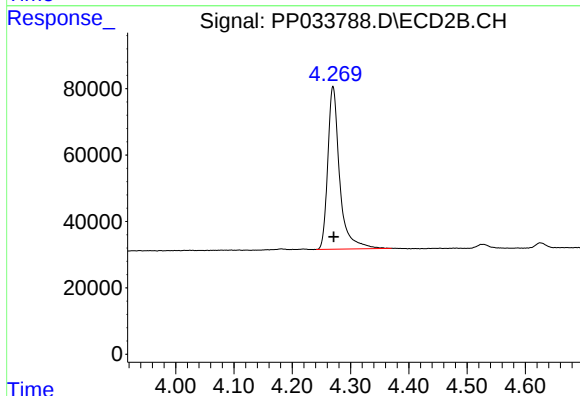


#1 Tetrachloro-m-xylene

R.T.: 4.270 min
Delta R.T.: -0.001 min
Response: 693175
Conc: 17.06 ng/ml

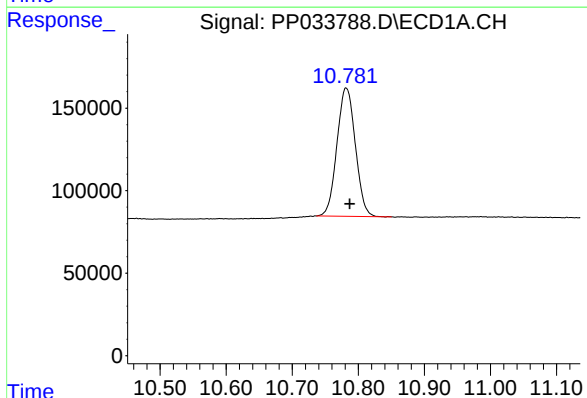


#2 Decachlorobiphenyl

R.T.: 10.782 min
Delta R.T.: -0.006 min
Response: 1503087
Conc: 17.80 ng/ml

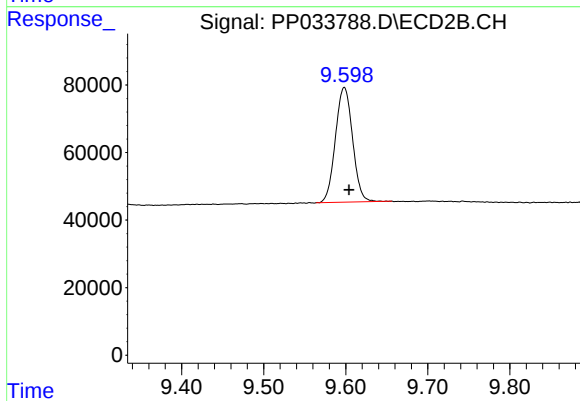

#2 Decachlorobiphenyl


R.T.: 9.598 min
Delta R.T.: -0.006 min
Response: 493440
Conc: 18.49 ng/ml

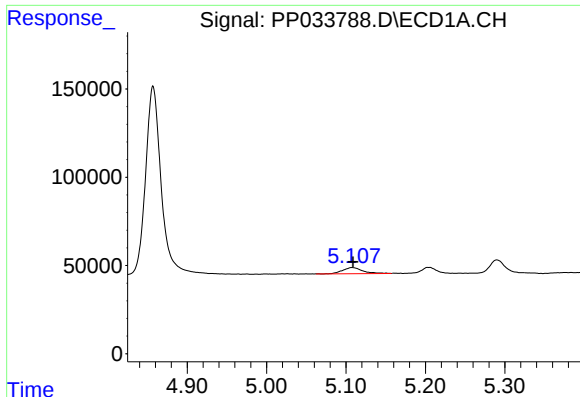

#8 AR-1221-1


R.T.: 5.108 min
Delta R.T.: -0.001 min
Response: 59727
Conc: 64.72 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

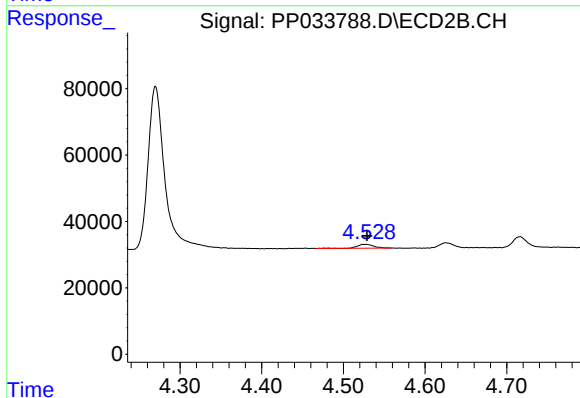


#8 AR-1221-1

R.T.: 4.528 min
Delta R.T.: 0.000 min
Response: 16256
Conc: 38.18 ng/ml

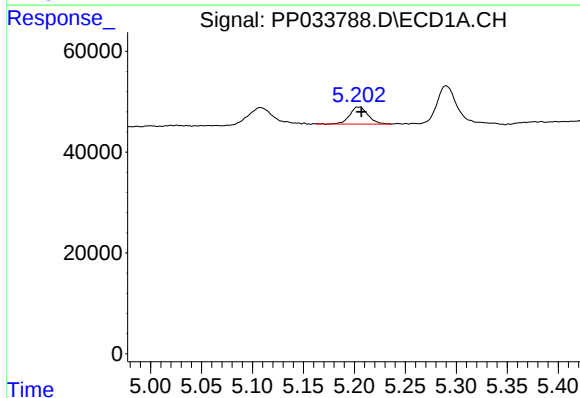


#9 AR-1221-2

R.T.: 5.204 min
Delta R.T.: -0.003 min
Response: 42665
Conc: 60.72 ng/ml

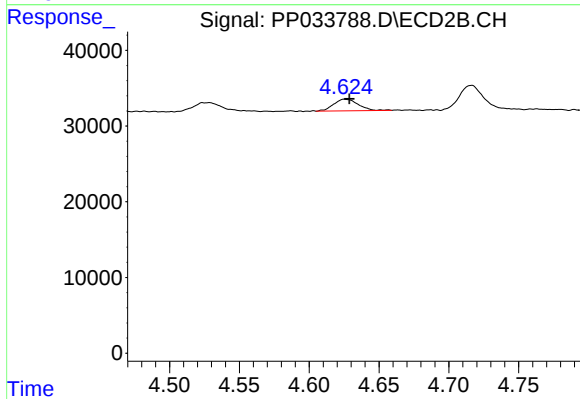

#9 AR-1221-2


R.T.: 4.626 min
Delta R.T.: -0.003 min
Response: 18754
Conc: 57.96 ng/ml

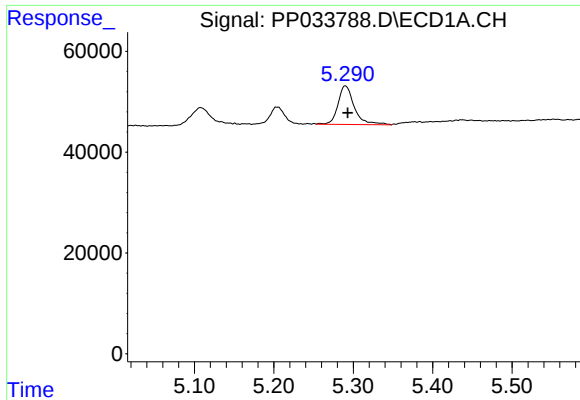

#10 AR-1221-3

R.T.: 5.290 min
Delta R.T.: -0.003 min
Response: 109295
Conc: 51.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2021

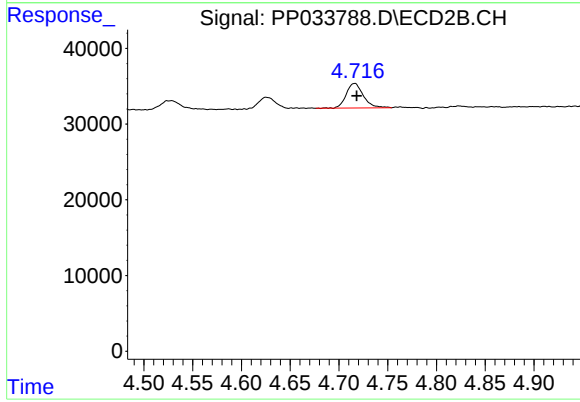

#10 AR-1221-3

R.T.: 4.716 min
Delta R.T.: -0.002 min
Response: 39431
Conc: 40.23 ng/ml