

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030922\
 Data File : PP044381.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Mar 2022 09:52
 Operator : YP\AJ
 Sample : N1827-07 10X
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CLI-2022-28A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 09 13:46:36 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 03 02:21:53 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.910	3.165	3066555	2913546	1.480	1.665
2) SA Decachlor...	10.046	8.531	2692323	3134006	1.956	2.043

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030922\
Data File : PP044381.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Mar 2022 09:52
Operator : YP\AJ
Sample : N1827-07 10X
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
CLI-2022-28A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 09 13:46:36 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 03 02:21:53 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

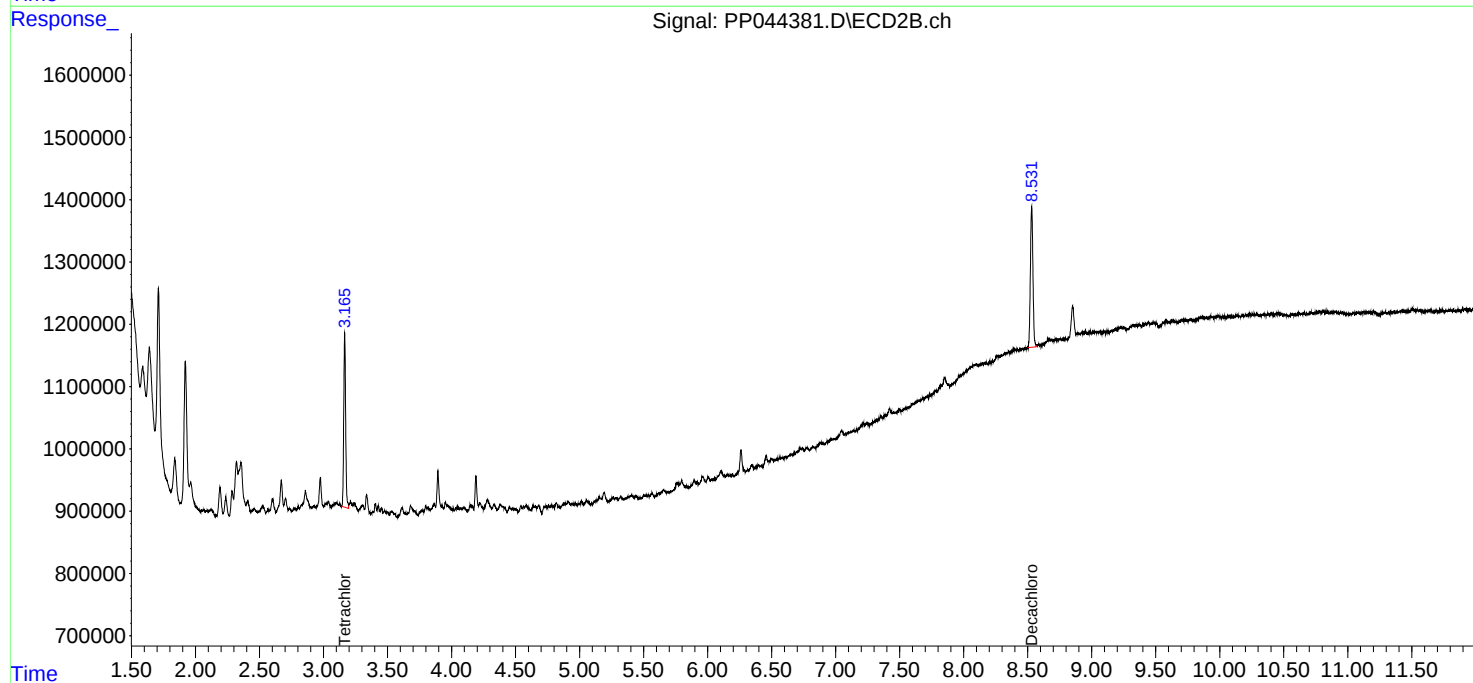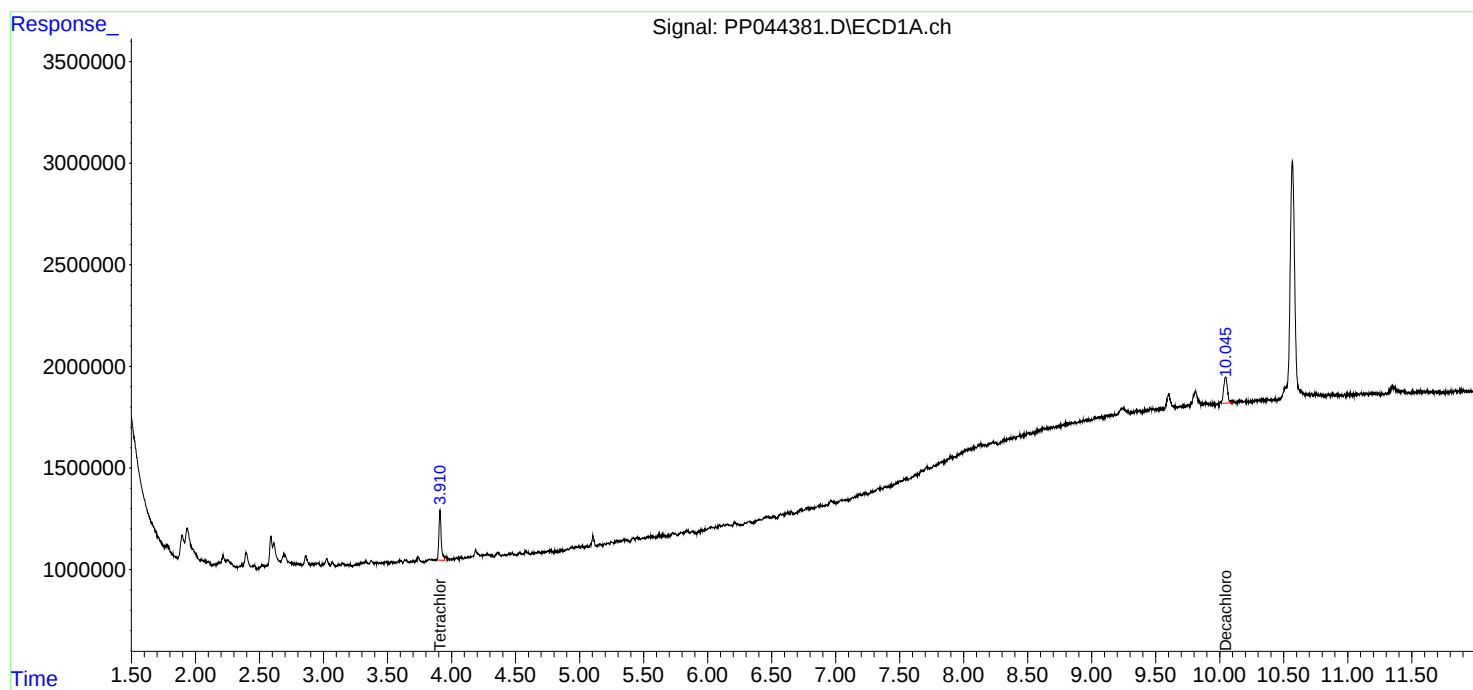


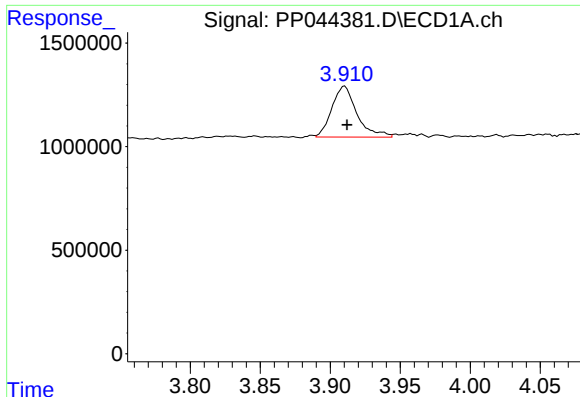

#1 Tetrachloro-m-xylene


R.T.: 3.910 min
Delta R.T.: -0.002 min
Response: 3066555
Conc: 1.48 ng/ml

Instrument :
ECD_P
ClientSampleId :
CLI-2022-28A

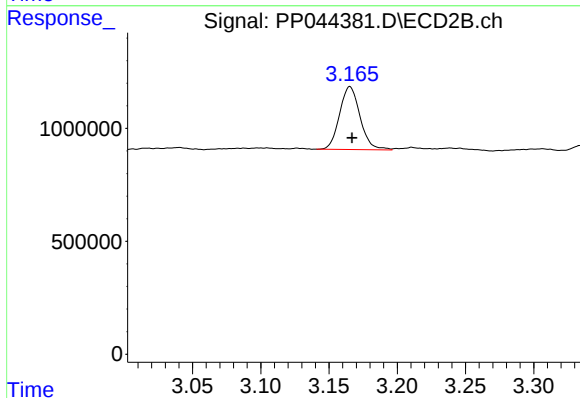


#1 Tetrachloro-m-xylene

R.T.: 3.165 min
Delta R.T.: -0.001 min
Response: 2913546
Conc: 1.67 ng/ml

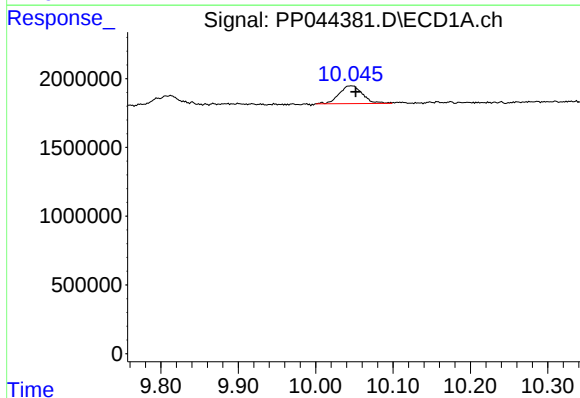

#2 Decachlorobiphenyl

R.T.: 10.046 min
Delta R.T.: -0.006 min
Response: 2692323
Conc: 1.96 ng/ml

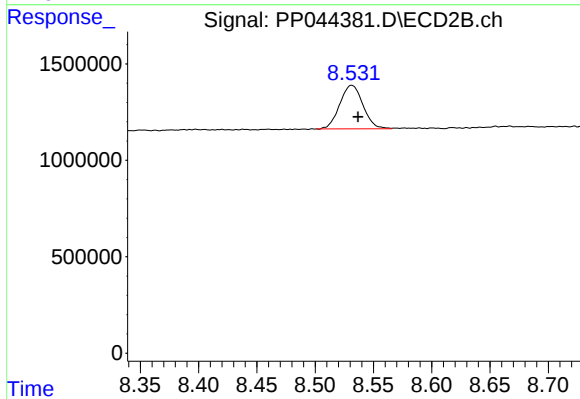

#2 Decachlorobiphenyl

R.T.: 8.531 min
Delta R.T.: -0.005 min
Response: 3134006
Conc: 2.04 ng/ml