

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030922\
 Data File : PP044423.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Mar 2022 21:00
 Operator : YP\AJ
 Sample : N1645-07
 Misc : AR1221 LOD 25 PPB
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 10 01:17:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 03 02:21:53 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.909	3.165	36675901	32073161	17.701	18.333
2) SA Decachlor...	10.045	8.530	24468073	28649596	17.777	18.677
Target Compounds						
8) L2 AR-1221-1	4.129	3.392	7668042	487217	310.326	21.224 #
9) L2 AR-1221-2	4.231	3.458f	1295275	7798217	69.037	451.491 #
10) L2 AR-1221-3	4.308	3.560	1440755	1201779	25.748	24.168



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030922\
Data File : PP044423.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Mar 2022 21:00
Operator : YP\AJ
Sample : N1645-07
Misc : AR1221 LOD 25 PPB
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 10 01:17:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 03 02:21:53 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

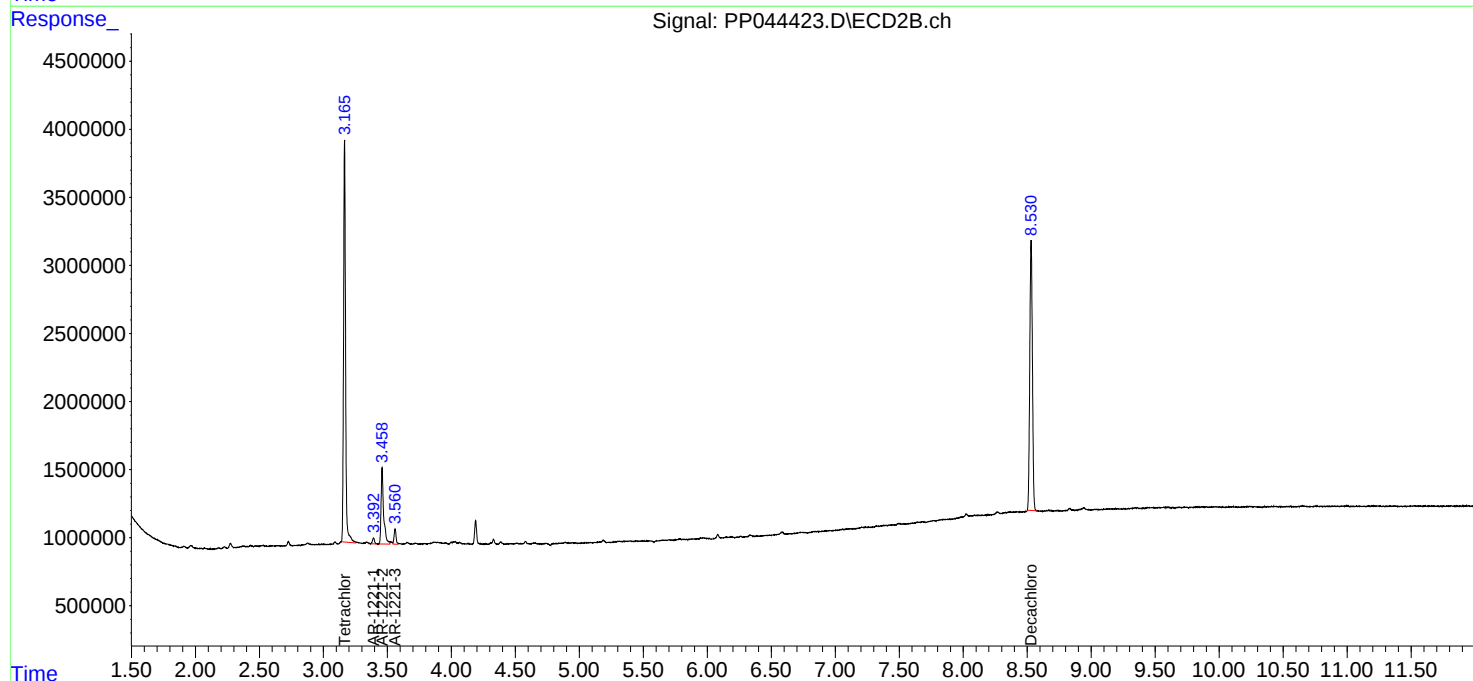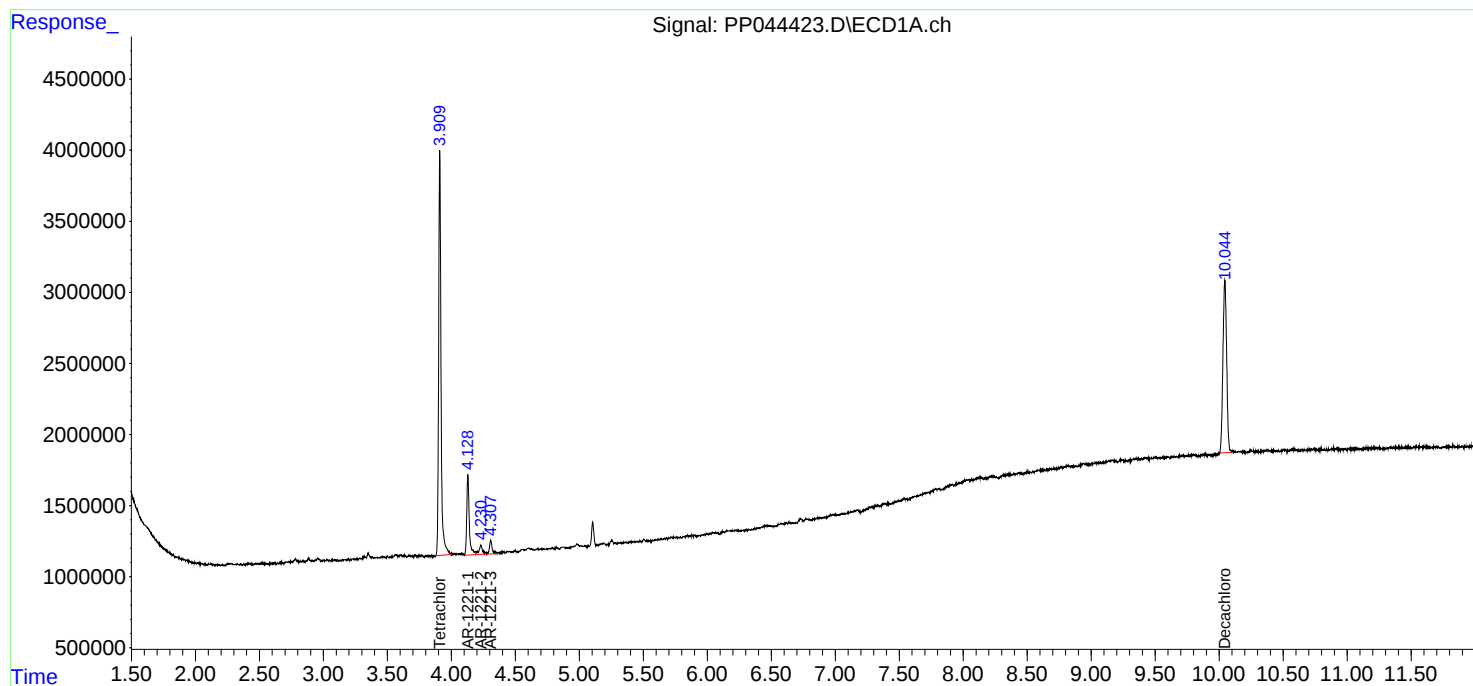


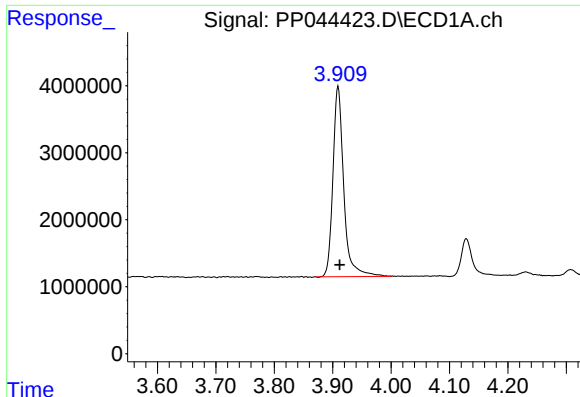

#1 Tetrachloro-m-xylene


R.T.: 3.909 min
Delta R.T.: -0.003 min
Response: 36675901
Conc: 17.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2022

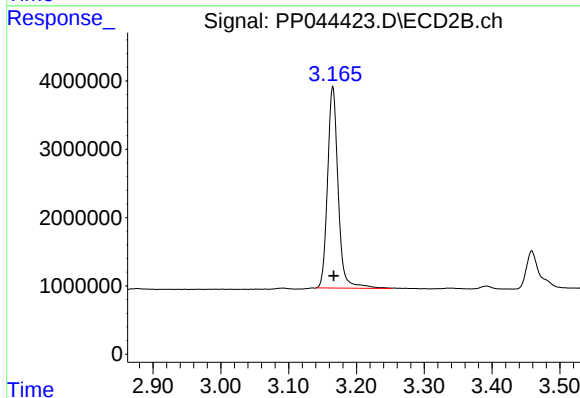


#1 Tetrachloro-m-xylene

R.T.: 3.165 min
Delta R.T.: -0.002 min
Response: 32073161
Conc: 18.33 ng/ml

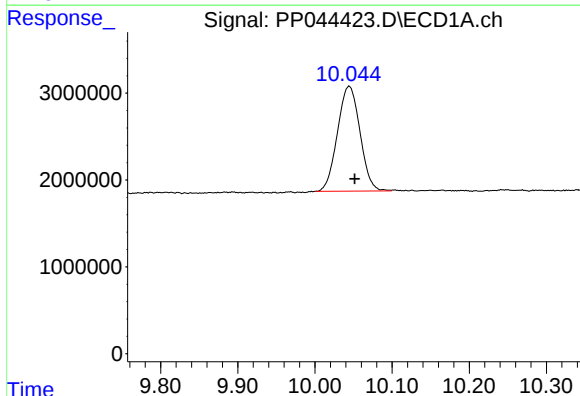


#2 Decachlorobiphenyl

R.T.: 10.045 min
Delta R.T.: -0.007 min
Response: 24468073
Conc: 17.78 ng/ml

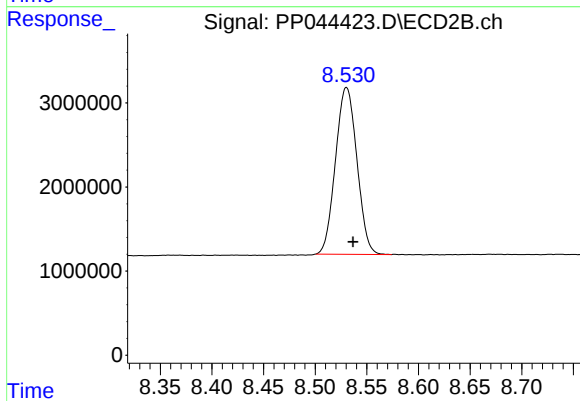

#2 Decachlorobiphenyl


R.T.: 8.530 min
Delta R.T.: -0.006 min
Response: 28649596
Conc: 18.68 ng/ml

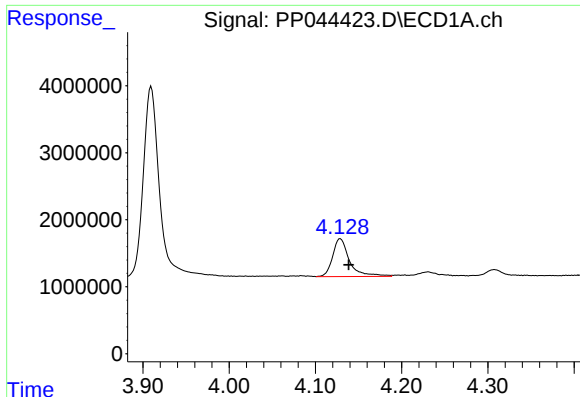

#8 AR-1221-1


R.T.: 4.129 min
Delta R.T.: -0.009 min
Response: 7668042
Conc: 310.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2022

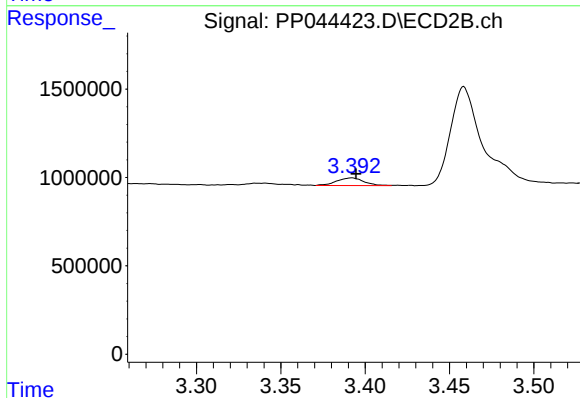


#8 AR-1221-1

R.T.: 3.392 min
Delta R.T.: -0.002 min
Response: 487217
Conc: 21.22 ng/ml

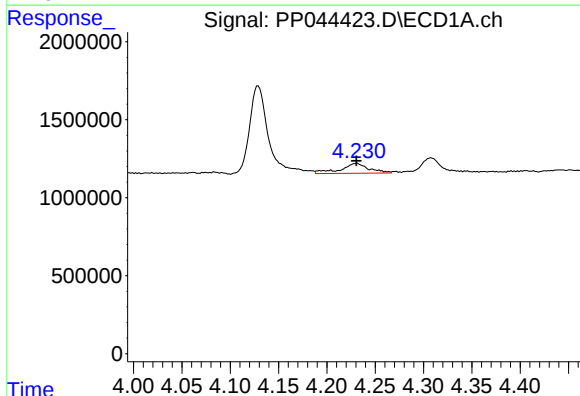


#9 AR-1221-2

R.T.: 4.231 min
Delta R.T.: 0.000 min
Response: 1295275
Conc: 69.04 ng/ml

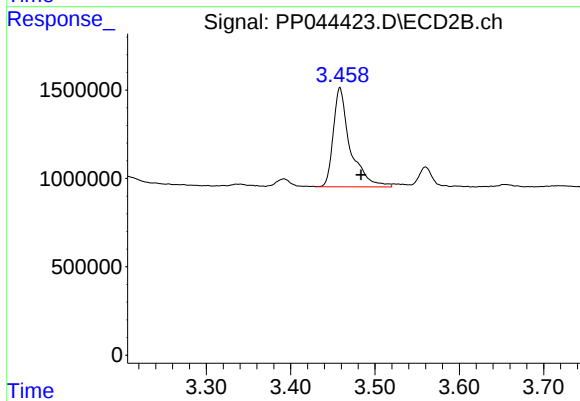

#9 AR-1221-2


R.T.: 3.458 min
Delta R.T.: -0.025 min
Response: 7798217
Conc: 451.49 ng/ml

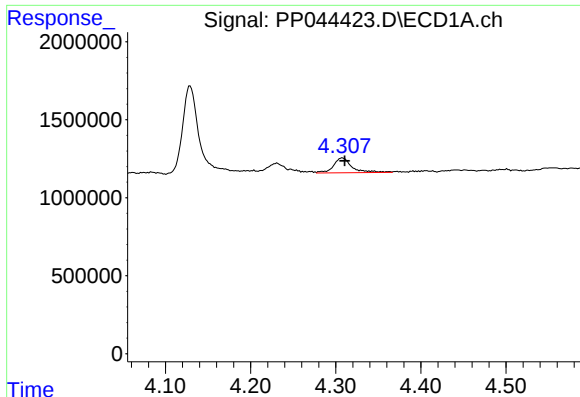

#10 AR-1221-3

R.T.: 4.308 min
Delta R.T.: -0.003 min
Response: 1440755
Conc: 25.75 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2022

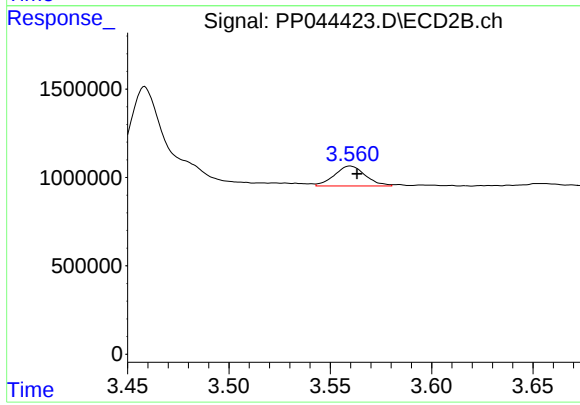

#10 AR-1221-3

R.T.: 3.560 min
Delta R.T.: -0.003 min
Response: 1201779
Conc: 24.17 ng/ml