

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030922\
 Data File : PP044424.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Mar 2022 21:15
 Operator : YP\AJ
 Sample : N1645-07
 Misc : AR1232 LOD 25 PPB
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 10 01:17:54 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 03 02:21:53 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.910	3.165	36441072	32405924	17.588	18.524
2) SA Decachlor...	10.045	8.530	24326899	28397716	17.675	18.512
Target Compounds						
11) L3 AR-1232-1	4.307	3.560	1152859	990793	25.122	23.843
12) L3 AR-1232-2	4.872	4.328	493447	1131773	21.927	32.770 #
13) L3 AR-1232-3	5.184	4.511	862431	495655	19.931	26.567 #
14) L3 AR-1232-4	5.360	4.603	463556	417581	23.088	25.325
15) L3 AR-1232-5	5.463	4.782	314469	447759	20.727	24.734



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030922\
Data File : PP044424.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Mar 2022 21:15
Operator : YP\AJ
Sample : N1645-07
Misc : AR1232 LOD 25 PPB
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 10 01:17:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 03 02:21:53 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

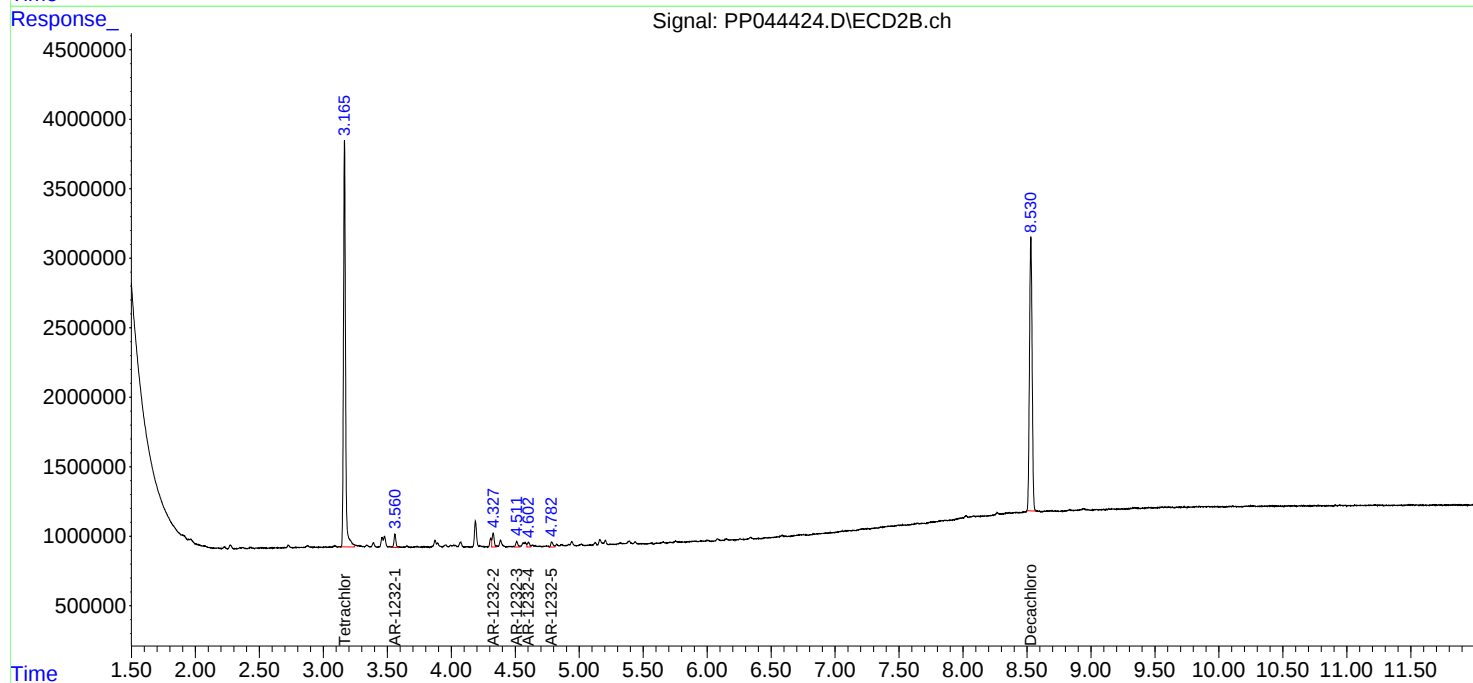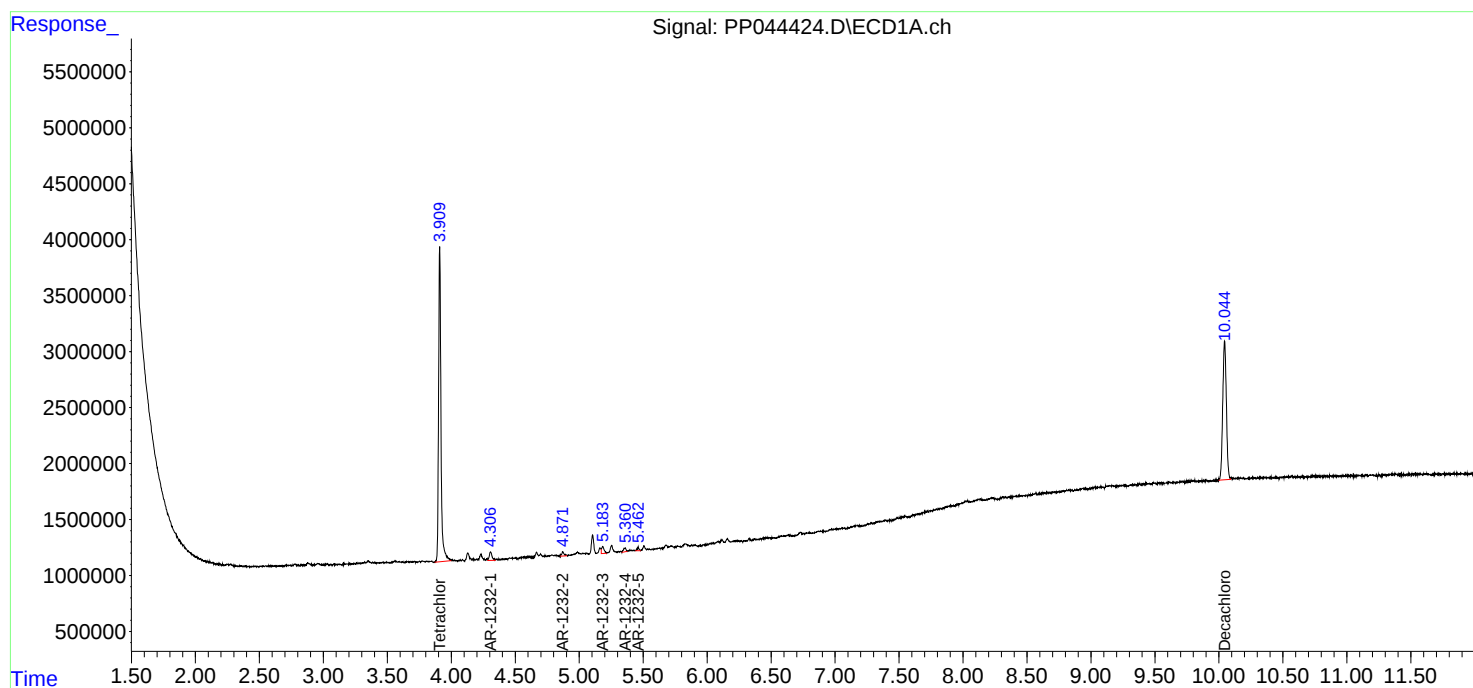


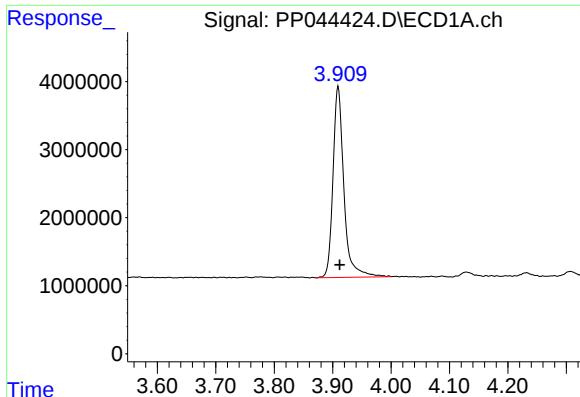

#1 Tetrachloro-m-xylene


R.T.: 3.910 min
Delta R.T.: -0.002 min
Response: 36441072
Conc: 17.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2022

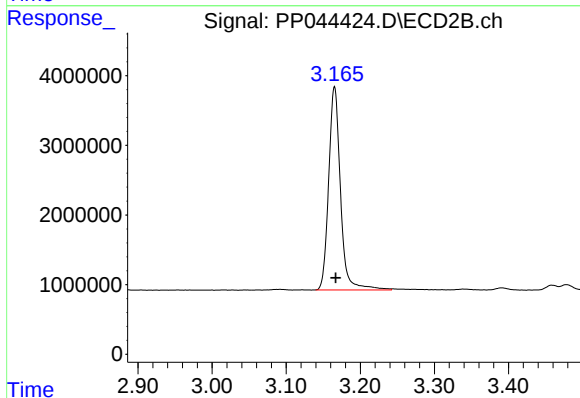


#1 Tetrachloro-m-xylene

R.T.: 3.165 min
Delta R.T.: -0.002 min
Response: 32405924
Conc: 18.52 ng/ml

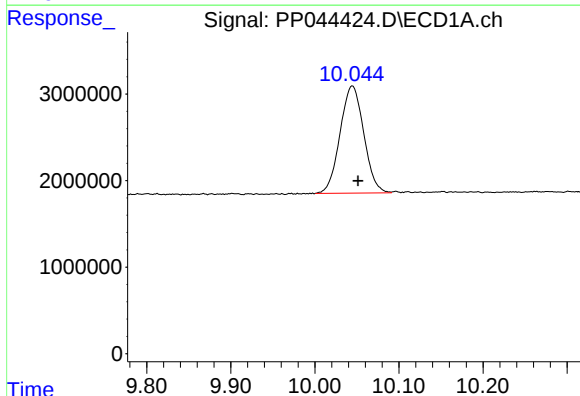


#2 Decachlorobiphenyl

R.T.: 10.045 min
Delta R.T.: -0.007 min
Response: 24326899
Conc: 17.67 ng/ml

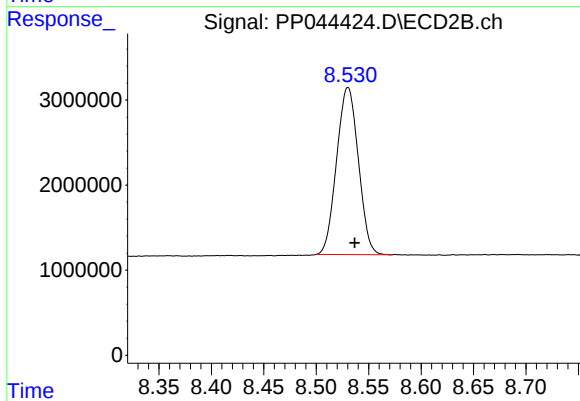

#2 Decachlorobiphenyl


R.T.: 8.530 min
Delta R.T.: -0.006 min
Response: 28397716
Conc: 18.51 ng/ml

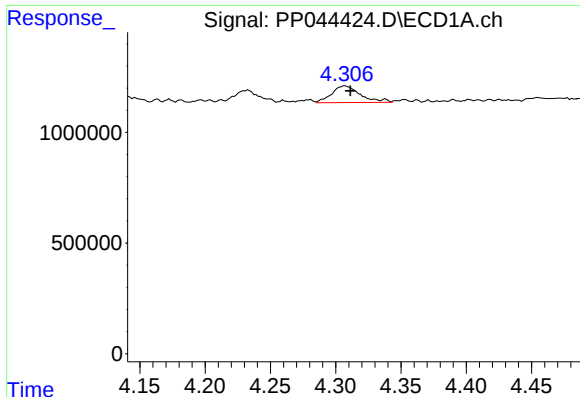

#11 AR-1232-1


R.T.: 4.307 min
Delta R.T.: -0.004 min
Response: 1152859
Conc: 25.12 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2022

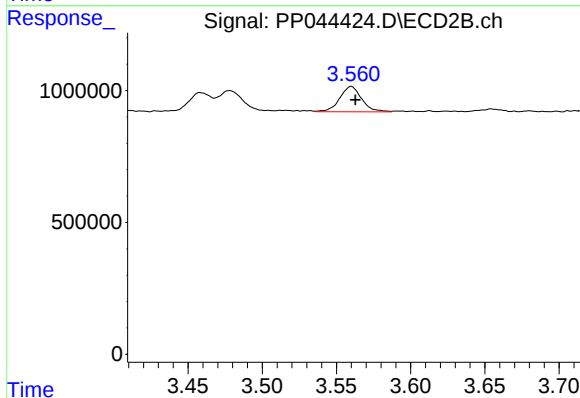


#11 AR-1232-1

R.T.: 3.560 min
Delta R.T.: -0.003 min
Response: 990793
Conc: 23.84 ng/ml

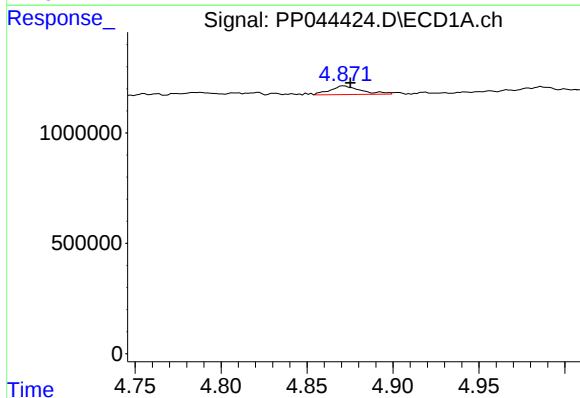


#12 AR-1232-2

R.T.: 4.872 min
Delta R.T.: -0.004 min
Response: 493447
Conc: 21.93 ng/ml

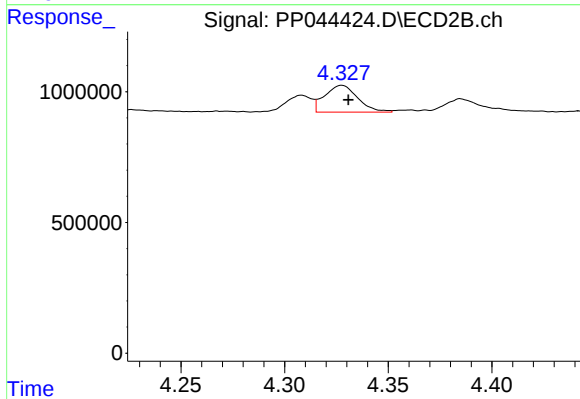

#12 AR-1232-2


R.T.: 4.328 min
Delta R.T.: -0.003 min
Response: 1131773
Conc: 32.77 ng/ml

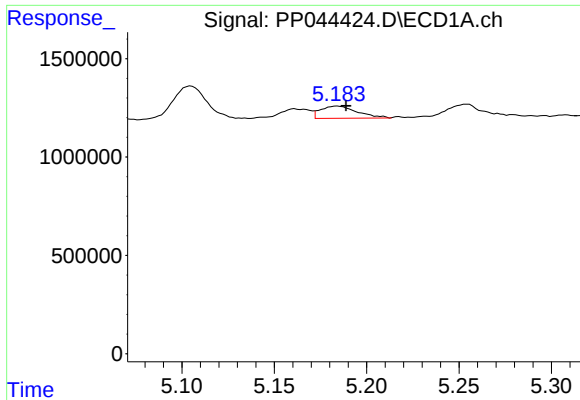

#13 AR-1232-3


R.T.: 5.184 min
Delta R.T.: -0.005 min
Response: 862431
Conc: 19.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2022

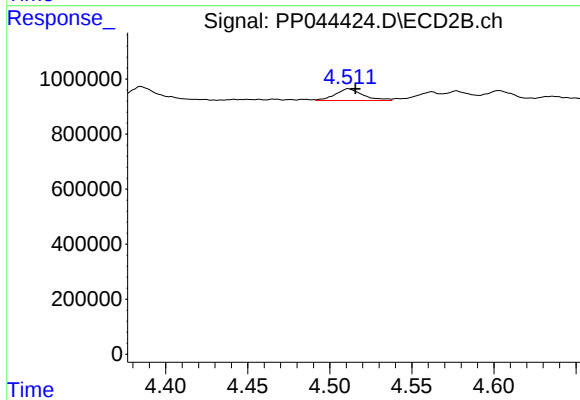


#13 AR-1232-3

R.T.: 4.511 min
Delta R.T.: -0.004 min
Response: 495655
Conc: 26.57 ng/ml

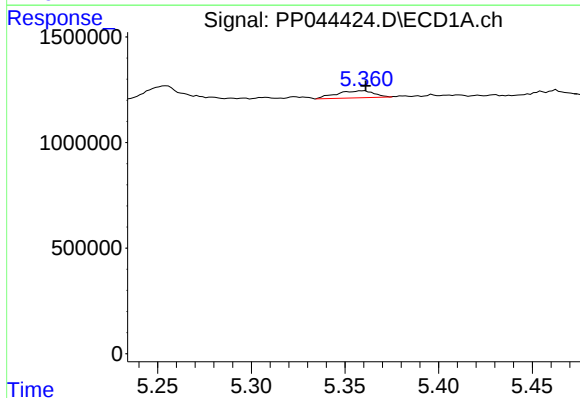


#14 AR-1232-4

R.T.: 5.360 min
Delta R.T.: -0.002 min
Response: 463556
Conc: 23.09 ng/ml

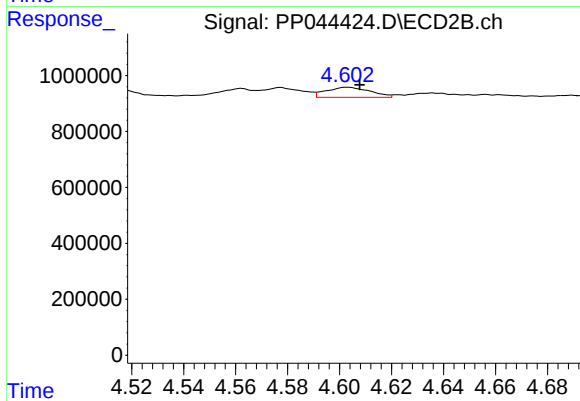

#14 AR-1232-4


R.T.: 4.603 min
Delta R.T.: -0.005 min
Response: 417581
Conc: 25.32 ng/ml

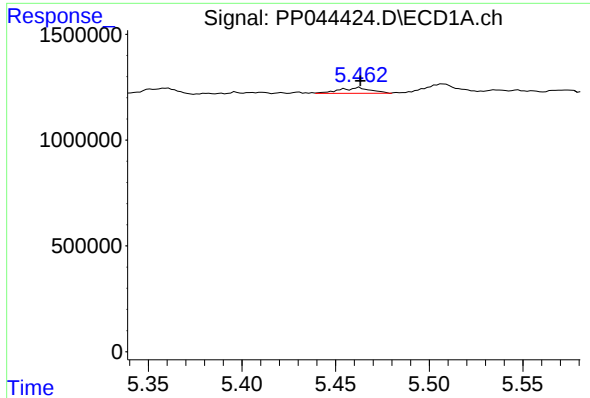

#15 AR-1232-5

R.T.: 5.463 min
Delta R.T.: 0.000 min
Response: 314469
Conc: 20.73 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2022

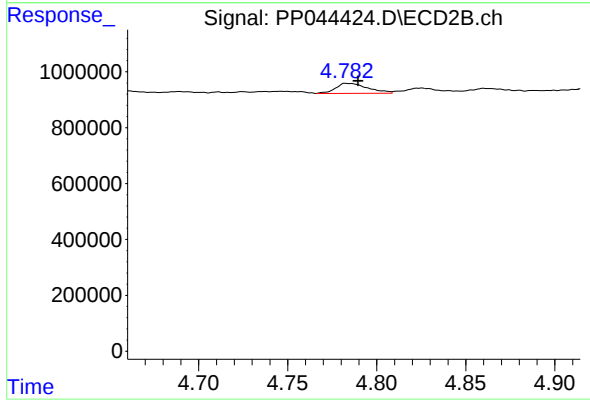

#15 AR-1232-5

R.T.: 4.782 min
Delta R.T.: -0.007 min
Response: 447759
Conc: 24.73 ng/ml