

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030922\
 Data File : PP044428.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Mar 2022 22:16
 Operator : YP\AJ
 Sample : N1645-07
 Misc : AR1262 LOD 25 PPB
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 10 01:19:57 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 03 02:21:53 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.909	3.165	36129365	31833978	17.437	18.197
2) SA Decachlor...	10.044	8.530	24354883	28538855	17.695	18.604
Target Compounds						
36) L8 AR-1262-1	7.586	6.496	2479899	2820308	24.537	27.176
37) L8 AR-1262-2	8.174	6.775	4709041	2461689	28.361	25.720
38) L8 AR-1262-3	8.507	7.351	2670221	1981970	23.858	25.124
39) L8 AR-1262-4	8.600	7.420	1364832	3507491	27.495	24.286
40) L8 AR-1262-5	9.278	7.963	1107454	1828287	19.403	25.537 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030922\
Data File : PP044428.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Mar 2022 22:16
Operator : YP\AJ
Sample : N1645-07
Misc : AR1262 LOD 25 PPB
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 10 01:19:57 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 03 02:21:53 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

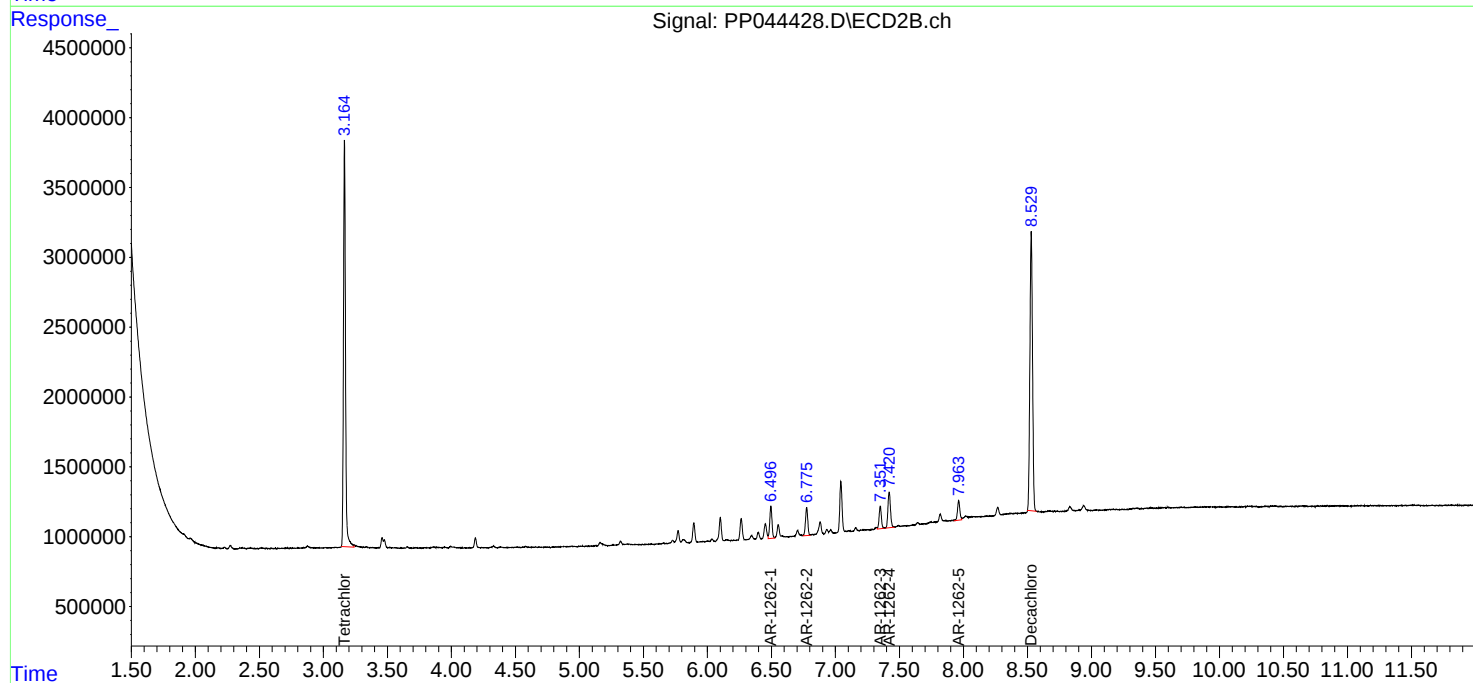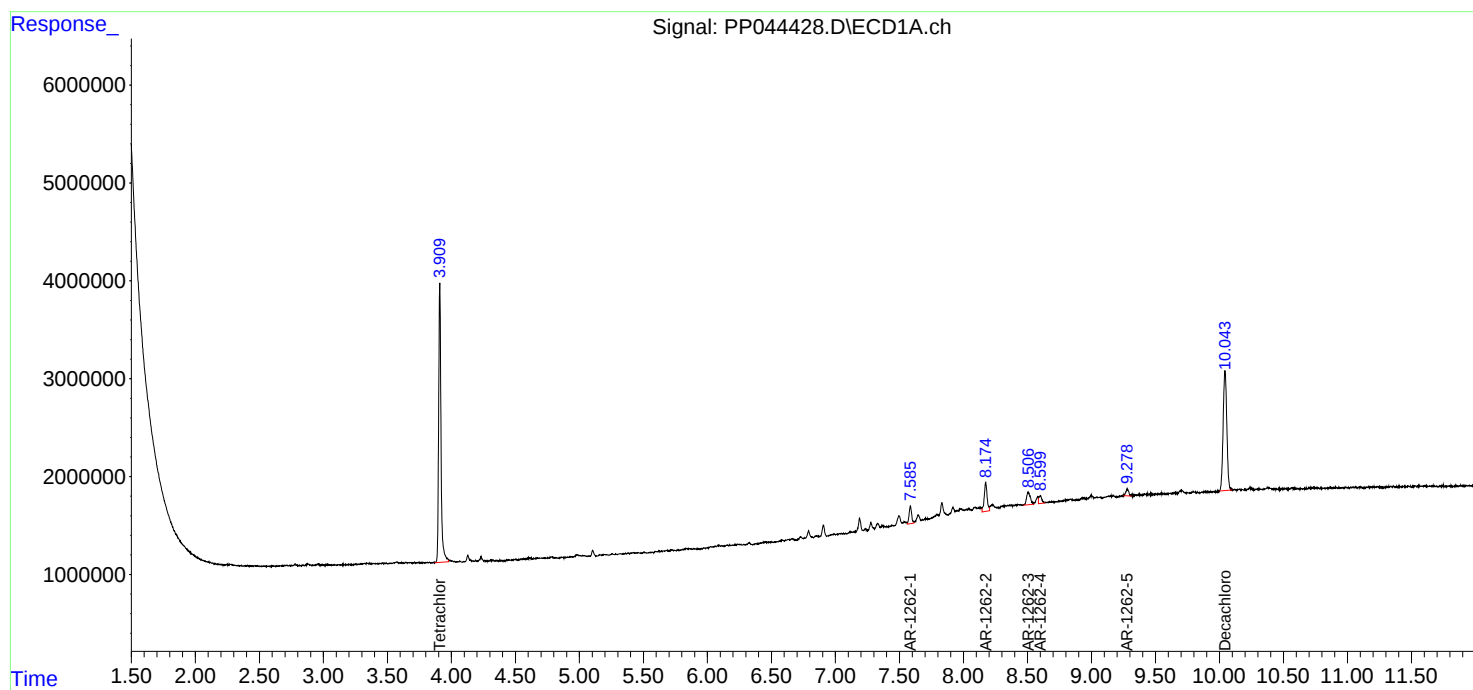


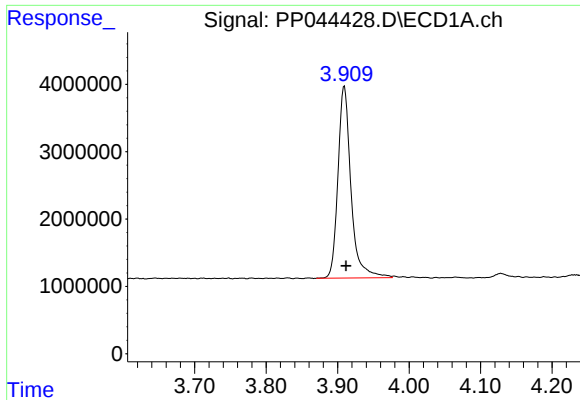

#1 Tetrachloro-m-xylene


R.T.: 3.909 min
Delta R.T.: -0.003 min
Response: 36129365
Conc: 17.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2022

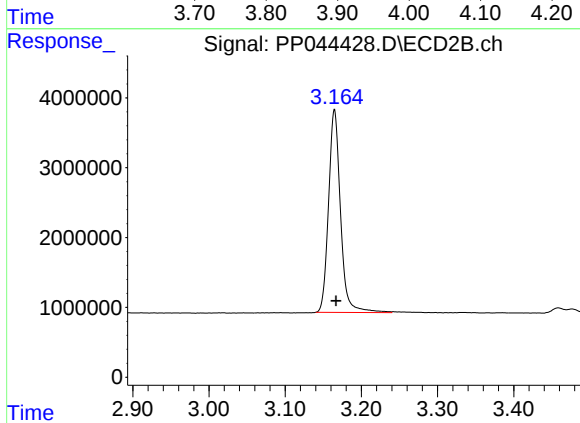


#1 Tetrachloro-m-xylene

R.T.: 3.165 min
Delta R.T.: -0.002 min
Response: 31833978
Conc: 18.20 ng/ml

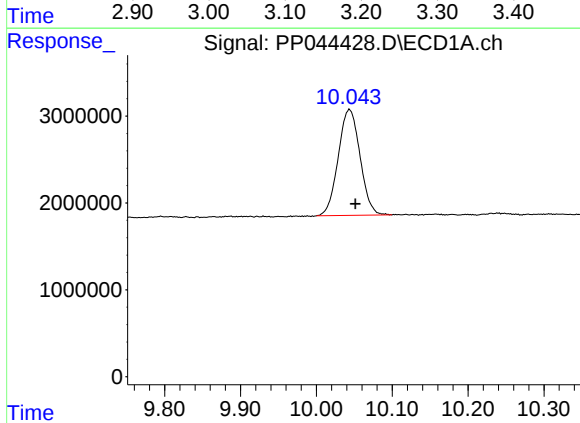


#2 Decachlorobiphenyl

R.T.: 10.044 min
Delta R.T.: -0.008 min
Response: 24354883
Conc: 17.70 ng/ml

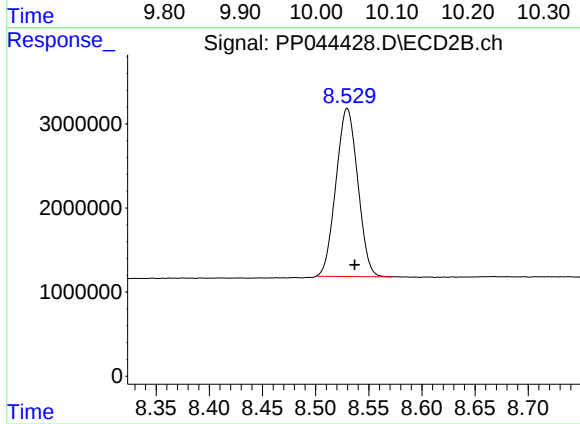

#2 Decachlorobiphenyl


R.T.: 8.530 min
Delta R.T.: -0.007 min
Response: 28538855
Conc: 18.60 ng/ml

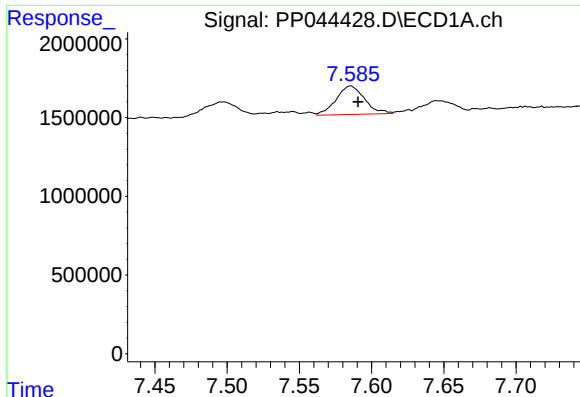

#36 AR-1262-1


R.T.: 7.586 min
Delta R.T.: -0.005 min
Response: 2479899
Conc: 24.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2022

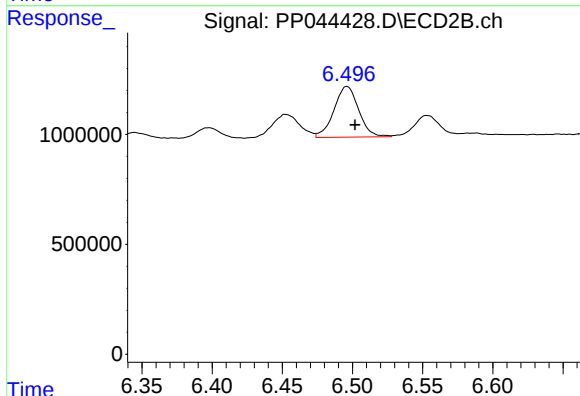


#36 AR-1262-1

R.T.: 6.496 min
Delta R.T.: -0.006 min
Response: 2820308
Conc: 27.18 ng/ml

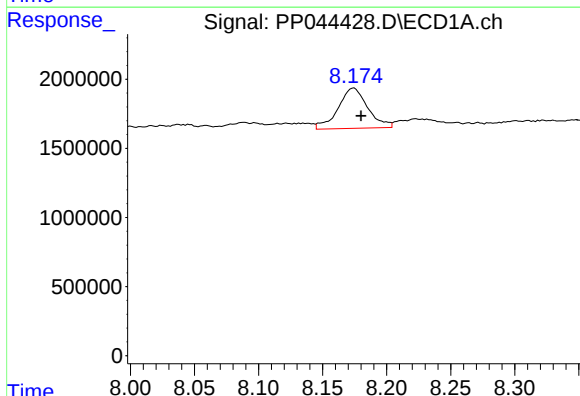


#37 AR-1262-2

R.T.: 8.174 min
Delta R.T.: -0.006 min
Response: 4709041
Conc: 28.36 ng/ml

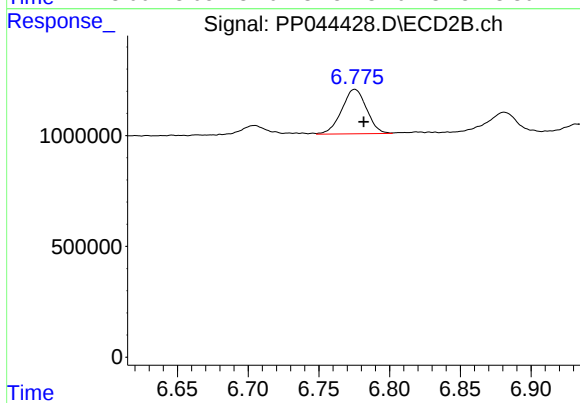

#37 AR-1262-2


R.T.: 6.775 min
Delta R.T.: -0.006 min
Response: 2461689
Conc: 25.72 ng/ml

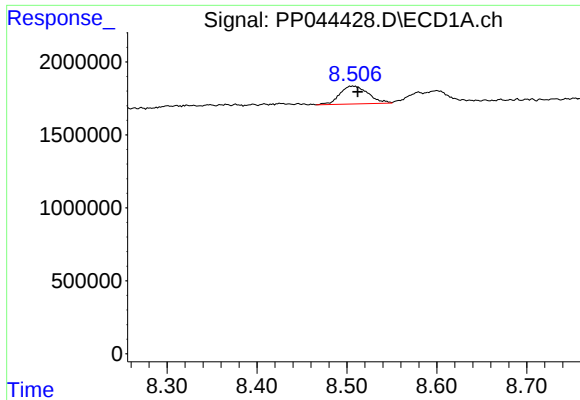

#38 AR-1262-3


R.T.: 8.507 min
Delta R.T.: -0.005 min
Response: 2670221
Conc: 23.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2022

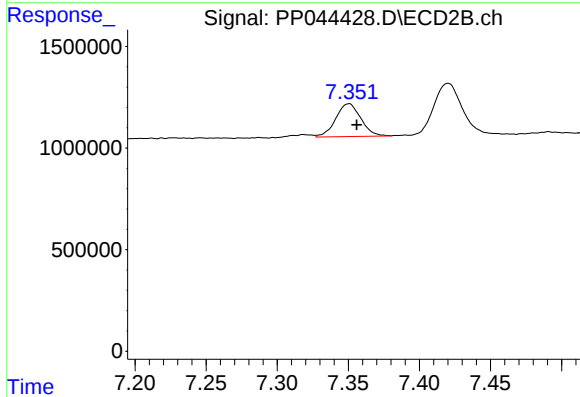


#38 AR-1262-3

R.T.: 7.351 min
Delta R.T.: -0.005 min
Response: 1981970
Conc: 25.12 ng/ml

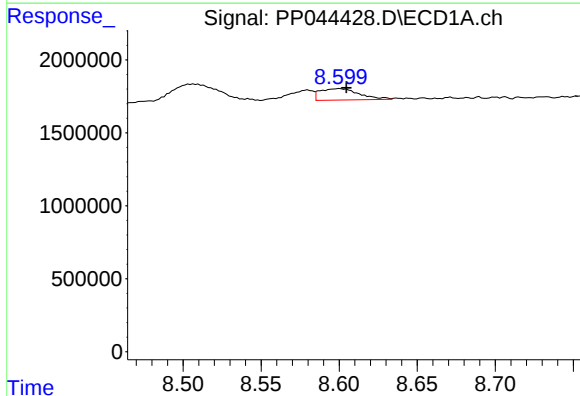


#39 AR-1262-4

R.T.: 8.600 min
Delta R.T.: -0.005 min
Response: 1364832
Conc: 27.49 ng/ml

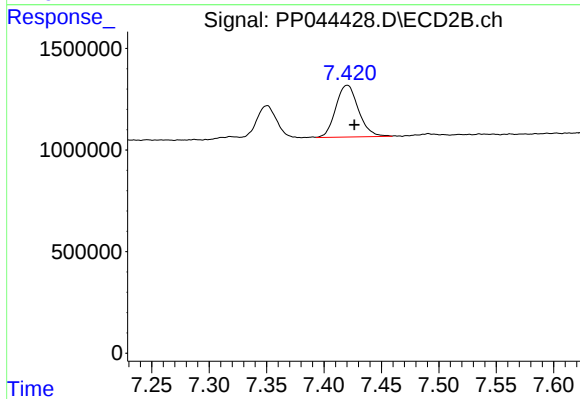

#39 AR-1262-4


R.T.: 7.420 min
Delta R.T.: -0.006 min
Response: 3507491
Conc: 24.29 ng/ml

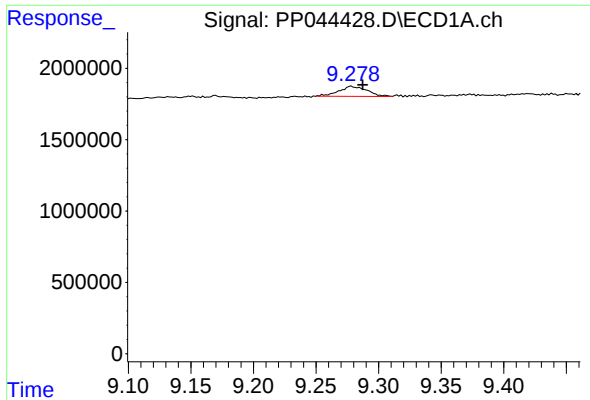

#40 AR-1262-5

R.T.: 9.278 min
Delta R.T.: -0.009 min
Response: 1107454
Conc: 19.40 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2022

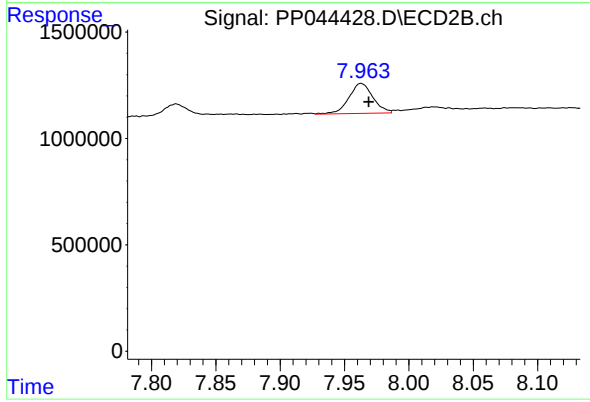

#40 AR-1262-5

R.T.: 7.963 min
Delta R.T.: -0.006 min
Response: 1828287
Conc: 25.54 ng/ml