

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030922\
 Data File : PP044429.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Mar 2022 22:31
 Operator : YP\AJ
 Sample : N1645-07
 Misc : AR1268 LOD 25 PPB
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT1-2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 10 01:20:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 03 02:21:53 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.910	3.165	37525713	32828856	18.111	18.765
2) SA Decachlor...	10.046	8.531	27644970	32114516	20.086	20.935
Target Compounds						
41) L9 AR-1268-1	8.503	7.351	4884789	5841216	25.009	25.684
42) L9 AR-1268-2	8.602	7.422	4448441	5209610	24.422	25.430
43) L9 AR-1268-3	8.839	7.643	3614918	4389181	23.421	25.111
44) L9 AR-1268-4	9.280	7.964	1369323	2042946	21.885	25.176
45) L9 AR-1268-5	9.704	8.269	10916073	13764099	23.249	25.536



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030922\
Data File : PP044429.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Mar 2022 22:31
Operator : YP\AJ
Sample : N1645-07
Misc : AR1268 LOD 25 PPB
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 10 01:20:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 03 02:21:53 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

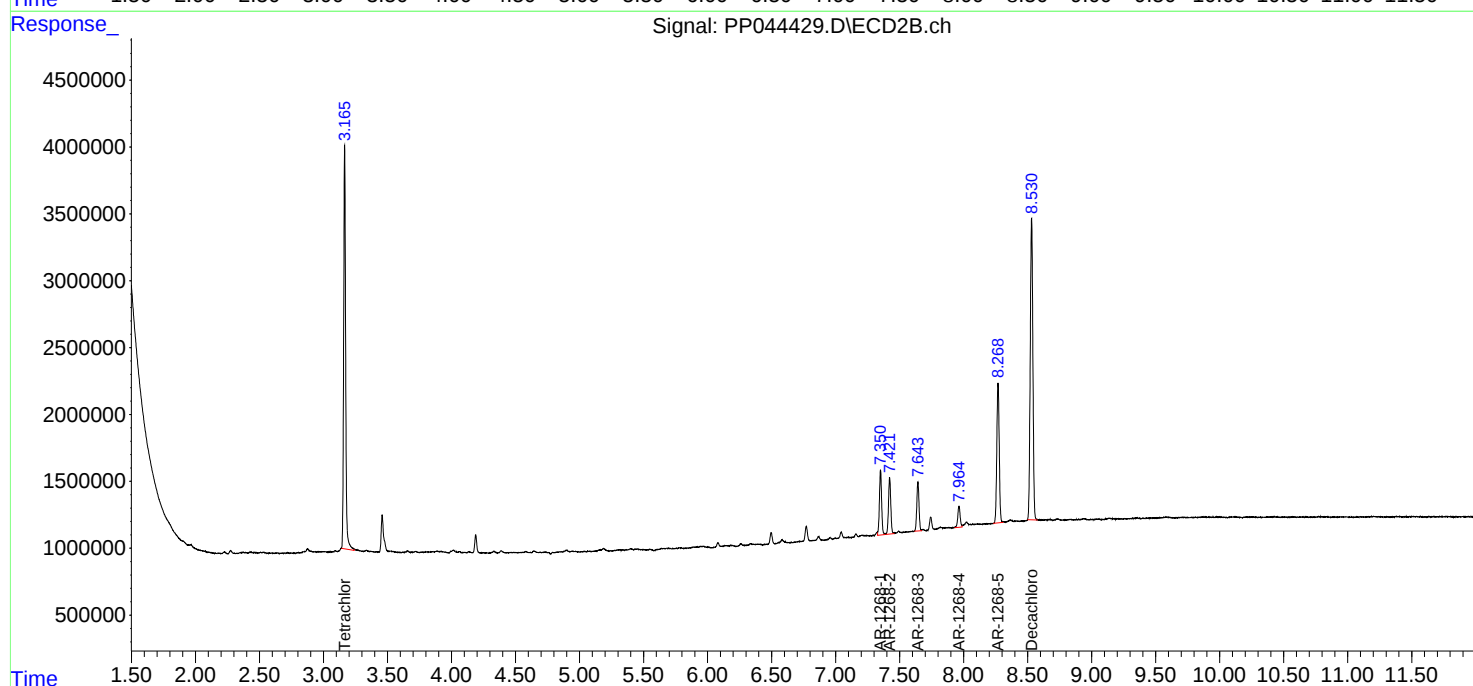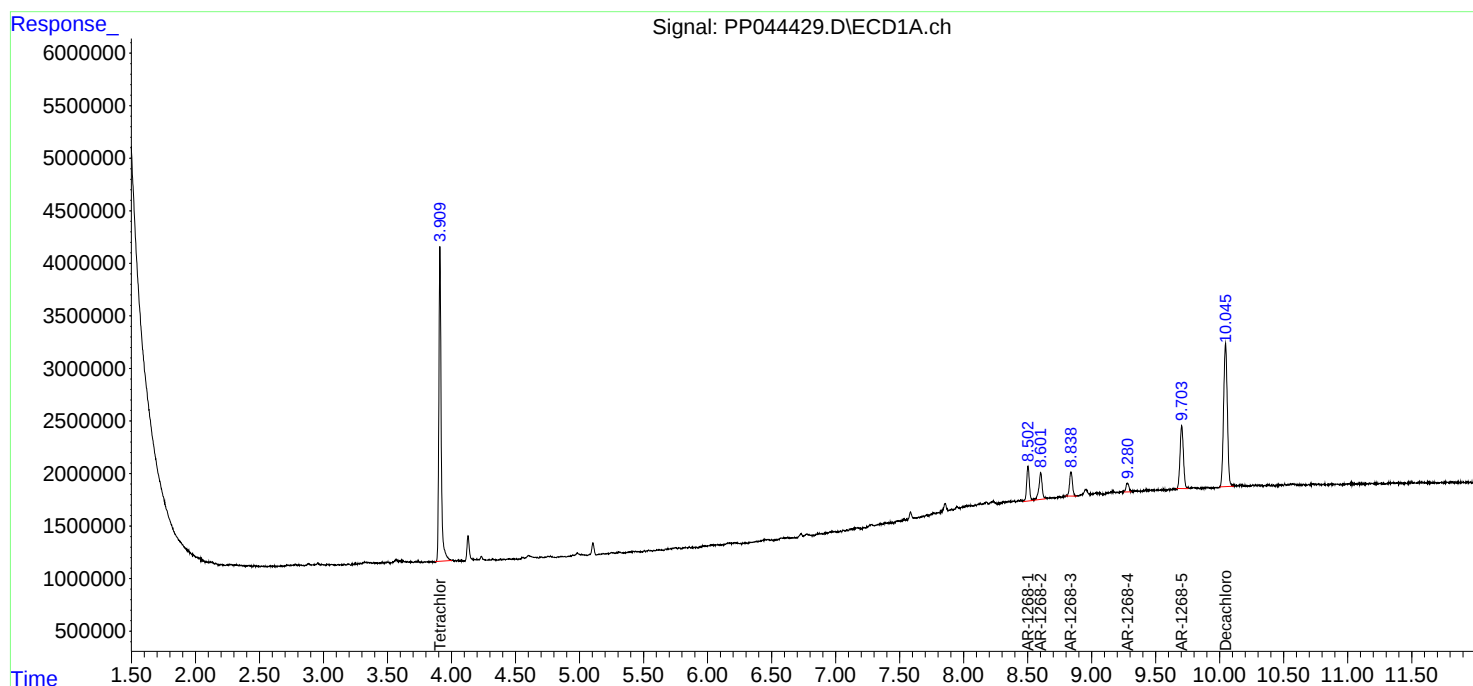


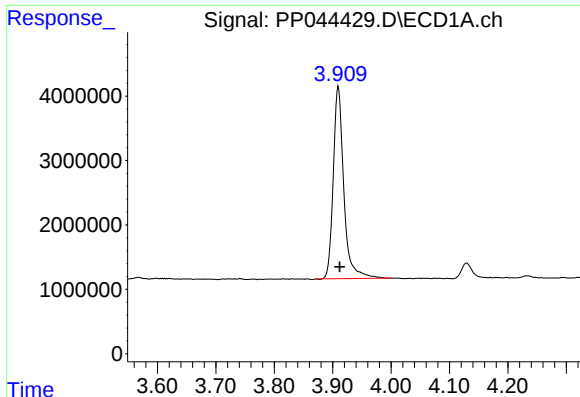

#1 Tetrachloro-m-xylene


R.T.: 3.910 min
Delta R.T.: -0.002 min
Response: 37525713
Conc: 18.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2022

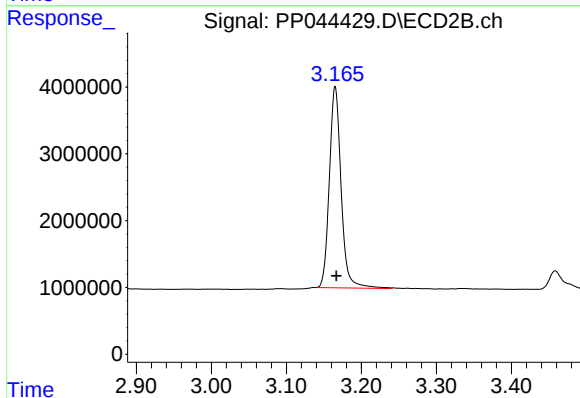


#1 Tetrachloro-m-xylene

R.T.: 3.165 min
Delta R.T.: -0.002 min
Response: 32828856
Conc: 18.77 ng/ml

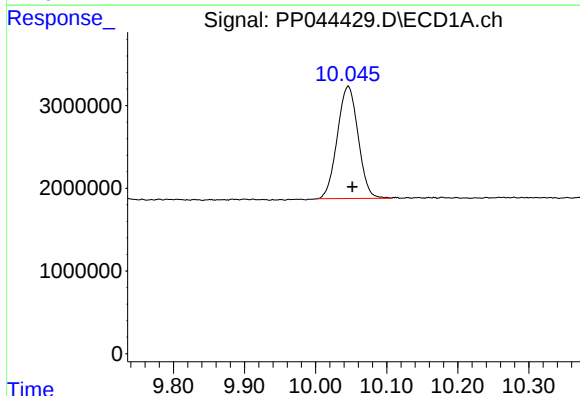


#2 Decachlorobiphenyl

R.T.: 10.046 min
Delta R.T.: -0.005 min
Response: 27644970
Conc: 20.09 ng/ml

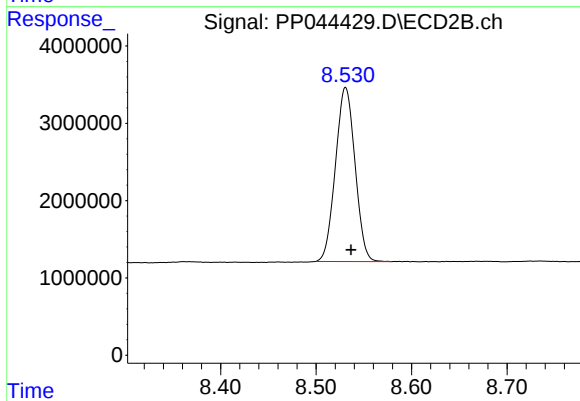

#2 Decachlorobiphenyl


R.T.: 8.531 min
Delta R.T.: -0.006 min
Response: 32114516
Conc: 20.94 ng/ml

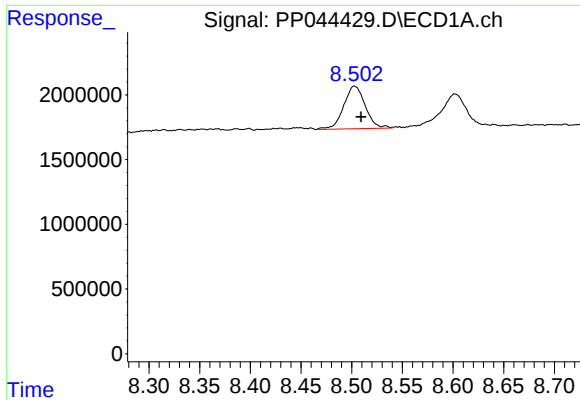

#41 AR-1268-1


R.T.: 8.503 min
Delta R.T.: -0.006 min
Response: 4884789
Conc: 25.01 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2022

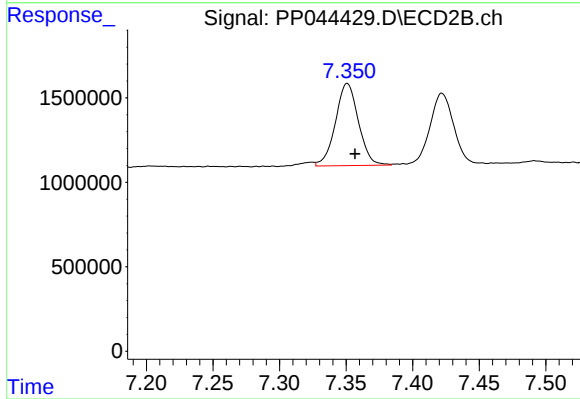


#41 AR-1268-1

R.T.: 7.351 min
Delta R.T.: -0.006 min
Response: 5841216
Conc: 25.68 ng/ml

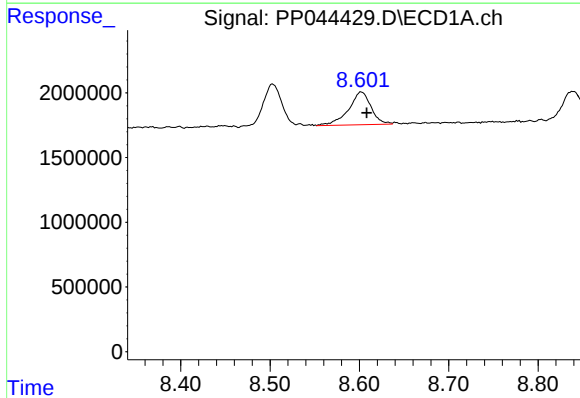


#42 AR-1268-2

R.T.: 8.602 min
Delta R.T.: -0.006 min
Response: 4448441
Conc: 24.42 ng/ml

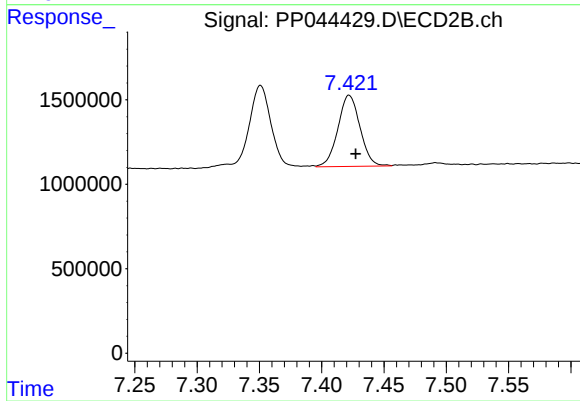

#42 AR-1268-2


R.T.: 7.422 min
Delta R.T.: -0.006 min
Response: 5209610
Conc: 25.43 ng/ml

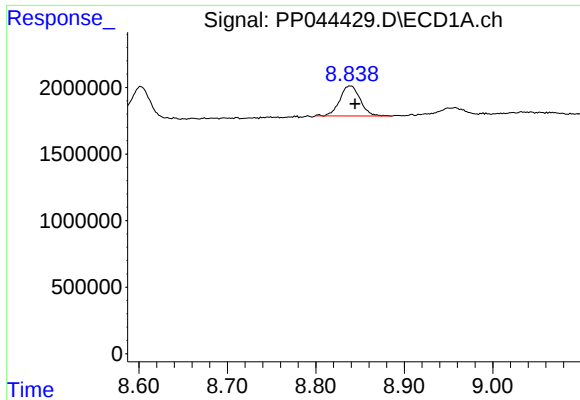

#43 AR-1268-3


R.T.: 8.839 min
Delta R.T.: -0.005 min
Response: 3614918
Conc: 23.42 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2022

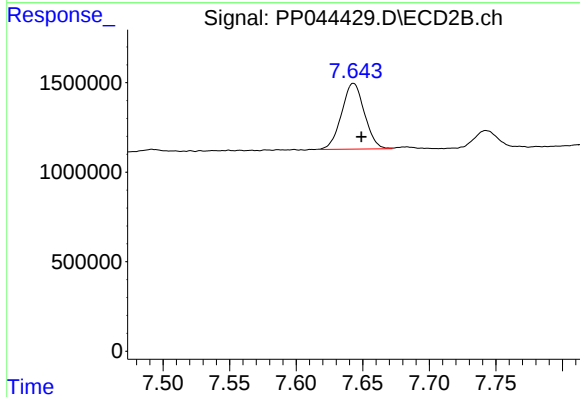


#43 AR-1268-3

R.T.: 7.643 min
Delta R.T.: -0.006 min
Response: 4389181
Conc: 25.11 ng/ml

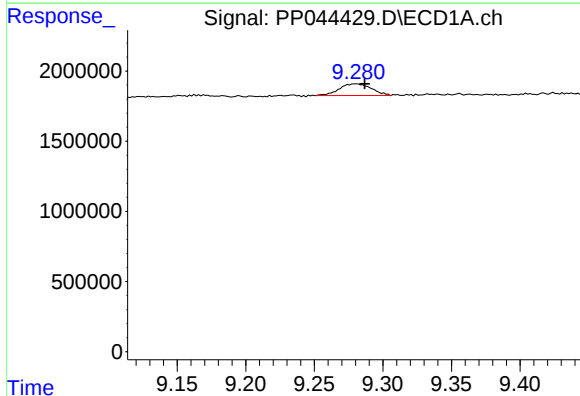


#44 AR-1268-4

R.T.: 9.280 min
Delta R.T.: -0.006 min
Response: 1369323
Conc: 21.89 ng/ml

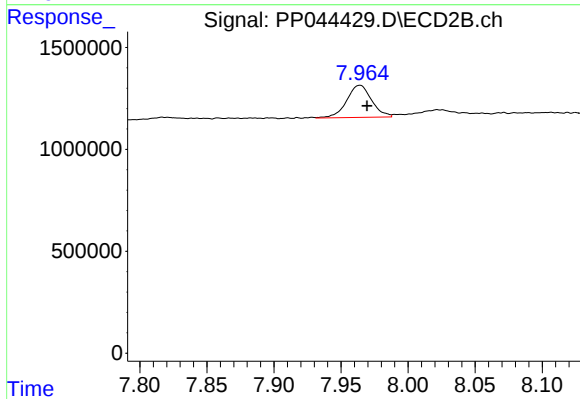

#44 AR-1268-4


R.T.: 7.964 min
Delta R.T.: -0.005 min
Response: 2042946
Conc: 25.18 ng/ml

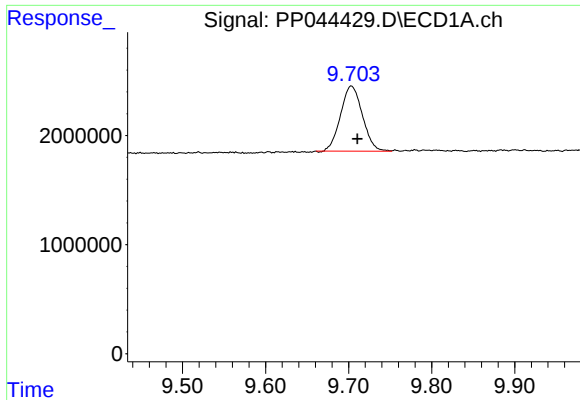

#45 AR-1268-5

R.T.: 9.704 min
Delta R.T.: -0.007 min
Response: 10916073
Conc: 23.25 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT1-2022

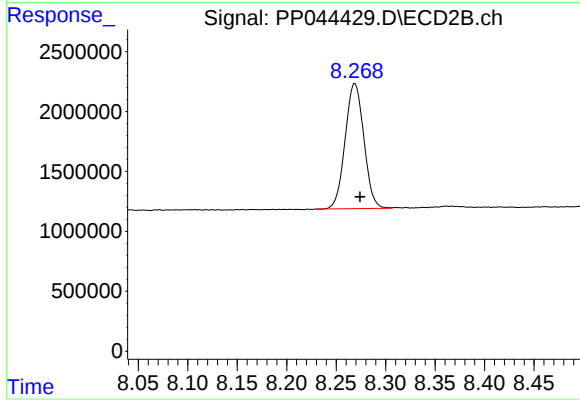

#45 AR-1268-5

R.T.: 8.269 min
Delta R.T.: -0.005 min
Response: 13764099
Conc: 25.54 ng/ml