

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030923\
 Data File : PP056317.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Mar 2023 15:30
 Operator : YP\AJ
 Sample : 01829-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SS-04-20230306

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/09/2023
 Supervised By :Ankita Jodhani 03/09/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 08 20:33:43 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 08 02:03:40 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.319	3.561	35644788	29705097	22.956	21.051
2) SA Decachlor...	10.059	8.557	44566204	26122761	22.436	23.369
Target Compounds						
31) L7 AR-1260-1	7.097	6.125	2278184	1281770	23.117	18.802
32) L7 AR-1260-2	7.357	6.314	2342025	1179160	20.191	15.414
33) L7 AR-1260-3	7.719	6.466	3030090	1308263	35.398	18.092 #
34) L7 AR-1260-4	7.943	6.938	4951173	2373243	50.080	39.576m
35) L7 AR-1260-5	8.260	7.183	8607201	5956343	43.069	46.614

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030923\
Data File : PP056317.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Mar 2023 15:30
Operator : YP\AJ
Sample : 01829-04
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
SS-04-20230306


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/09/2023
Supervised By :Ankita Jodhani 03/09/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 08 20:33:43 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030823.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 08 02:03:40 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

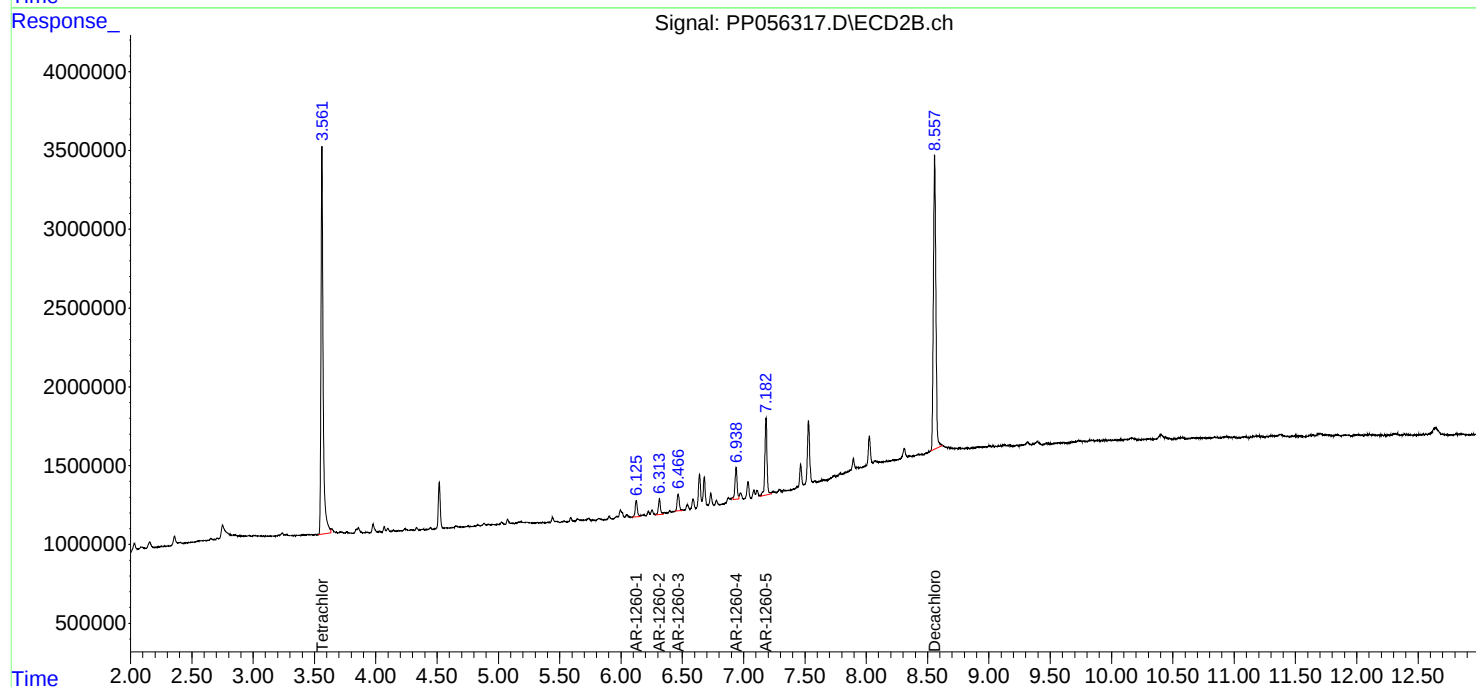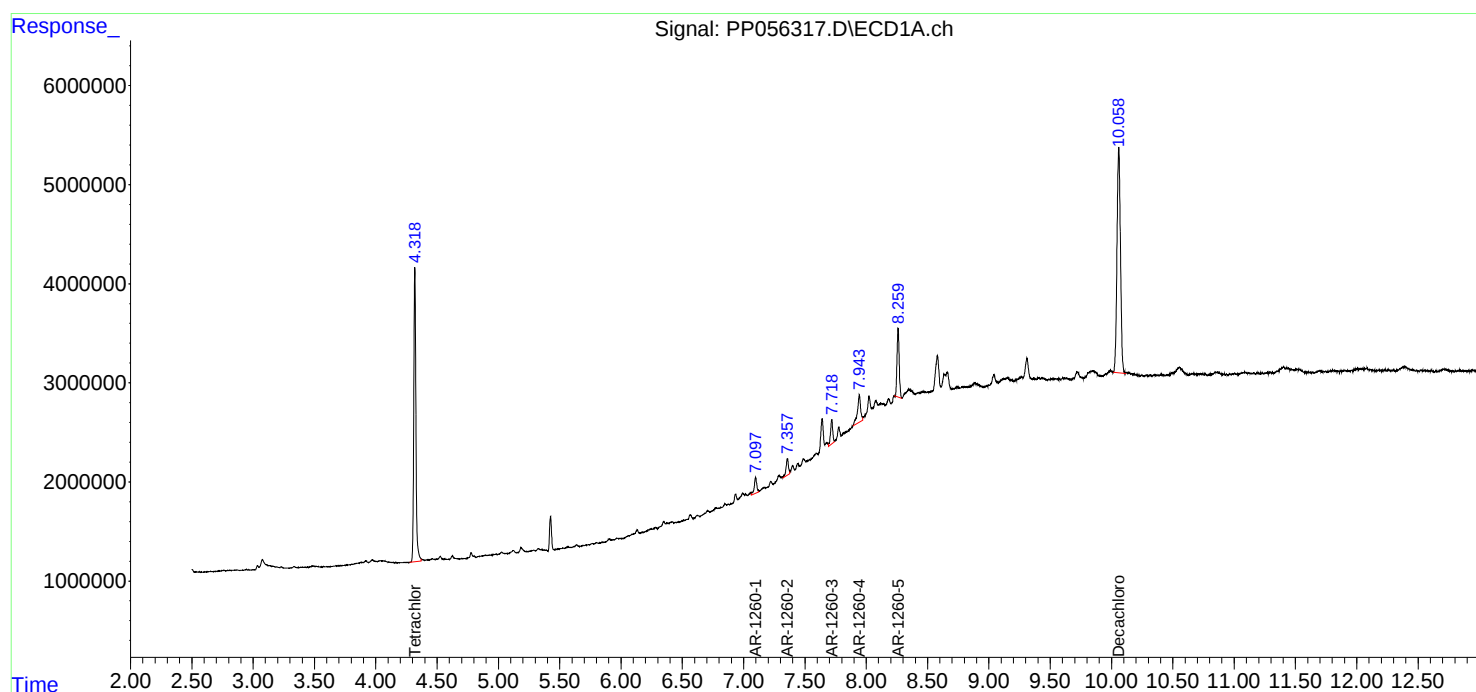

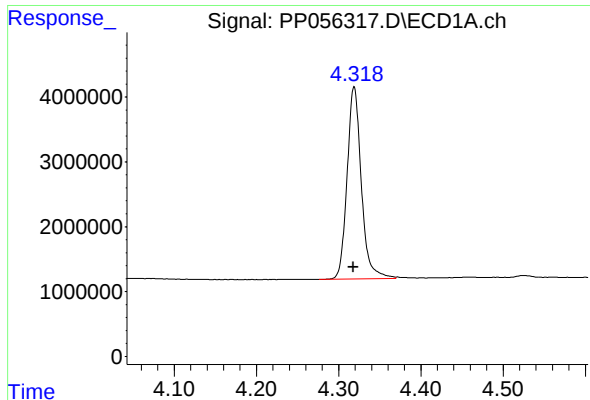


#1 Tetrachloro-m-xylene

R.T.: 4.319 min
Delta R.T.: 0.000 min
Response: 35644788
Conc: 22.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
SS-04-20230306


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/09/2023
Supervised By :Ankita Jodhani 03/09/2023

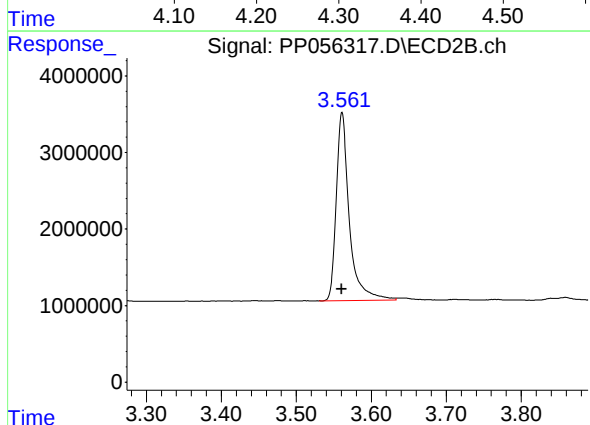


#1 Tetrachloro-m-xylene

R.T.: 3.561 min
Delta R.T.: 0.000 min
Response: 29705097
Conc: 21.05 ng/ml

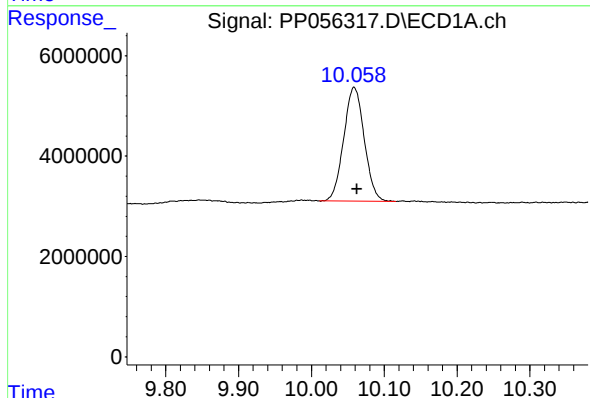


#2 Decachlorobiphenyl

R.T.: 10.059 min
Delta R.T.: -0.004 min
Response: 44566204
Conc: 22.44 ng/ml

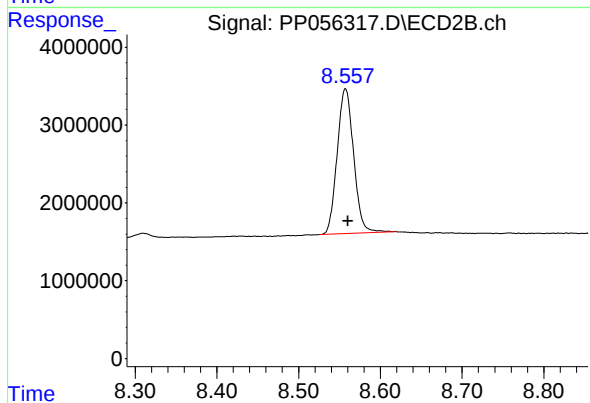

#2 Decachlorobiphenyl

R.T.: 8.557 min
Delta R.T.: -0.003 min
Response: 26122761
Conc: 23.37 ng/ml

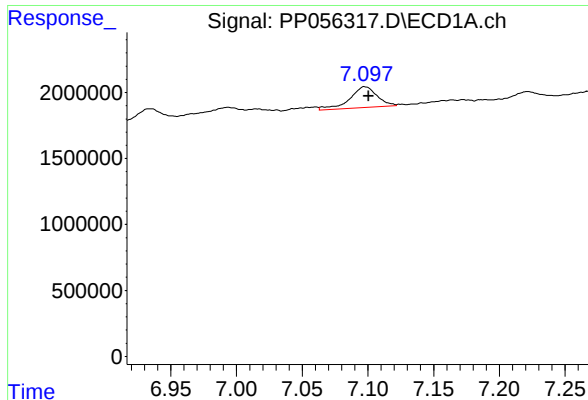


#31 AR-1260-1

R.T.: 7.097 min
Delta R.T.: -0.003 min
Response: 2278184
Conc: 23.12 ng/ml

Instrument :
ECD_P
ClientSampleId :
SS-04-20230306


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/09/2023
Supervised By :Ankita Jodhani 03/09/2023

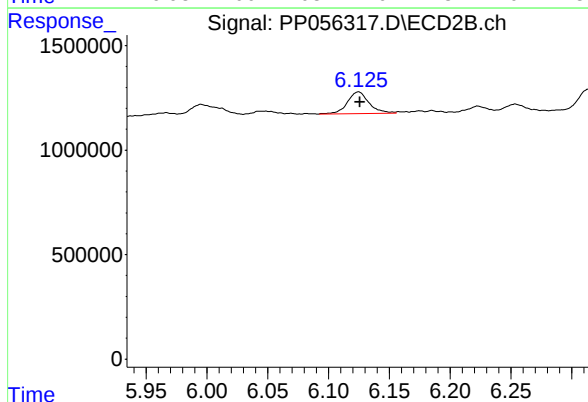


#31 AR-1260-1

R.T.: 6.125 min
Delta R.T.: -0.001 min
Response: 1281770
Conc: 18.80 ng/ml

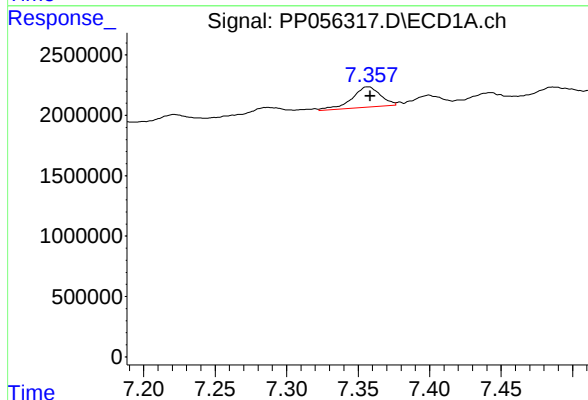


#32 AR-1260-2

R.T.: 7.357 min
Delta R.T.: -0.001 min
Response: 2342025
Conc: 20.19 ng/ml

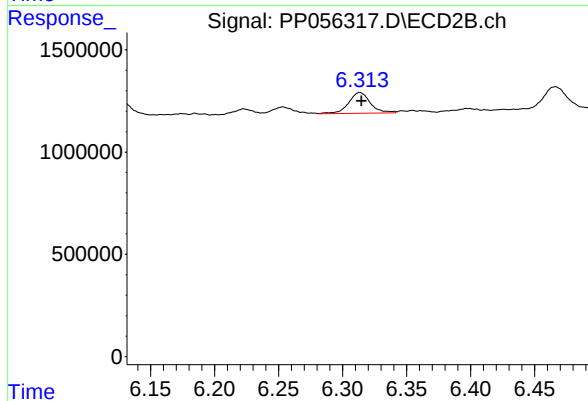

#32 AR-1260-2

R.T.: 6.314 min
Delta R.T.: -0.001 min
Response: 1179160
Conc: 15.41 ng/ml

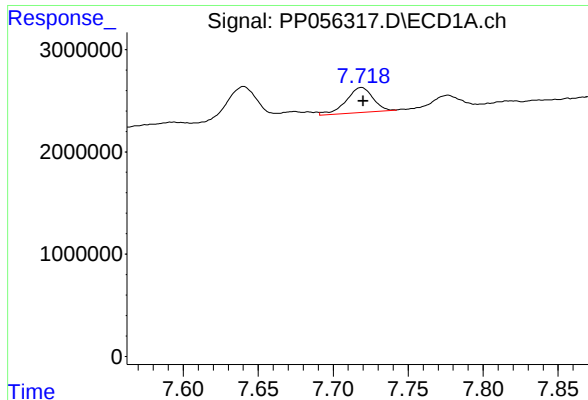


#33 AR-1260-3

R.T.: 7.719 min
Delta R.T.: -0.001 min
Response: 3030090
Conc: 35.40 ng/ml

Instrument :
ECD_P
ClientSampleId :
SS-04-20230306


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/09/2023
Supervised By :Ankita Jodhani 03/09/2023

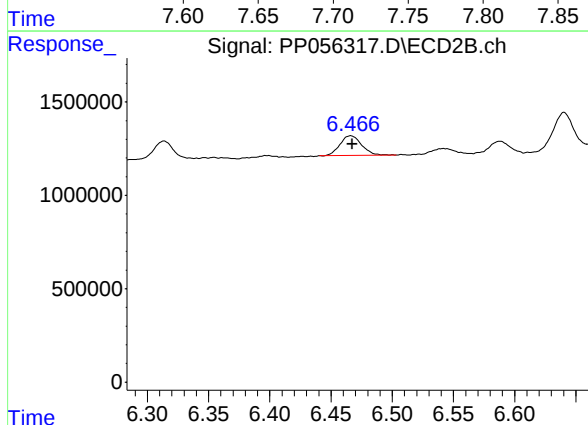


#33 AR-1260-3

R.T.: 6.466 min
Delta R.T.: -0.002 min
Response: 1308263
Conc: 18.09 ng/ml

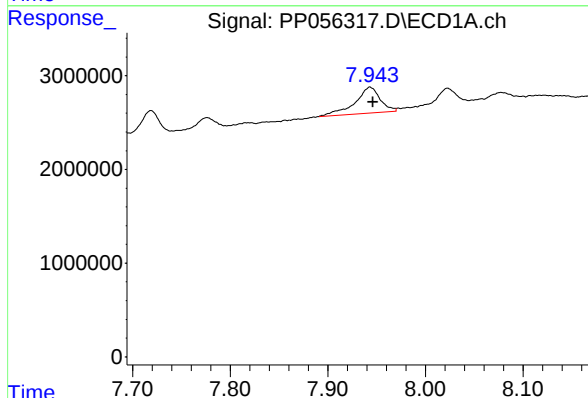


#34 AR-1260-4

R.T.: 7.943 min
Delta R.T.: -0.003 min
Response: 4951173
Conc: 50.08 ng/ml

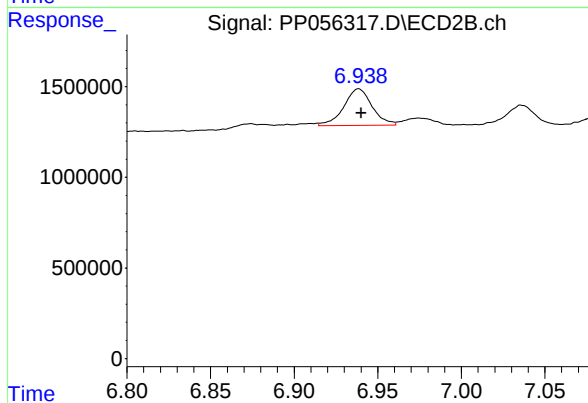

#34 AR-1260-4

R.T.: 6.938 min
Delta R.T.: -0.002 min
Response: 2373243
Conc: 39.58 ng/ml m

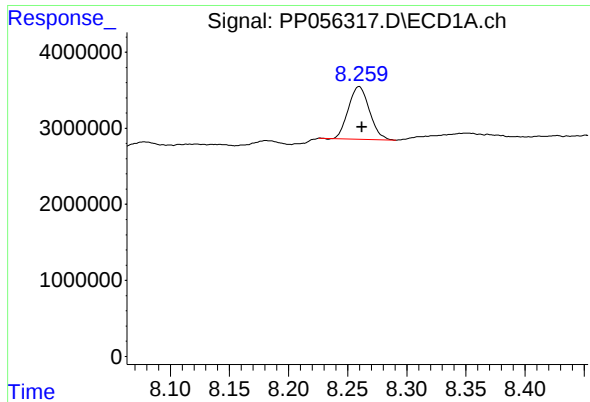


#35 AR-1260-5

R.T.: 8.260 min
Delta R.T.: -0.003 min
Response: 8607201
Conc: 43.07 ng/ml

Instrument :
ECD_P
ClientSampleId :
SS-04-20230306

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/09/2023
Supervised By :Ankita Jodhani 03/09/2023

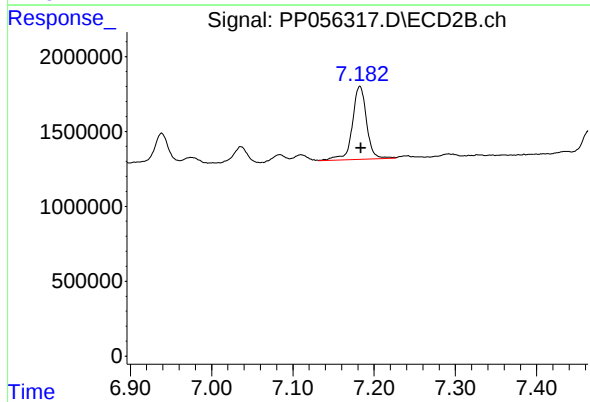

#35 AR-1260-5

R.T.: 7.183 min
Delta R.T.: -0.001 min
Response: 5956343
Conc: 46.61 ng/ml