

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030923\
 Data File : PP056320.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Mar 2023 16:20
 Operator : YP\AJ
 Sample : 01829-07
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SS-07-20230306

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/09/2023
 Supervised By :Ankita Jodhani 03/09/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 08 20:34:56 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 08 02:03:40 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.319	3.562	35824382	29571467	23.072	20.957
2) SA Decachlor...	10.059	8.557	38297490	23490688	19.280	21.014
Target Compounds						
31) L7 AR-1260-1	7.100	6.125	1603865	1428825	16.275	20.959 #
32) L7 AR-1260-2	7.355	6.314	2838233	1093545	24.469	14.295 #
33) L7 AR-1260-3	7.719	6.467	2564435	1371479	29.958	18.967 #
34) L7 AR-1260-4	7.944	6.938	5050482	2491427	51.084	41.546m
35) L7 AR-1260-5	8.260	7.182	7108986	4203010	35.572	32.893m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030923\
Data File : PP056320.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Mar 2023 16:20
Operator : YP\AJ
Sample : 01829-07
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
SS-07-20230306


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/09/2023
Supervised By :Ankita Jodhani 03/09/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 08 20:34:56 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030823.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 08 02:03:40 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

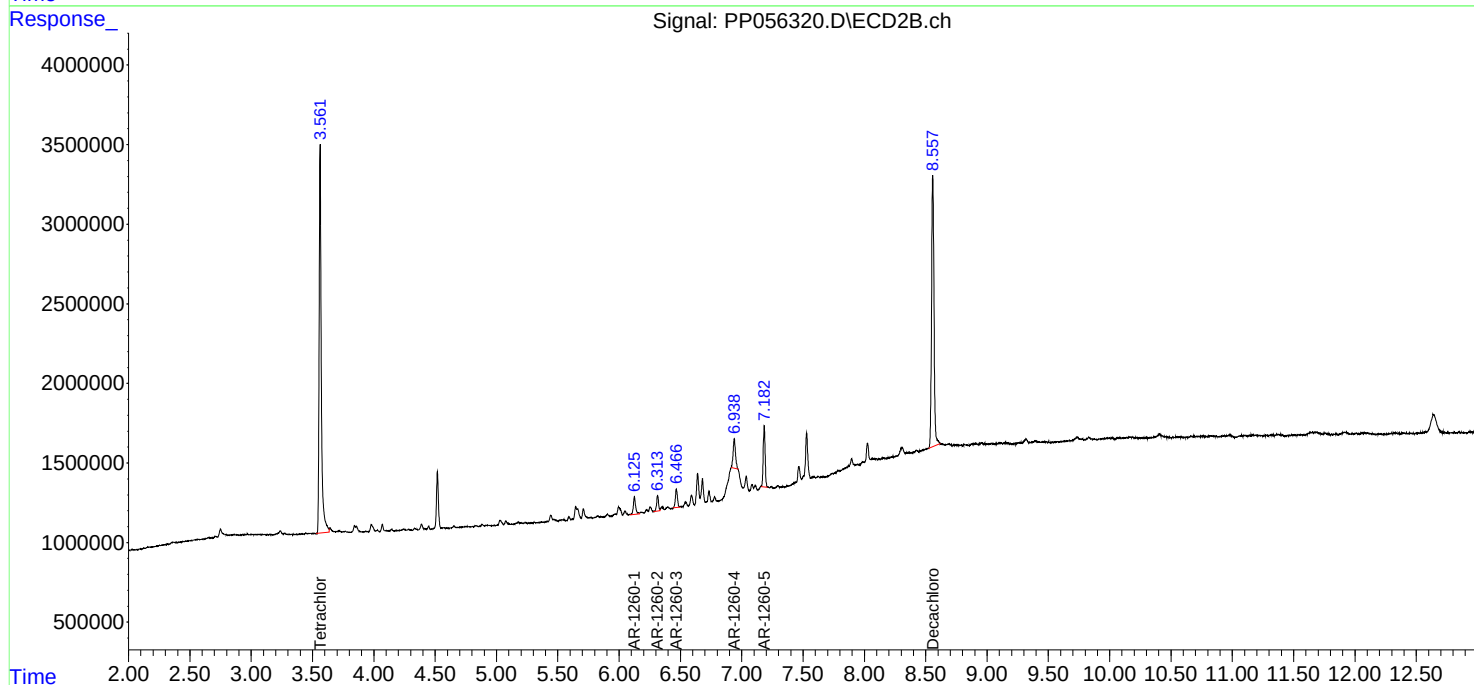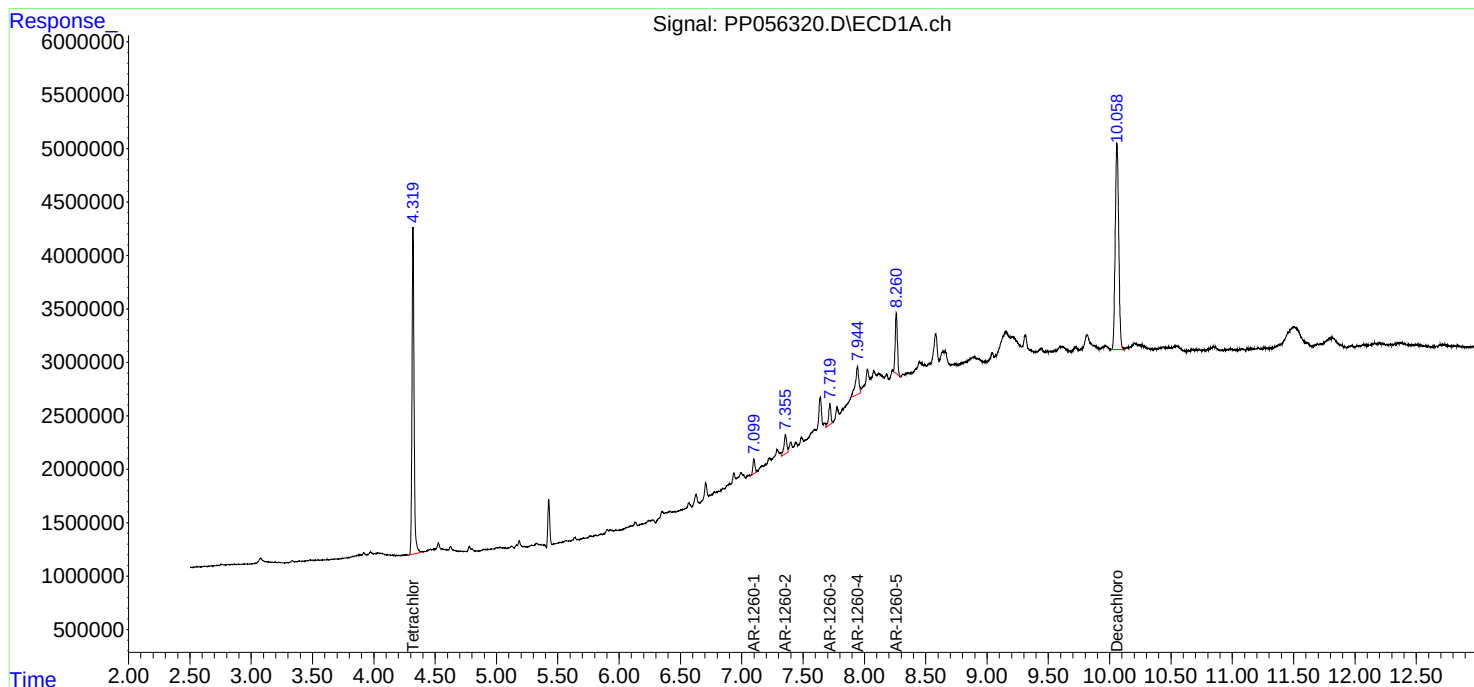

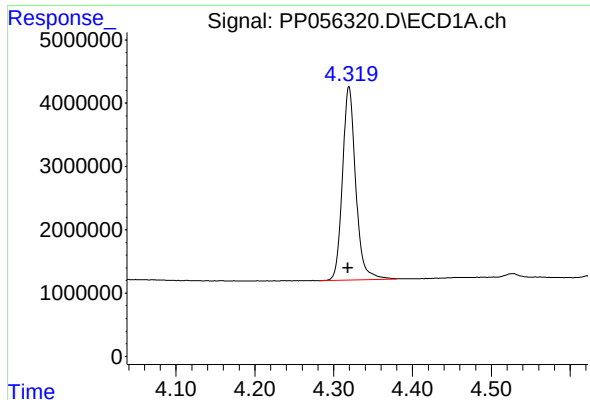


#1 Tetrachloro-m-xylene

R.T.: 4.319 min
Delta R.T.: 0.001 min
Response: 35824382
Conc: 23.07 ng/ml

Instrument :
ECD_P
ClientSampleId :
SS-07-20230306


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/09/2023
Supervised By :Ankita Jodhani 03/09/2023

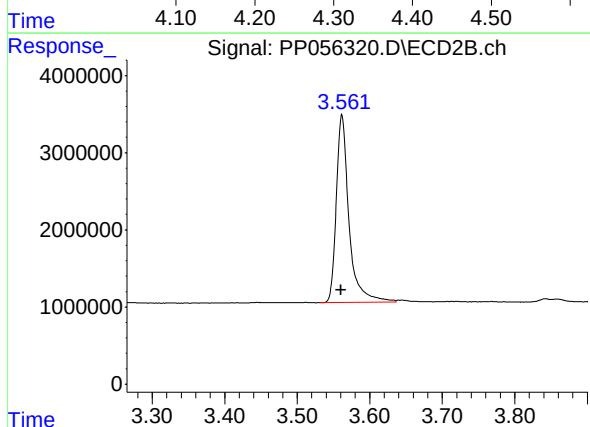


#1 Tetrachloro-m-xylene

R.T.: 3.562 min
Delta R.T.: 0.002 min
Response: 29571467
Conc: 20.96 ng/ml

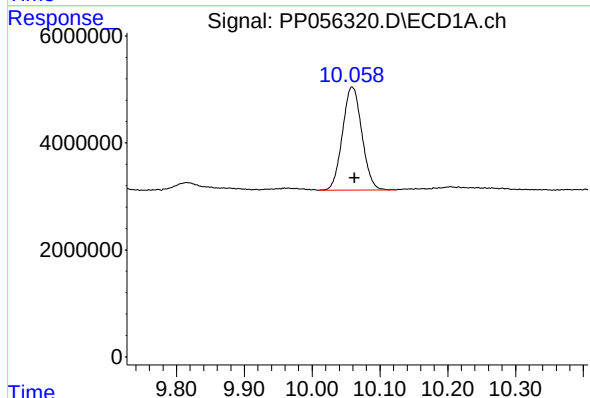


#2 Decachlorobiphenyl

R.T.: 10.059 min
Delta R.T.: -0.004 min
Response: 38297490
Conc: 19.28 ng/ml

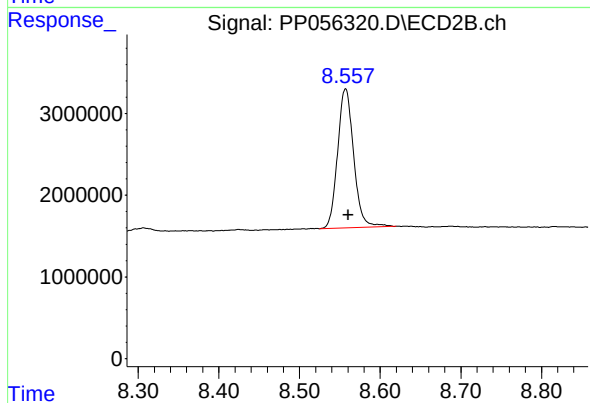

#2 Decachlorobiphenyl

R.T.: 8.557 min
Delta R.T.: -0.003 min
Response: 23490688
Conc: 21.01 ng/ml

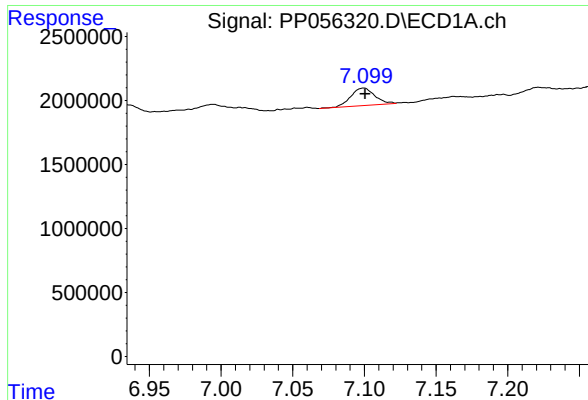


#31 AR-1260-1

R.T.: 7.100 min
Delta R.T.: 0.000 min
Response: 1603865
Conc: 16.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
SS-07-20230306


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/09/2023
Supervised By :Ankita Jodhani 03/09/2023

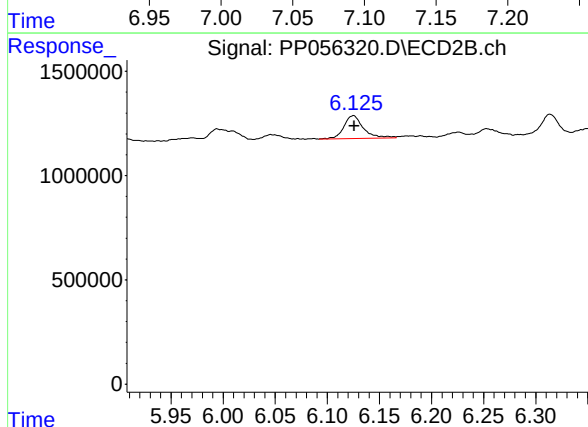


#31 AR-1260-1

R.T.: 6.125 min
Delta R.T.: 0.000 min
Response: 1428825
Conc: 20.96 ng/ml

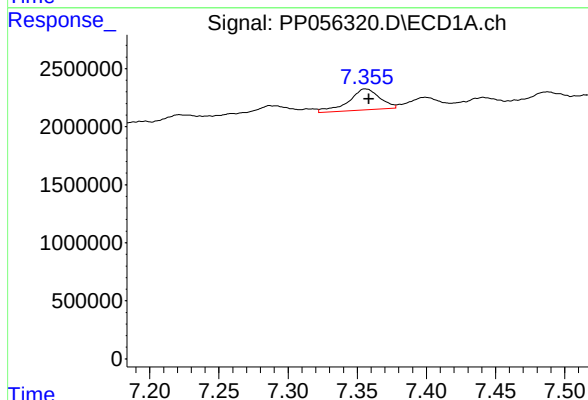


#32 AR-1260-2

R.T.: 7.355 min
Delta R.T.: -0.003 min
Response: 2838233
Conc: 24.47 ng/ml

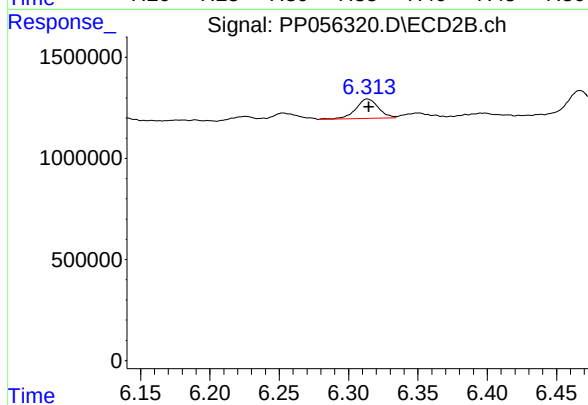

#32 AR-1260-2

R.T.: 6.314 min
Delta R.T.: -0.001 min
Response: 1093545
Conc: 14.30 ng/ml

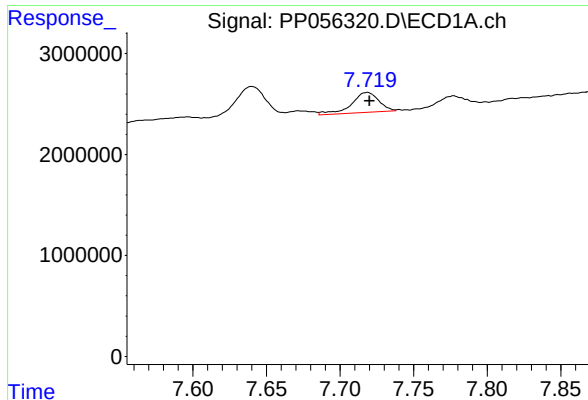


#33 AR-1260-3

R.T.: 7.719 min
Delta R.T.: -0.001 min
Response: 2564435
Conc: 29.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
SS-07-20230306


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/09/2023
Supervised By :Ankita Jodhani 03/09/2023

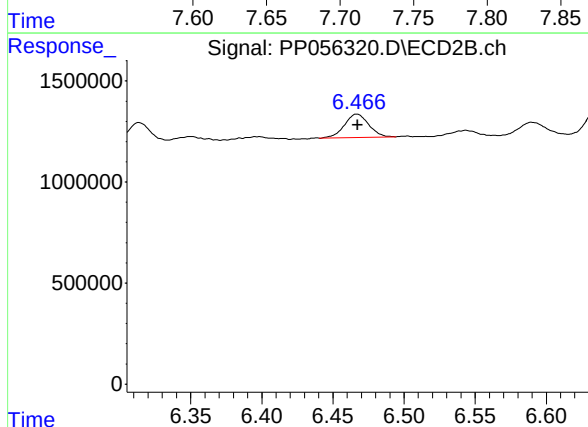


#33 AR-1260-3

R.T.: 6.467 min
Delta R.T.: 0.000 min
Response: 1371479
Conc: 18.97 ng/ml

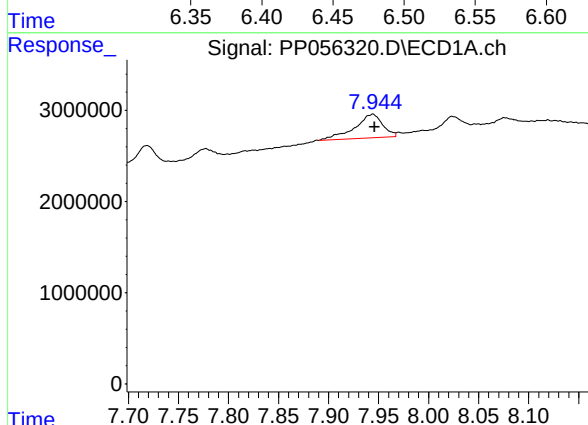


#34 AR-1260-4

R.T.: 7.944 min
Delta R.T.: -0.002 min
Response: 5050482
Conc: 51.08 ng/ml

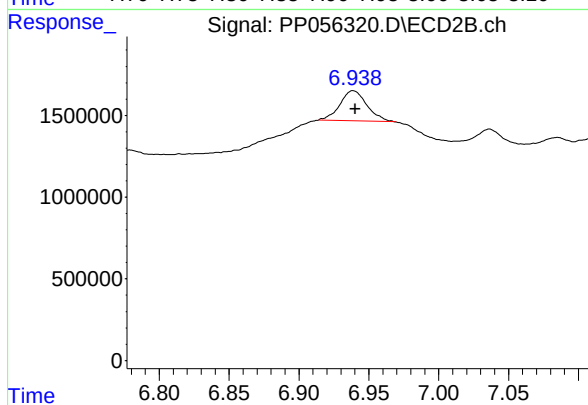

#34 AR-1260-4

R.T.: 6.938 min
Delta R.T.: -0.002 min
Response: 2491427
Conc: 41.55 ng/ml m

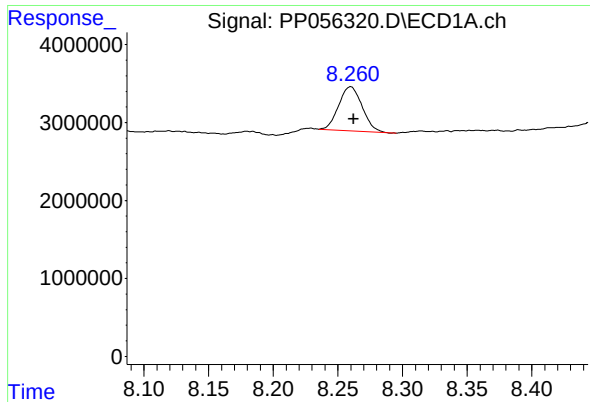


#35 AR-1260-5

R.T.: 8.260 min
Delta R.T.: -0.002 min
Response: 7108986
Conc: 35.57 ng/ml

Instrument :
ECD_P
ClientSampleId :
SS-07-20230306

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/09/2023
Supervised By :Ankita Jodhani 03/09/2023

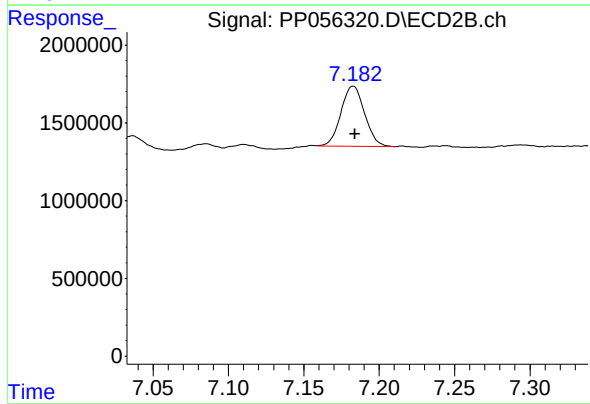

#35 AR-1260-5

R.T.: 7.182 min
Delta R.T.: -0.002 min
Response: 4203010
Conc: 32.89 ng/ml