

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030923\
 Data File : PP056331.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Mar 2023 20:03
 Operator : YP\AJ
 Sample : 01829-13
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SS-11-20230306

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/09/2023
 Supervised By :Ankita Jodhani 03/09/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 09 04:18:57 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 08 02:03:40 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.321	3.562	29349067	21654384	18.902	15.346
2) SA Decachlor...	10.064	8.562	39994543	25525674	20.135m	22.834

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP030923\
Data File : PP056331.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Mar 2023 20:03
Operator : YP\AJ
Sample : 01829-13
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
SS-11-20230306


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/09/2023
Supervised By :Ankita Jodhani 03/09/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 09 04:18:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030823.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 08 02:03:40 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

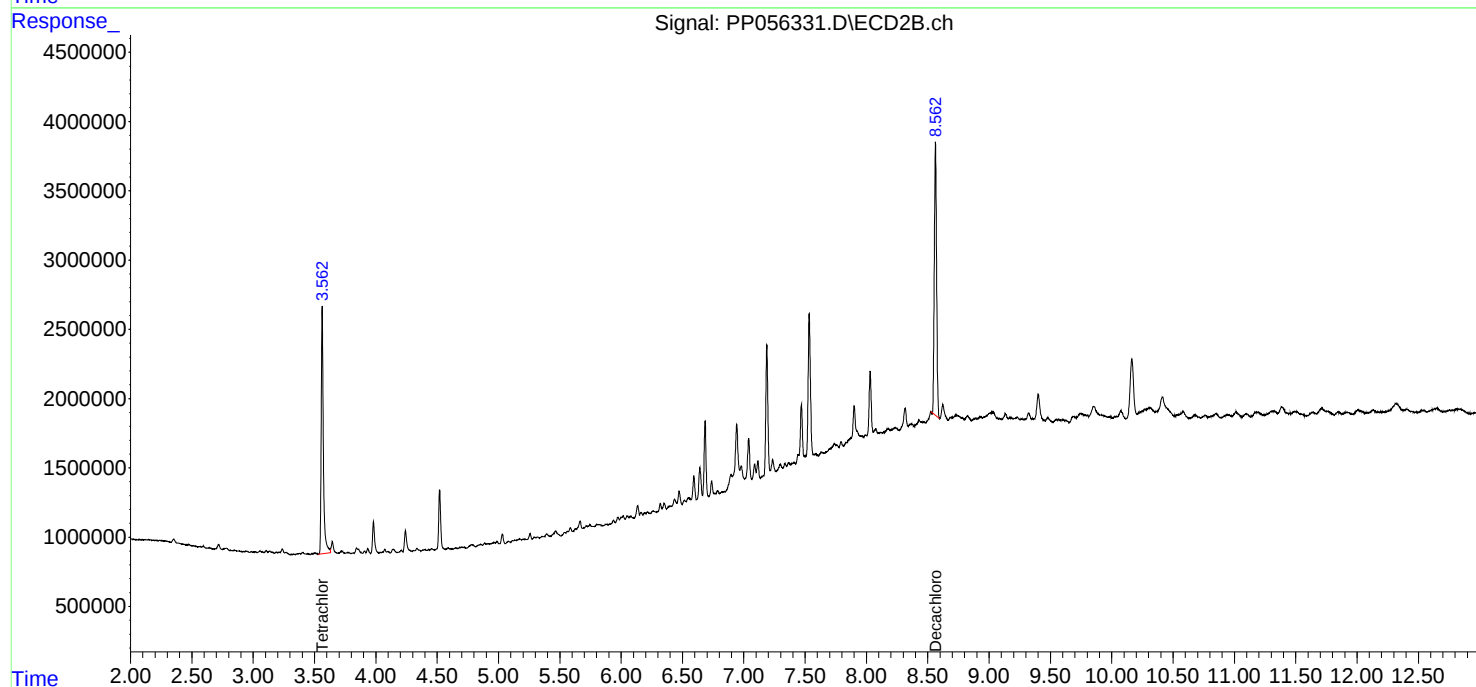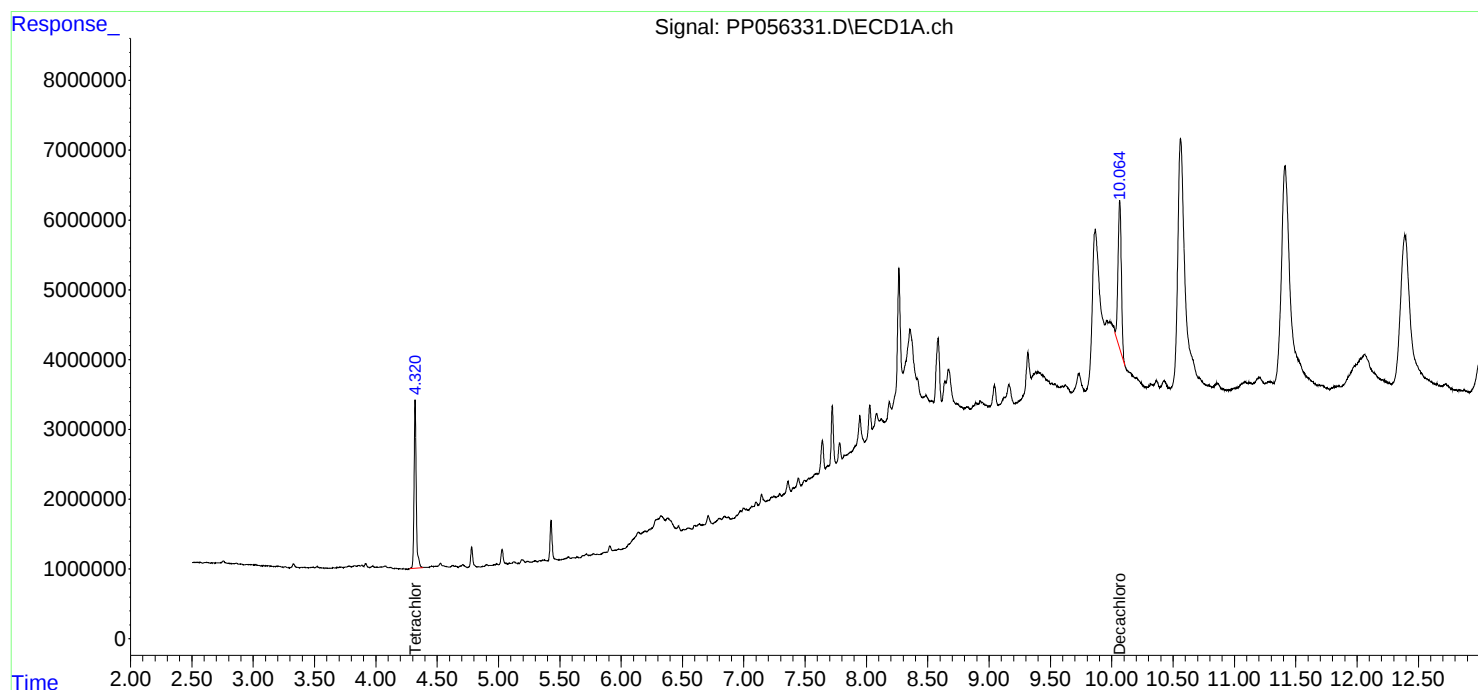

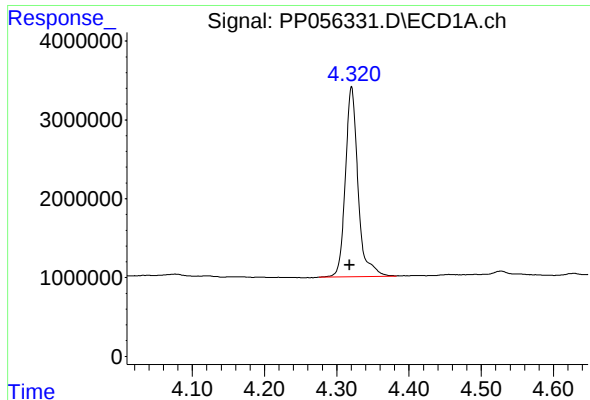


#1 Tetrachloro-m-xylene

R.T.: 4.321 min
Delta R.T.: 0.003 min
Response: 29349067
Conc: 18.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
SS-11-20230306


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/09/2023
Supervised By :Ankita Jodhani 03/09/2023

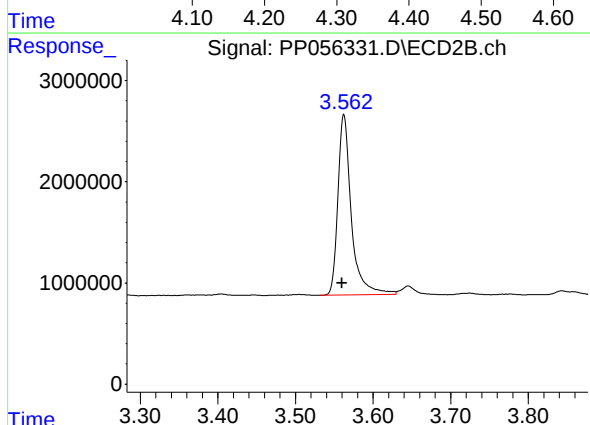


#1 Tetrachloro-m-xylene

R.T.: 3.562 min
Delta R.T.: 0.002 min
Response: 21654384
Conc: 15.35 ng/ml

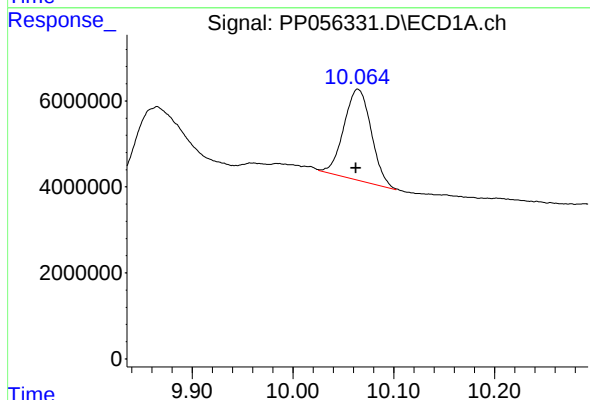

#2 Decachlorobiphenyl

R.T.: 10.064 min
Delta R.T.: 0.001 min
Response: 39994543
Conc: 20.13 ng/ml m

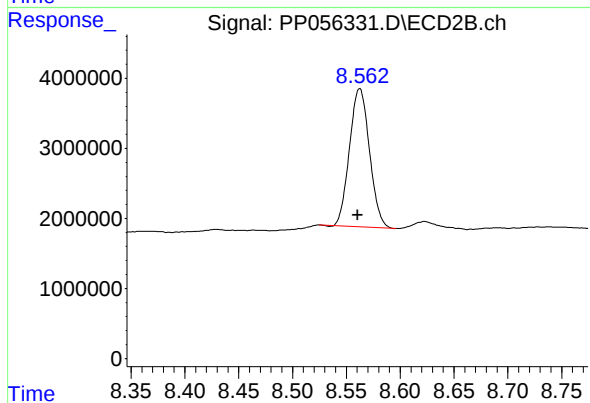

#2 Decachlorobiphenyl

R.T.: 8.562 min
Delta R.T.: 0.002 min
Response: 25525674
Conc: 22.83 ng/ml