

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031021\
 Data File : PP033843.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 10 Mar 2021 22:29
 Operator : DD\AJ
 Sample : PB135069BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PB135069BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 01:23:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 10 03:01:34 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.857	4.268	1813924	858525	20.964	21.133
2) SA Decachlor...	10.783	9.594	1832665	589712	21.700	22.099

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031021\
Data File : PP033843.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Mar 2021 22:29
Operator : DD\AJ
Sample : PB135069BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PB135069BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 01:23:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 10 03:01:34 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

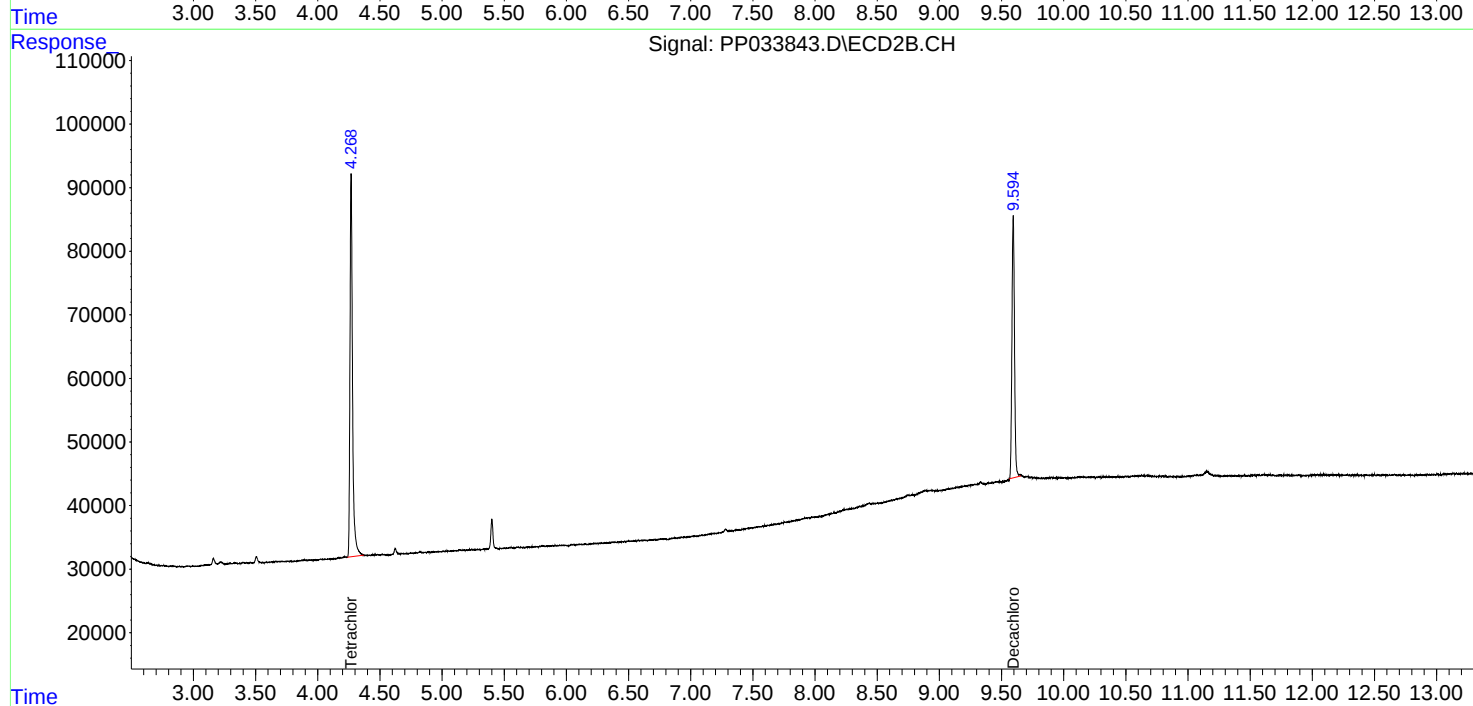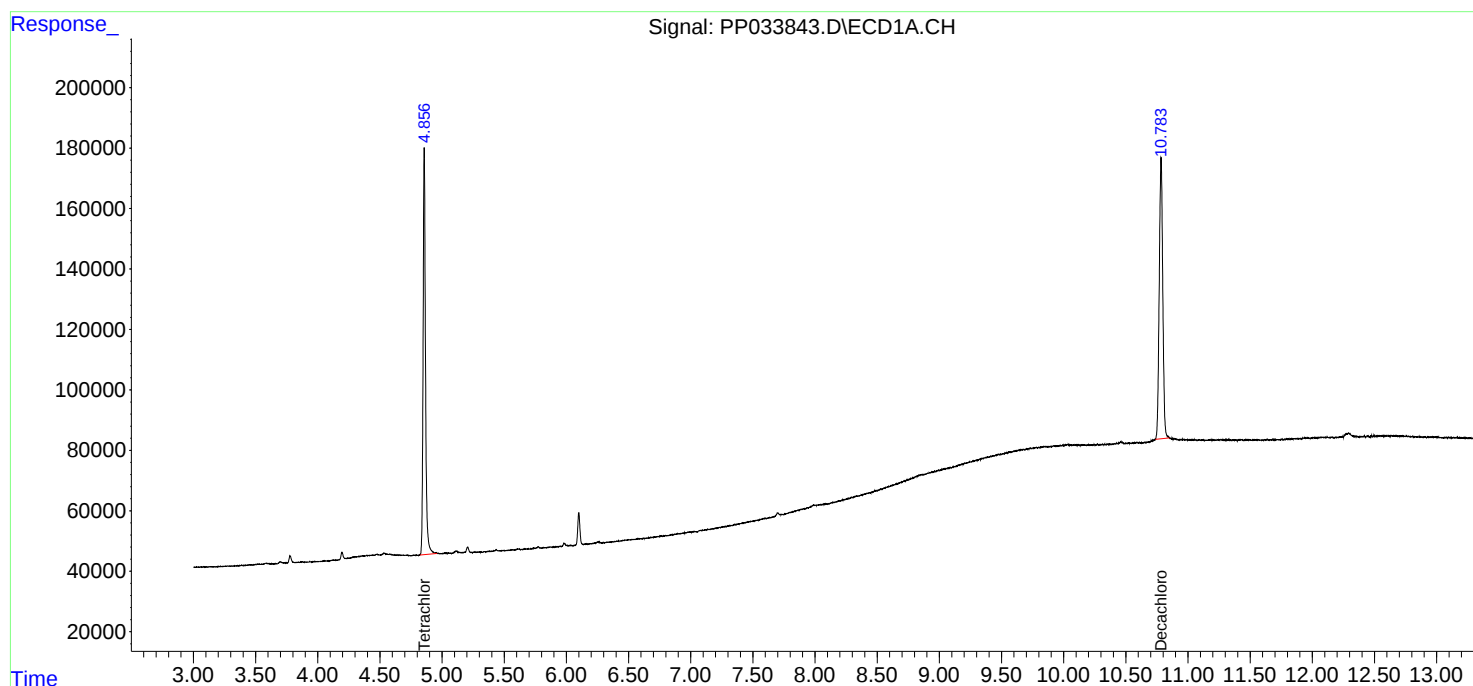


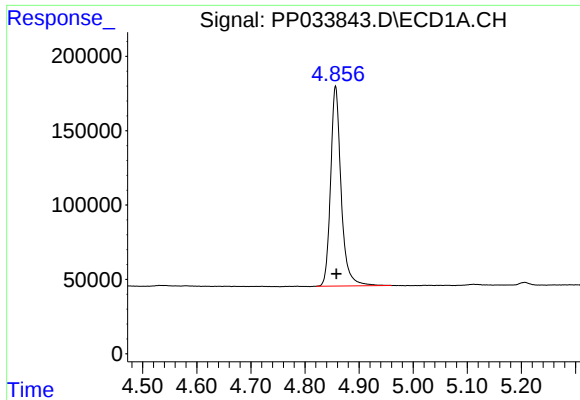

#1 Tetrachloro-m-xylene


R.T.: 4.857 min
Delta R.T.: -0.001 min
Response: 1813924
Conc: 20.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB135069BL

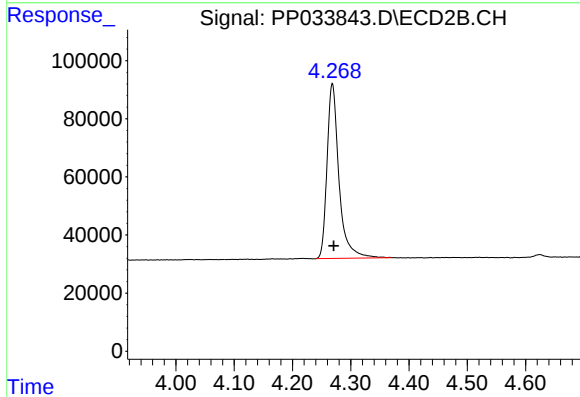


#1 Tetrachloro-m-xylene

R.T.: 4.268 min
Delta R.T.: -0.003 min
Response: 858525
Conc: 21.13 ng/ml

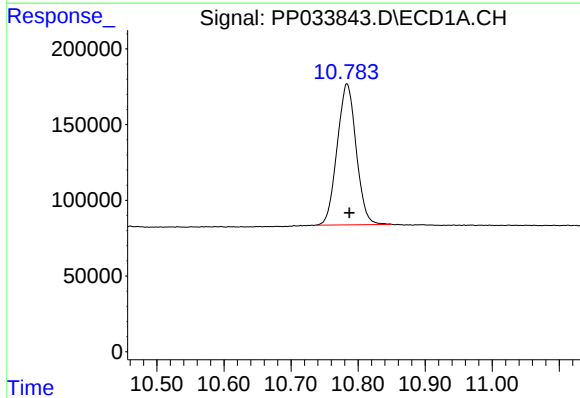

#2 Decachlorobiphenyl

R.T.: 10.783 min
Delta R.T.: -0.004 min
Response: 1832665
Conc: 21.70 ng/ml

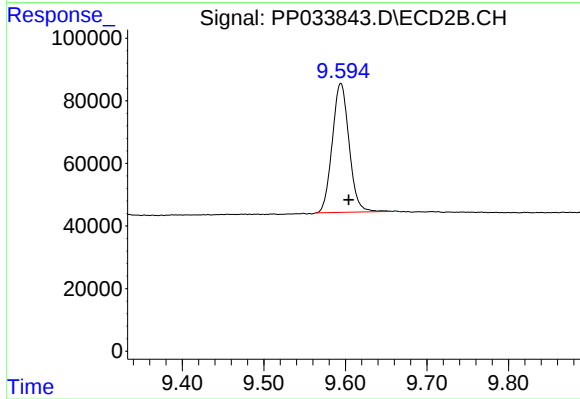

#2 Decachlorobiphenyl

R.T.: 9.594 min
Delta R.T.: -0.010 min
Response: 589712
Conc: 22.10 ng/ml