

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031021\
 Data File : PP033871.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Mar 2021 7:45
 Operator : DD\AJ
 Sample : M1458-09
 Misc : AR1254 MDL 25 PPB
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT1-2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 08:17:26 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 10 03:01:34 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.856	4.268	1263810	610539	14.606	15.028
2)	SA Decachlor...	10.782	9.593	1260716	417626	14.928	15.650
Target Compounds							
26)	L6 AR-1254-1	7.073	6.396	104971	49691	36.815	30.204
27)	L6 AR-1254-2	7.303	6.553	140161	42982	31.929	29.999
28)	L6 AR-1254-3	7.683	6.974	152372	69144	32.111	29.953
29)	L6 AR-1254-4	7.978	7.210	107756	31150	31.931	24.083
30)	L6 AR-1254-5	8.405	7.638	100606	49477	26.854	25.475



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031021\
Data File : PP033871.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Mar 2021 7:45
Operator : DD\AJ
Sample : M1458-09
Misc : AR1254 MDL 25 PPB
ALS Vial : 45 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 08:17:26 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030921.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 10 03:01:34 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

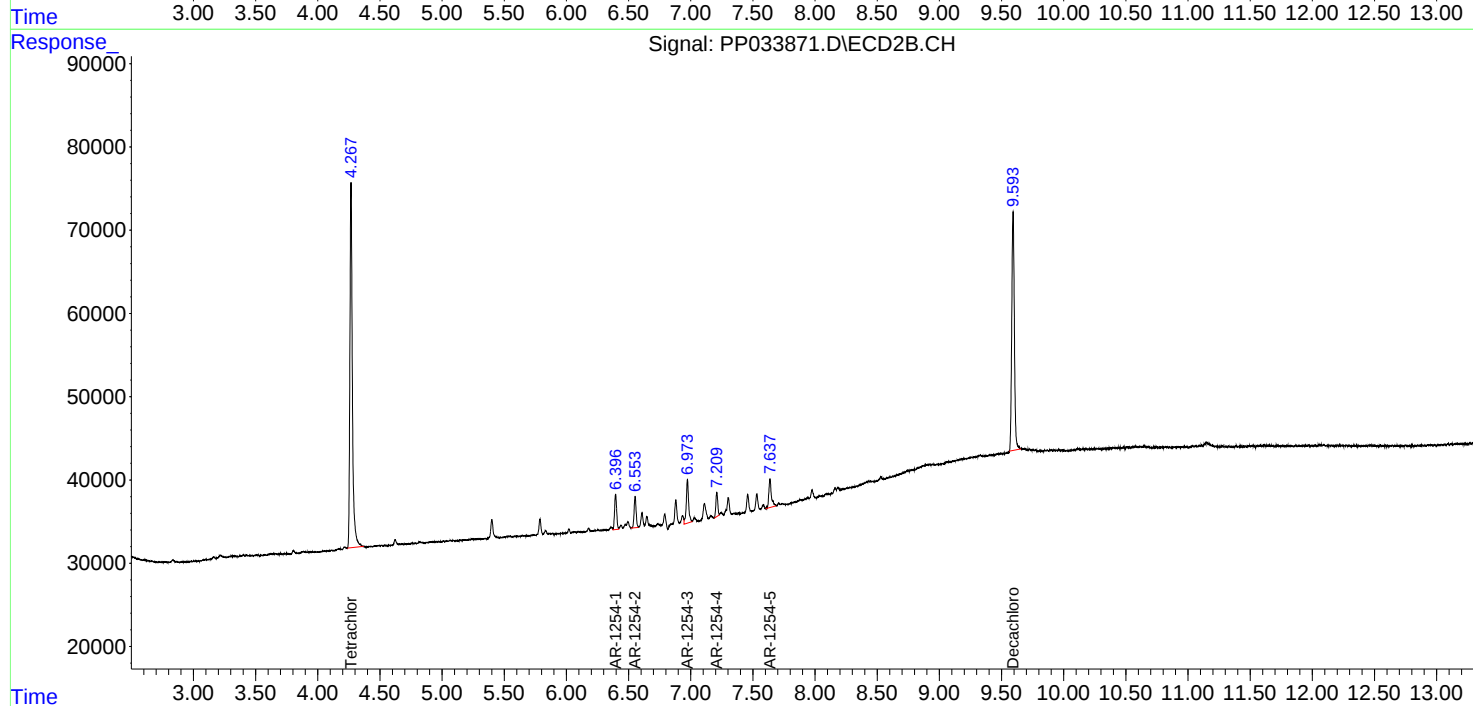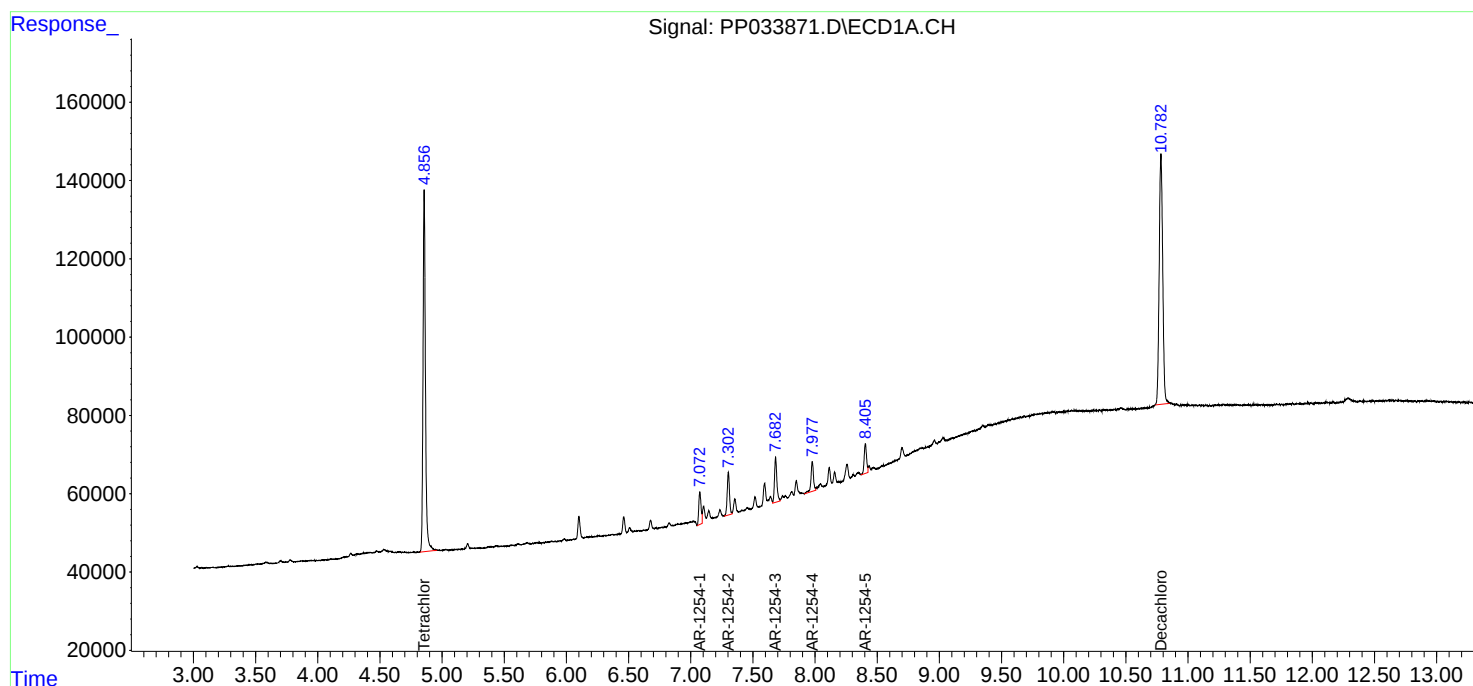


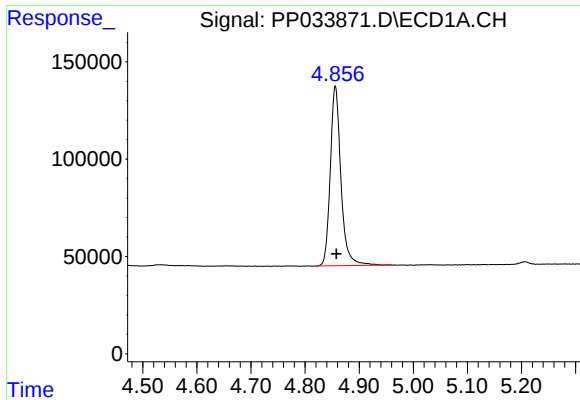

#1 Tetrachloro-m-xylene


R.T.: 4.856 min
Delta R.T.: -0.002 min
Response: 1263810
Conc: 14.61 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2021

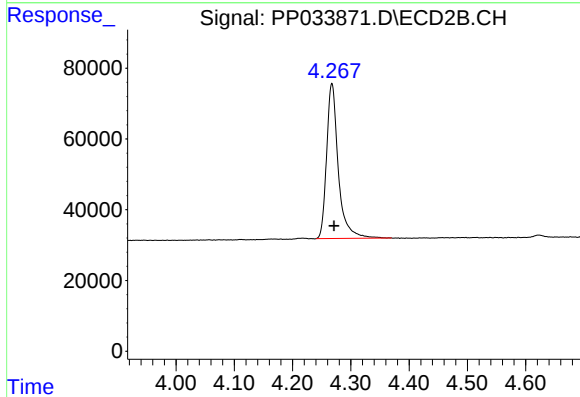


#1 Tetrachloro-m-xylene

R.T.: 4.268 min
Delta R.T.: -0.004 min
Response: 610539
Conc: 15.03 ng/ml

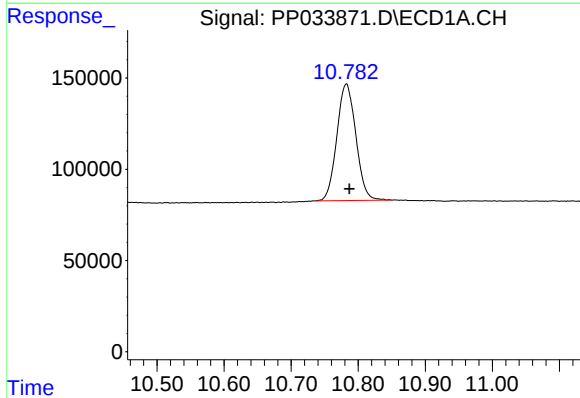


#2 Decachlorobiphenyl

R.T.: 10.782 min
Delta R.T.: -0.005 min
Response: 1260716
Conc: 14.93 ng/ml

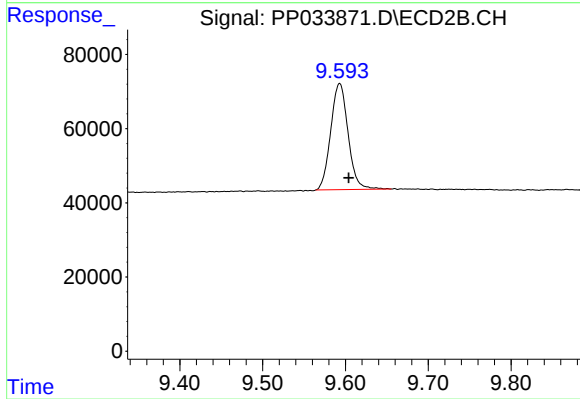

#2 Decachlorobiphenyl


R.T.: 9.593 min
Delta R.T.: -0.011 min
Response: 417626
Conc: 15.65 ng/ml

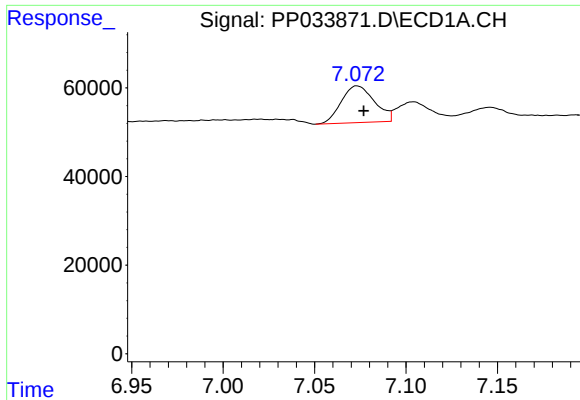

#26 AR-1254-1


R.T.: 7.073 min
Delta R.T.: -0.004 min
Response: 104971
Conc: 36.82 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2021

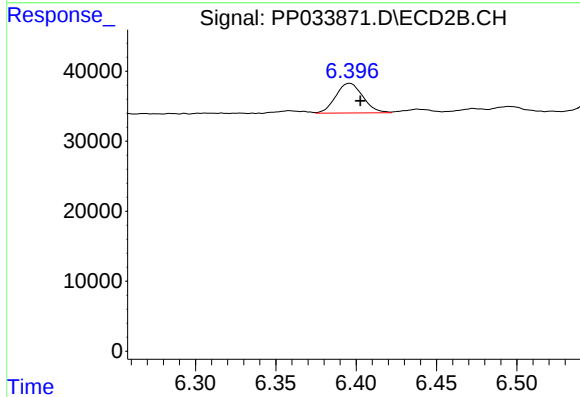


#26 AR-1254-1

R.T.: 6.396 min
Delta R.T.: -0.007 min
Response: 49691
Conc: 30.20 ng/ml

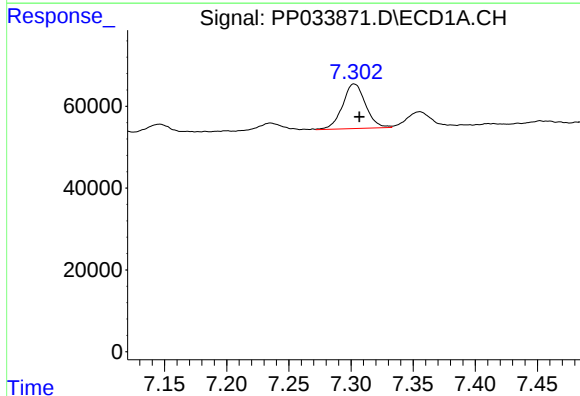


#27 AR-1254-2

R.T.: 7.303 min
Delta R.T.: -0.004 min
Response: 140161
Conc: 31.93 ng/ml

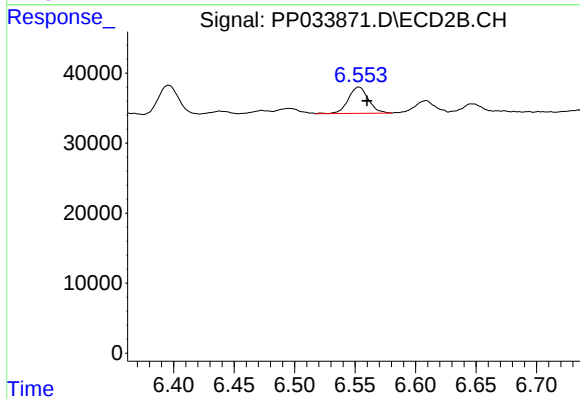

#27 AR-1254-2


R.T.: 6.553 min
Delta R.T.: -0.007 min
Response: 42982
Conc: 30.00 ng/ml

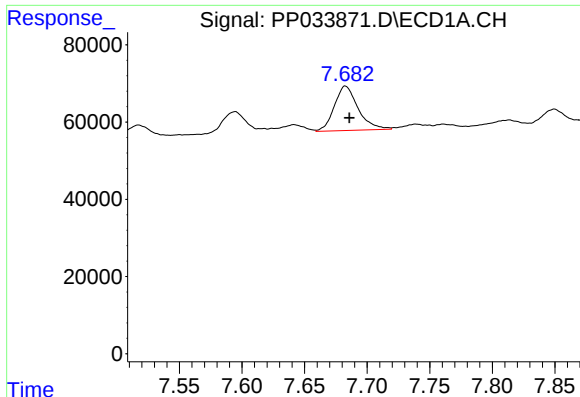

#28 AR-1254-3


R.T.: 7.683 min
Delta R.T.: -0.003 min
Response: 152372
Conc: 32.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2021

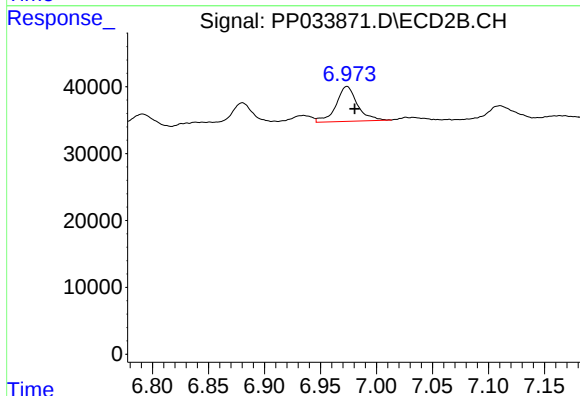


#28 AR-1254-3

R.T.: 6.974 min
Delta R.T.: -0.007 min
Response: 69144
Conc: 29.95 ng/ml

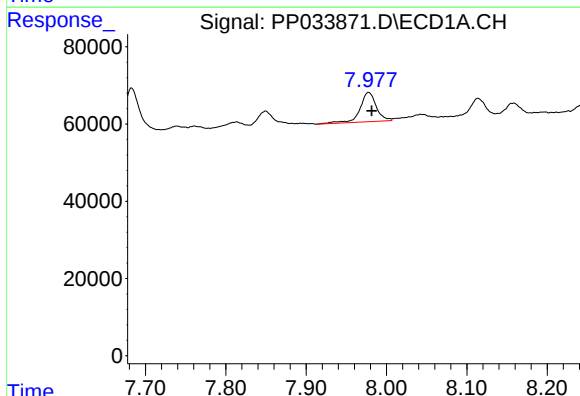


#29 AR-1254-4

R.T.: 7.978 min
Delta R.T.: -0.004 min
Response: 107756
Conc: 31.93 ng/ml

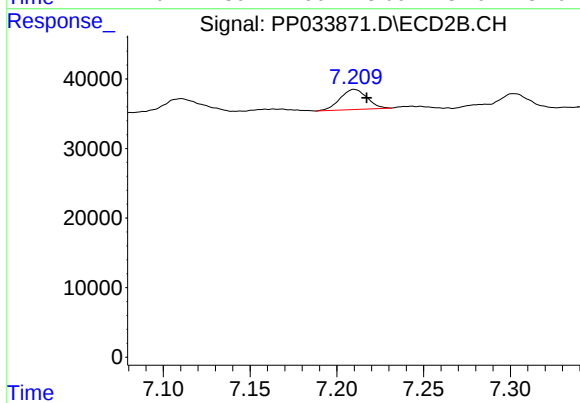

#29 AR-1254-4


R.T.: 7.210 min
Delta R.T.: -0.007 min
Response: 31150
Conc: 24.08 ng/ml

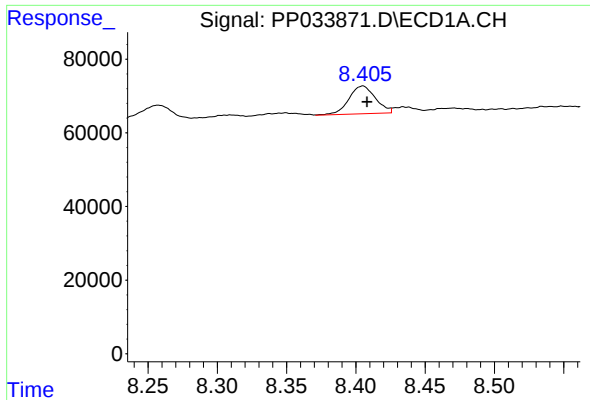

#30 AR-1254-5

R.T.: 8.405 min
Delta R.T.: -0.003 min
Response: 100606
Conc: 26.85 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT1-2021

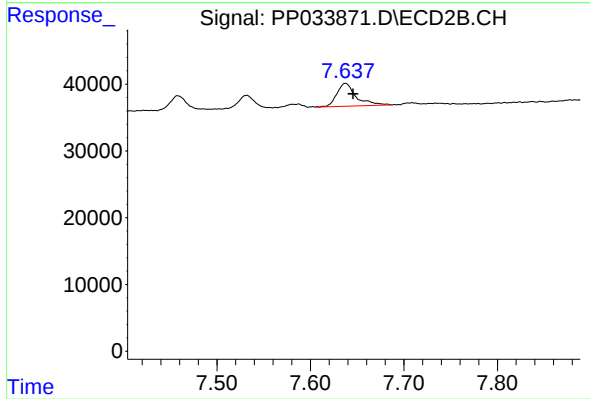

#30 AR-1254-5

R.T.: 7.638 min
Delta R.T.: -0.008 min
Response: 49477
Conc: 25.47 ng/ml