

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031022\
 Data File : PP044527.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Mar 2022 04:10
 Operator : YP\AJ
 Sample : N1864-09
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MB-B2-030922-4-6-DUP

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/11/2022
 Supervised By :Ankita Jodhani 03/11/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 11 05:14:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030222.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Mar 03 02:21:53 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.909	3.165	43257494	39095423	20.877	22.347
2) SA Decachlor...	10.042	8.529	27826637	26141889	20.218	17.042m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031022\
Data File : PP044527.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Mar 2022 04:10
Operator : YP\AJ
Sample : N1864-09
Misc :
ALS Vial : 62 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
MB-B2-030922-4-6-DUP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/11/2022
Supervised By :Ankita Jodhani 03/11/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 11 05:14:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030222.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Mar 03 02:21:53 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

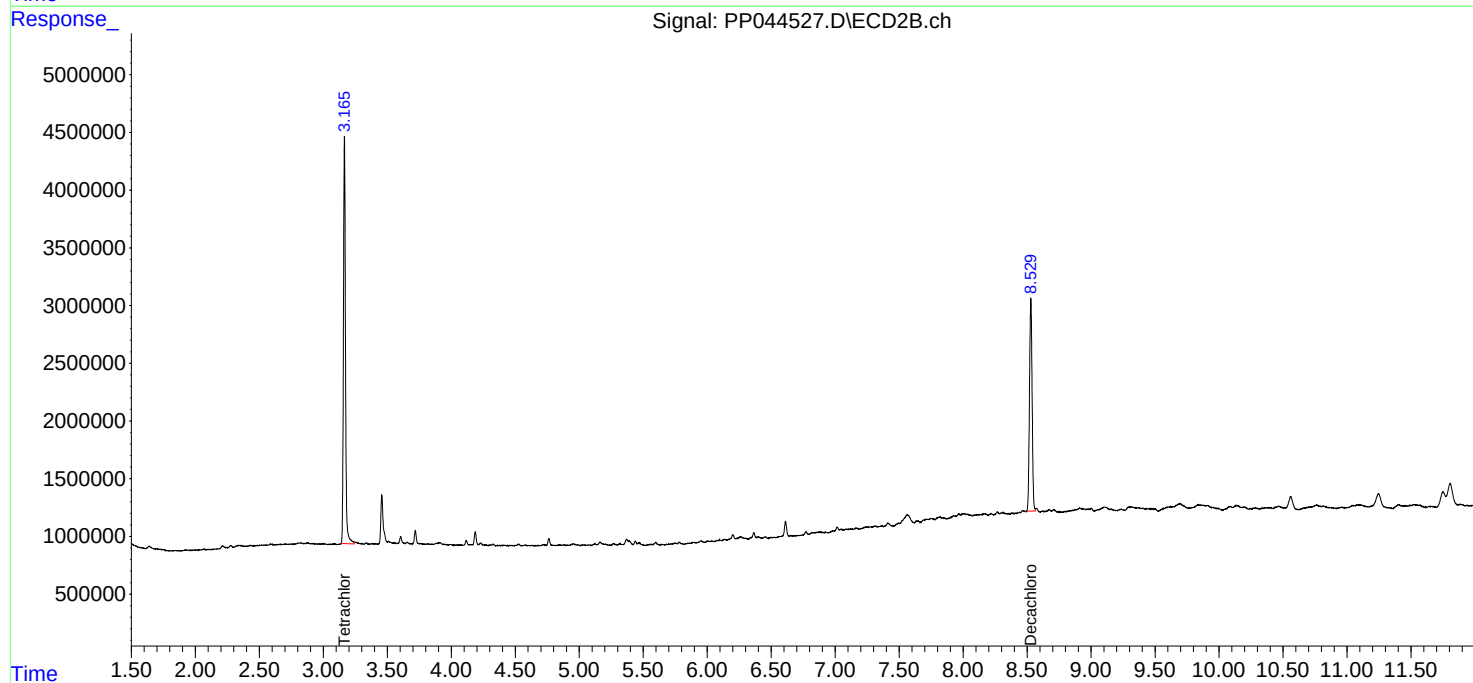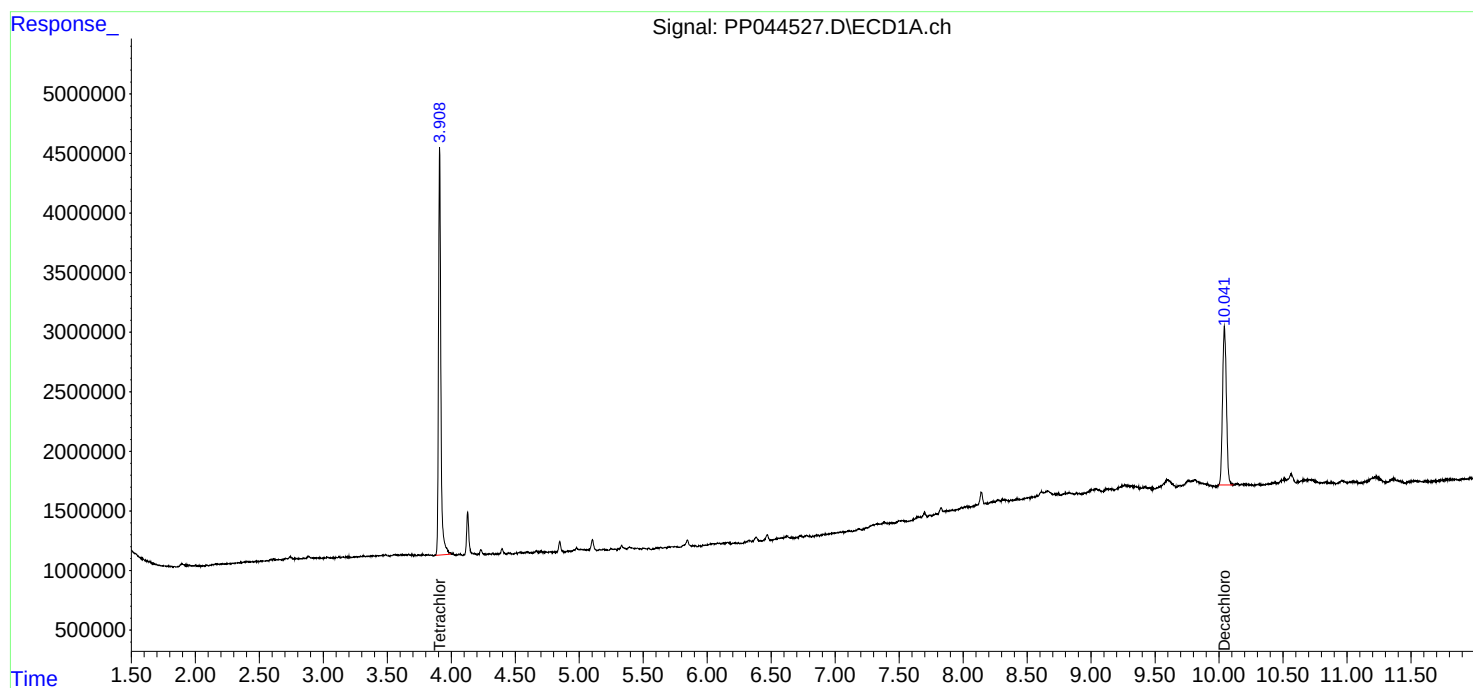

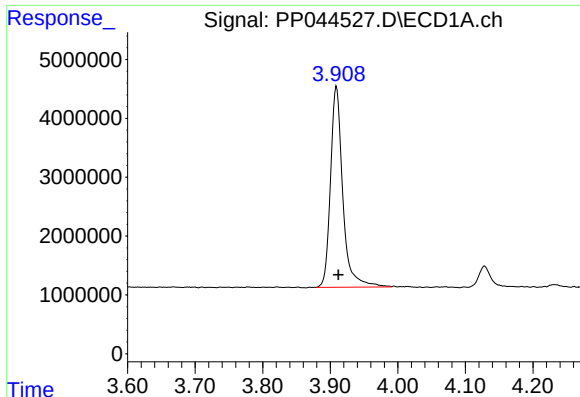


#1 Tetrachloro-m-xylene

R.T.: 3.909 min
Delta R.T.: -0.003 min
Response: 43257494
Conc: 20.88 ng/ml

Instrument :
ECD_P
ClientSampleId :
MB-B2-030922-4-6-DUP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/11/2022
Supervised By :Ankita Jodhani 03/11/2022

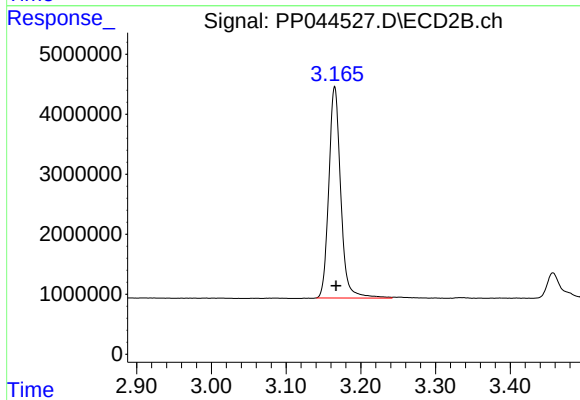


#1 Tetrachloro-m-xylene

R.T.: 3.165 min
Delta R.T.: -0.002 min
Response: 39095423
Conc: 22.35 ng/ml

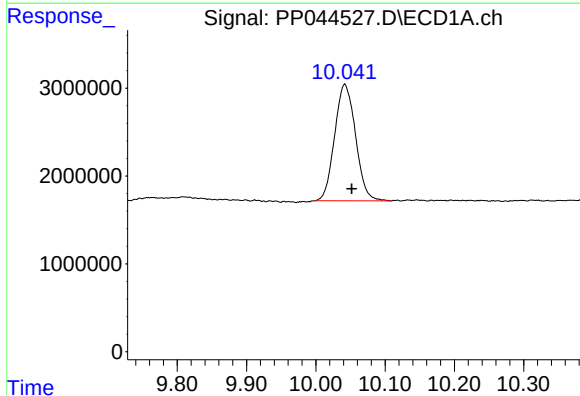

#2 Decachlorobiphenyl

R.T.: 10.042 min
Delta R.T.: -0.010 min
Response: 27826637
Conc: 20.22 ng/ml

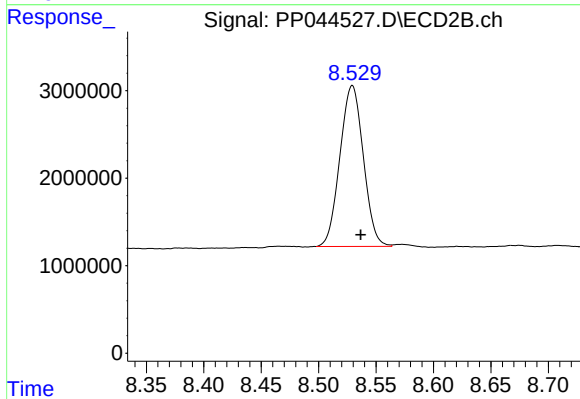

#2 Decachlorobiphenyl

R.T.: 8.529 min
Delta R.T.: -0.008 min
Response: 26141889
Conc: 17.04 ng/ml m