

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031023\
 Data File : PP056345.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Mar 2023 09:57
 Operator : YP\AJ
 Sample : 01829-07
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SS-07-20230306

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/10/2023
 Supervised By :Ankita Jodhani 03/10/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 09 20:08:05 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 08 02:03:40 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.319	3.560	37073253	29882901	23.876	21.177
2)	SA Decachlor...	10.058	8.556	39543931	24489670	19.908	21.908
Target Compounds							
31)	L7 AR-1260-1	7.098	6.123	2182881	1242005	22.150m	18.219m
32)	L7 AR-1260-2	7.359	6.311	2224635	1315090	19.179m	17.191m
33)	L7 AR-1260-3	7.717	6.466	2527834	1490042	29.530m	20.606 #
34)	L7 AR-1260-4	7.942	6.937	3480606	1966944	35.205m	32.800
35)	L7 AR-1260-5	8.260	7.180	6889057	4330200	34.472	33.888m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031023\
Data File : PP056345.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Mar 2023 09:57
Operator : YP\AJ
Sample : 01829-07
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
SS-07-20230306


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/10/2023
Supervised By :Ankita Jodhani 03/10/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 09 20:08:05 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030823.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 08 02:03:40 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

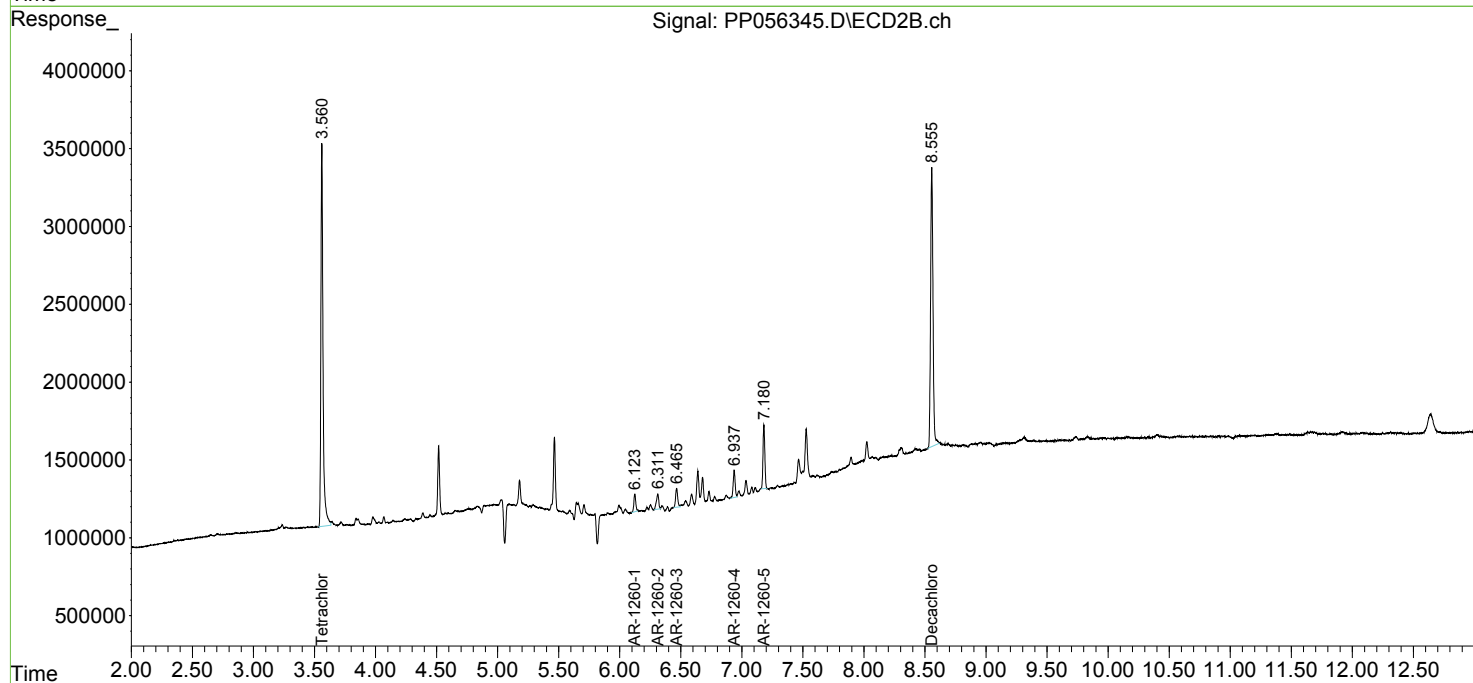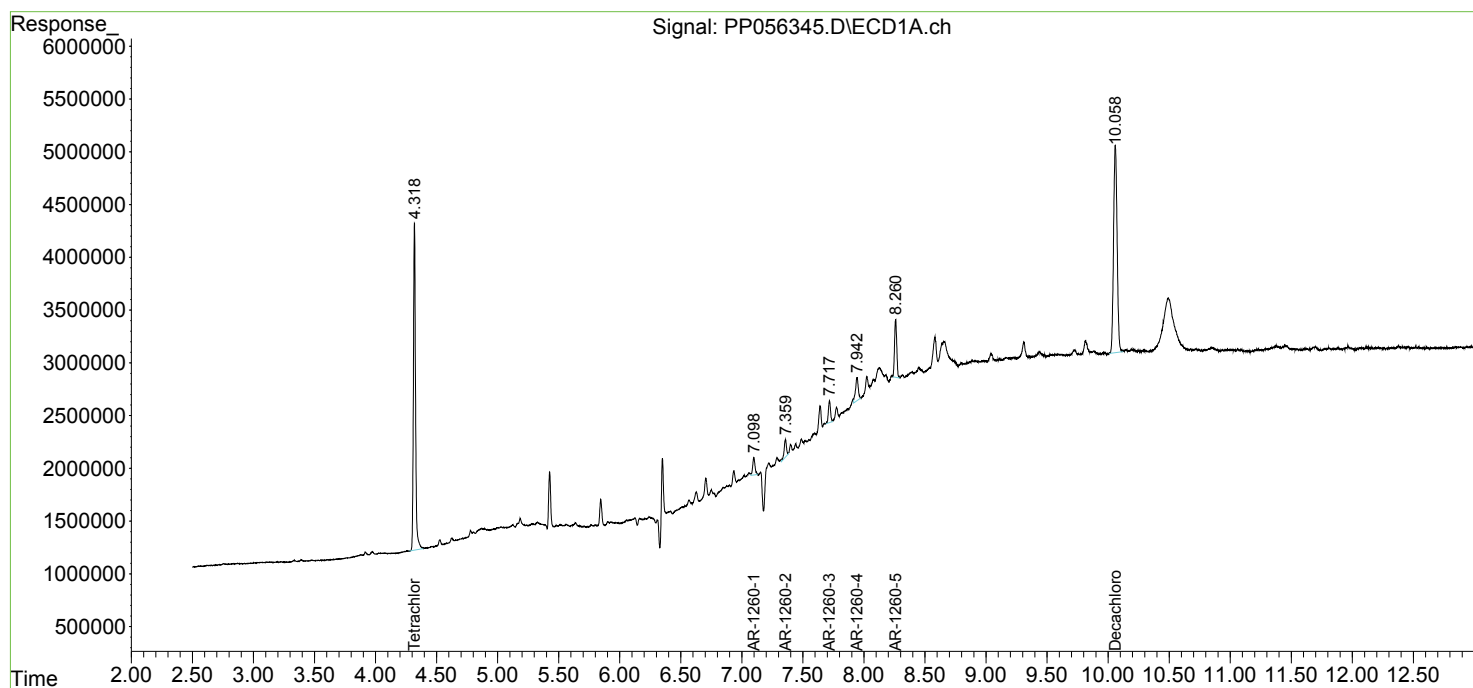

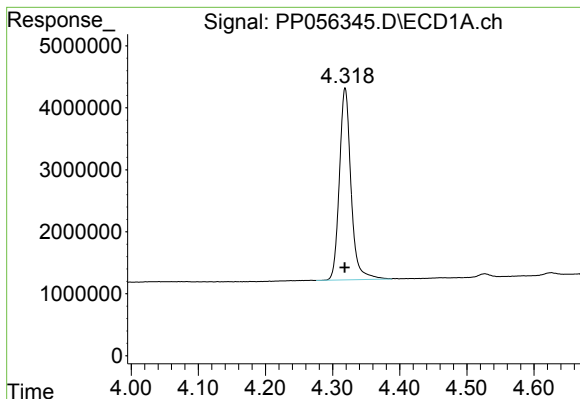


#1 Tetrachloro-m-xylene

R.T.: 4.319 min
Delta R.T.: 0.000 min
Response: 37073253
Conc: 23.88 ng/ml

Instrument :
ECD_P
ClientSampleId :
SS-07-20230306


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/10/2023
Supervised By :Ankita Jodhani 03/10/2023

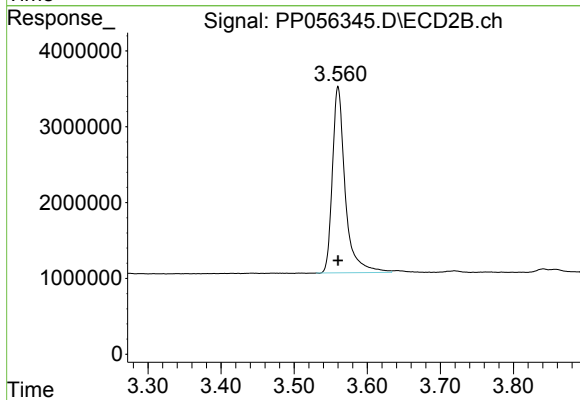


#1 Tetrachloro-m-xylene

R.T.: 3.560 min
Delta R.T.: 0.000 min
Response: 29882901
Conc: 21.18 ng/ml

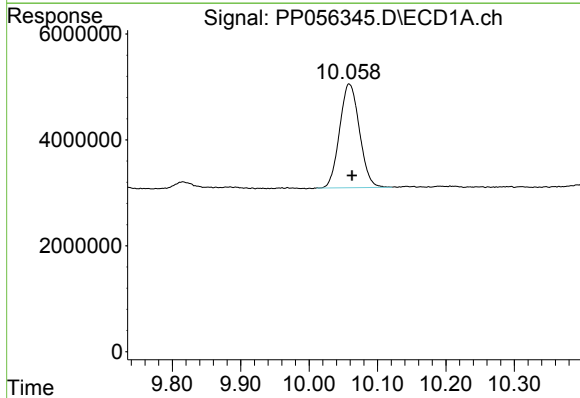


#2 Decachlorobiphenyl

R.T.: 10.058 min
Delta R.T.: -0.004 min
Response: 39543931
Conc: 19.91 ng/ml

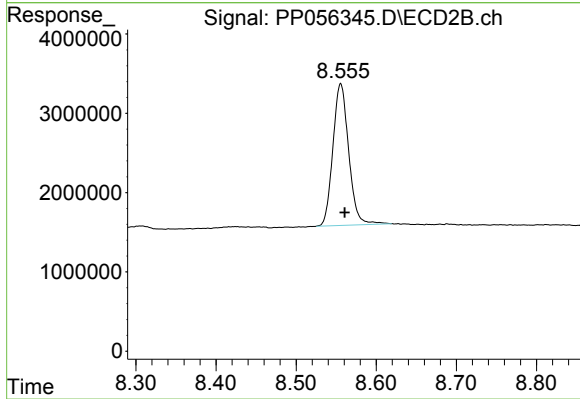

#2 Decachlorobiphenyl

R.T.: 8.556 min
Delta R.T.: -0.005 min
Response: 24489670
Conc: 21.91 ng/ml

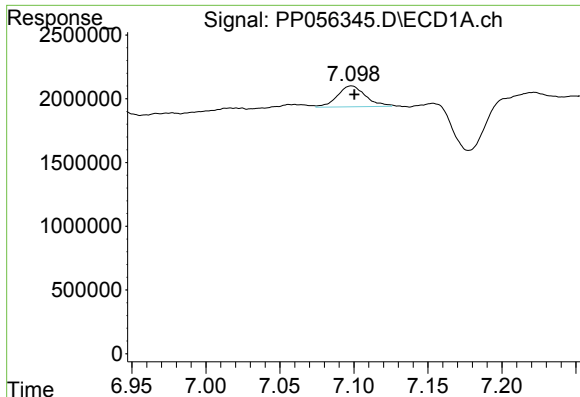


#31 AR-1260-1

R.T.: 7.098 min
Delta R.T.: -0.003 min
Response: 2182881
Conc: 22.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
SS-07-20230306


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/10/2023
Supervised By :Ankita Jodhani 03/10/2023

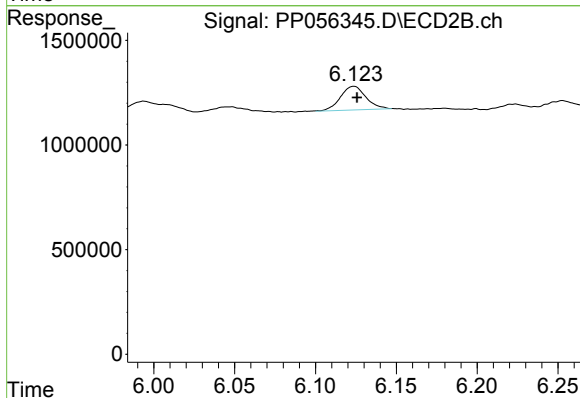


#31 AR-1260-1

R.T.: 6.123 min
Delta R.T.: -0.002 min
Response: 1242005
Conc: 18.22 ng/ml m

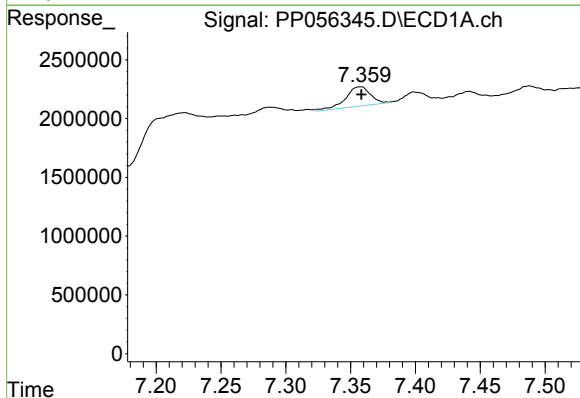


#32 AR-1260-2

R.T.: 7.359 min
Delta R.T.: 0.000 min
Response: 2224635
Conc: 19.18 ng/ml m

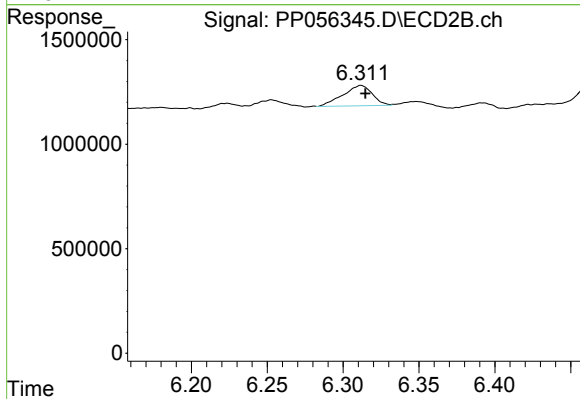

#32 AR-1260-2

R.T.: 6.311 min
Delta R.T.: -0.004 min
Response: 1315090
Conc: 17.19 ng/ml m

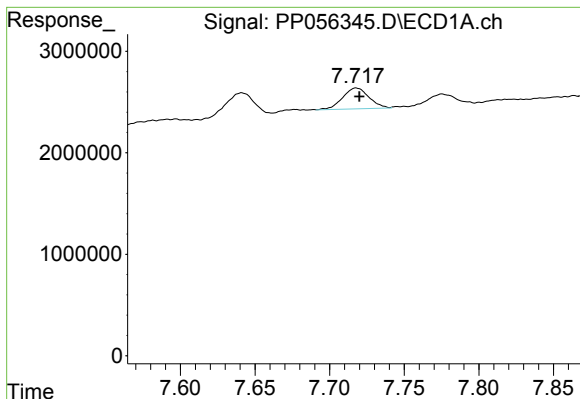


#33 AR-1260-3

R.T.: 7.717 min
Delta R.T.: -0.003 min
Response: 2527834
Conc: 29.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
SS-07-20230306


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/10/2023
Supervised By :Ankita Jodhani 03/10/2023

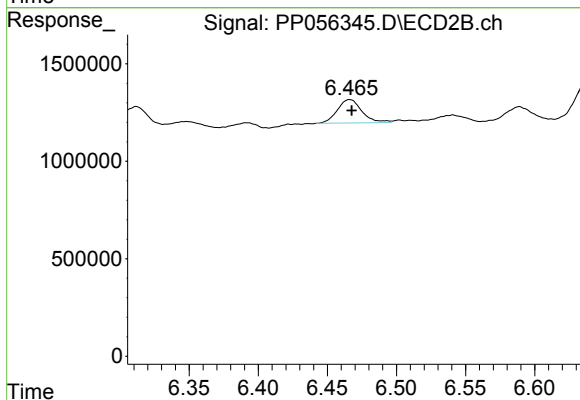


#33 AR-1260-3

R.T.: 6.466 min
Delta R.T.: -0.001 min
Response: 1490042
Conc: 20.61 ng/ml

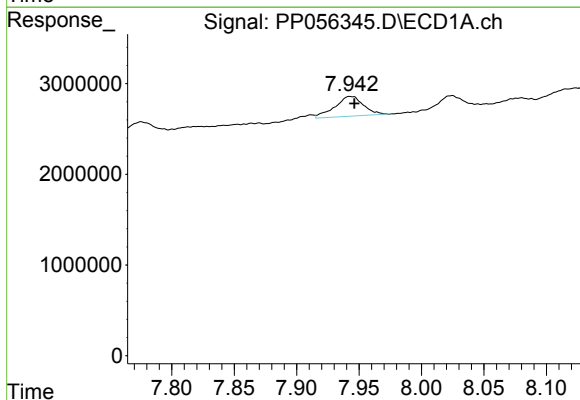


#34 AR-1260-4

R.T.: 7.942 min
Delta R.T.: -0.004 min
Response: 3480606
Conc: 35.21 ng/ml m

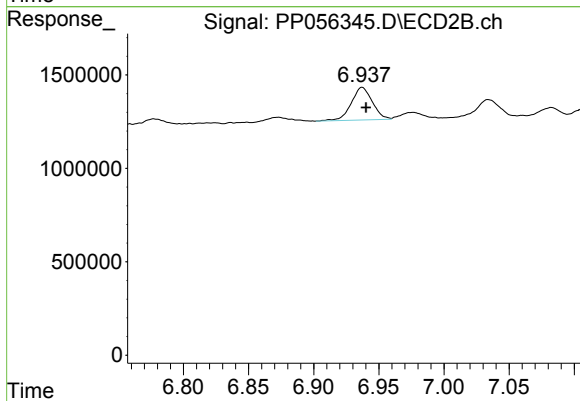

#34 AR-1260-4

R.T.: 6.937 min
Delta R.T.: -0.003 min
Response: 1966944
Conc: 32.80 ng/ml

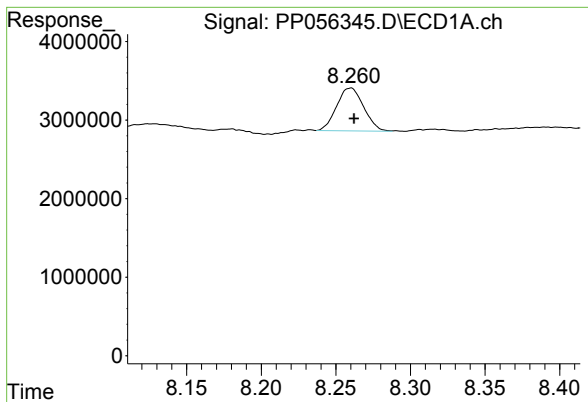


#35 AR-1260-5

R.T.: 8.260 min
Delta R.T.: -0.002 min
Response: 6889057
Conc: 34.47 ng/ml

Instrument :
ECD_P
ClientSampleId :
SS-07-20230306

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/10/2023
Supervised By :Ankita Jodhani 03/10/2023

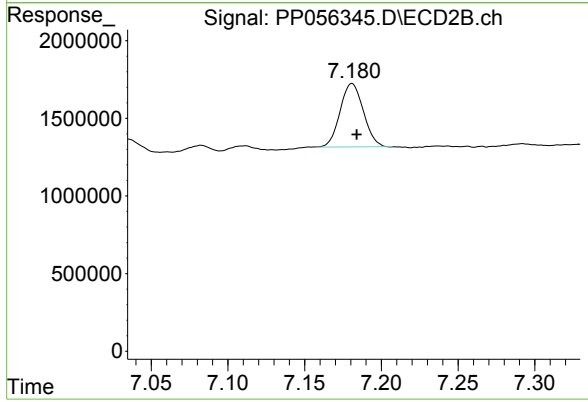

#35 AR-1260-5

R.T.: 7.180 min
Delta R.T.: -0.003 min
Response: 4330200
Conc: 33.89 ng/ml m