

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031023\
 Data File : PP056354.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Mar 2023 14:10
 Operator : YP\AJ
 Sample : 01841-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MORRIS-030823

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/10/2023
 Supervised By :Ankita Jodhani 03/10/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 09 20:22:15 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 08 02:03:40 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.310	3.560	21175214	46844095	13.637m	33.198m#
2) SA Decachlor...	10.060	8.558	41655394	21448044	20.971	19.187

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031023\
Data File : PP056354.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Mar 2023 14:10
Operator : YP\AJ
Sample : 01841-02
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
MORRIS-030823


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/10/2023
Supervised By :Ankita Jodhani 03/10/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 09 20:22:15 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030823.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 08 02:03:40 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

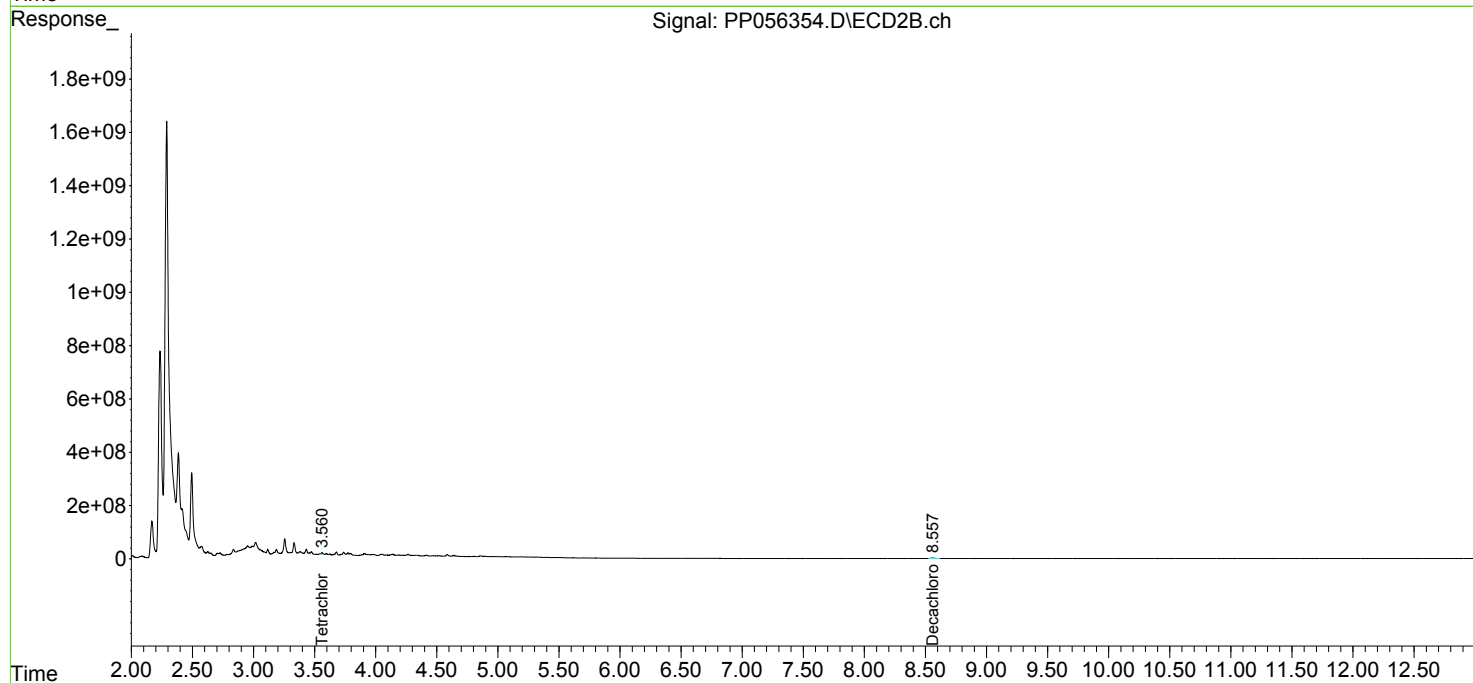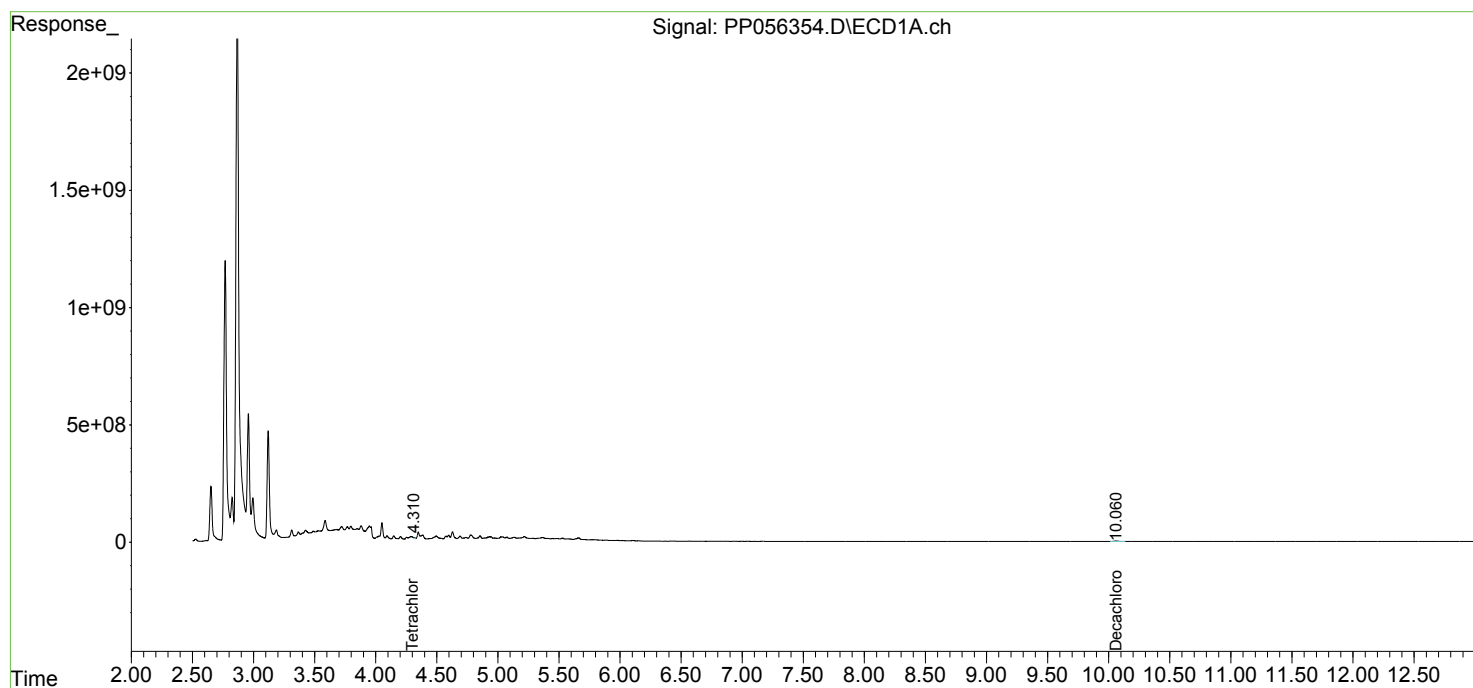

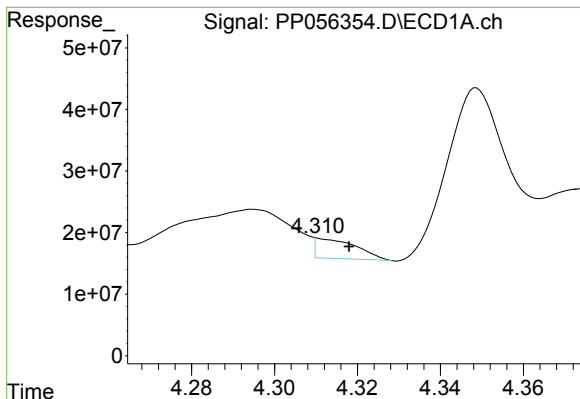


#1 Tetrachloro-m-xylene

R.T.: 4.310 min
Delta R.T.: -0.008 min
Response: 21175214
Conc: 13.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
MORRIS-030823


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/10/2023
Supervised By :Ankita Jodhani 03/10/2023

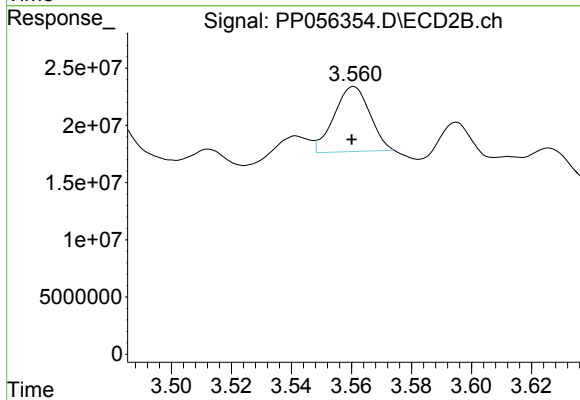


#1 Tetrachloro-m-xylene

R.T.: 3.560 min
Delta R.T.: 0.000 min
Response: 46844095
Conc: 33.20 ng/ml m

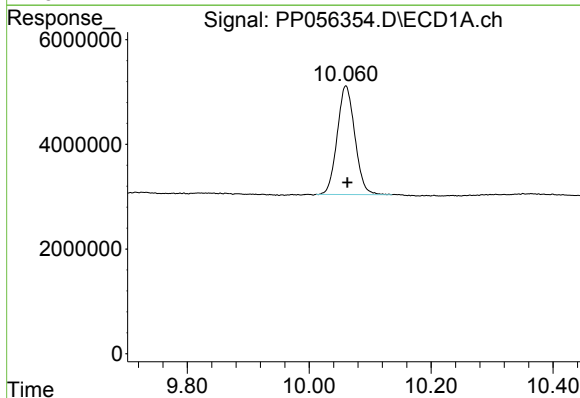

#2 Decachlorobiphenyl

R.T.: 10.060 min
Delta R.T.: -0.002 min
Response: 41655394
Conc: 20.97 ng/ml

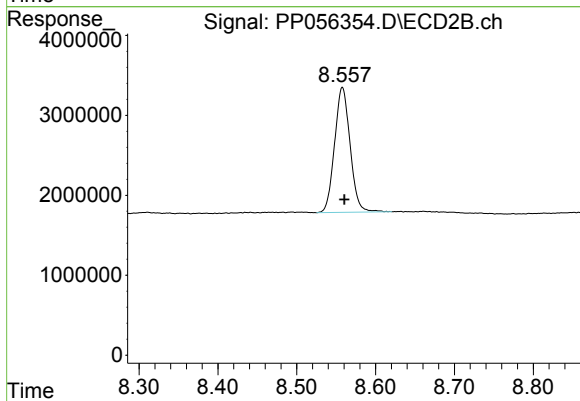

#2 Decachlorobiphenyl

R.T.: 8.558 min
Delta R.T.: -0.003 min
Response: 21448044
Conc: 19.19 ng/ml