

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031023\
 Data File : PP056355.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Mar 2023 14:27
 Operator : YP\AJ
 Sample : 01842-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 VNJ-228

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 03/10/2023
 Supervised By :Ankita Jodhani 03/10/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 09 20:23:34 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 08 02:03:40 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.320	3.563	34861631	28882029	22.452	20.468
2) SA Decachlor...	10.061	8.557	30697521	17413548	15.454	15.578m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031023\
Data File : PP056355.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Mar 2023 14:27
Operator : YP\AJ
Sample : 01842-01
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
VNJ-228


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/10/2023
Supervised By :Ankita Jodhani 03/10/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 09 20:23:34 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030823.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 08 02:03:40 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

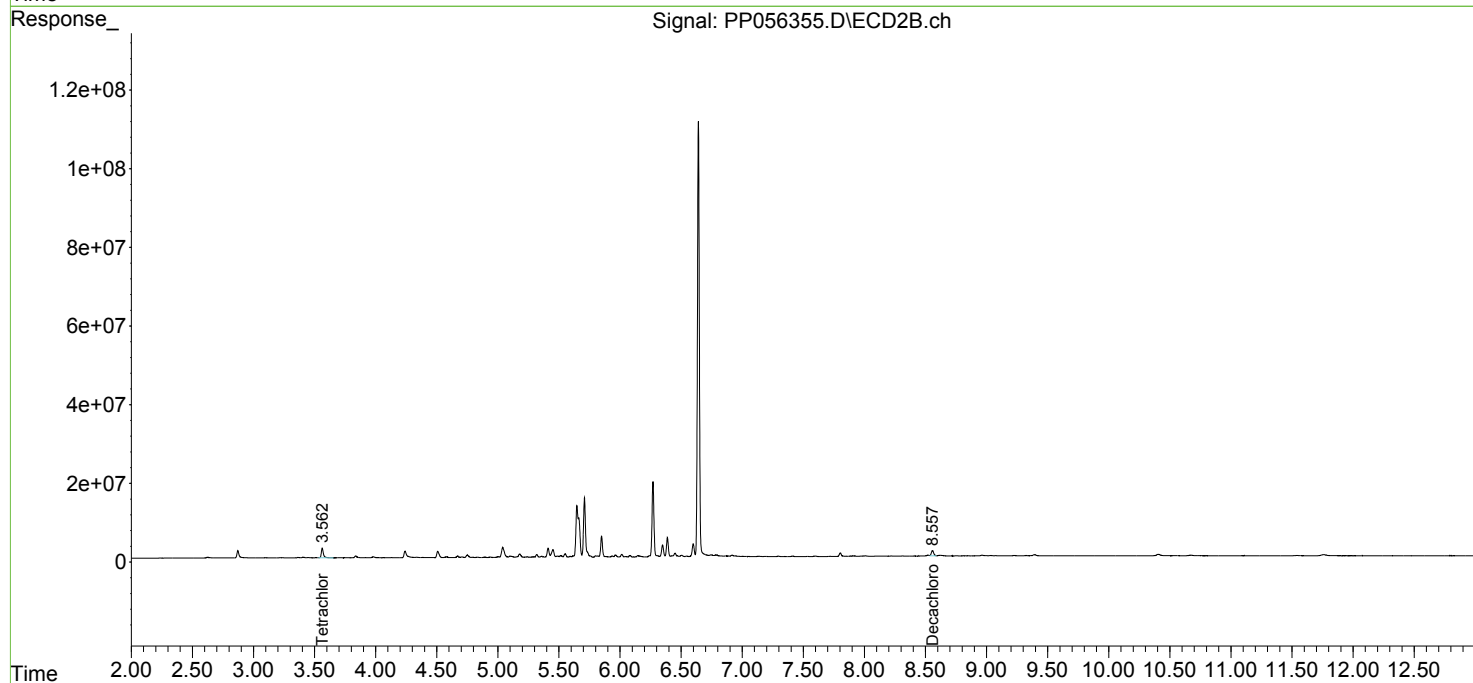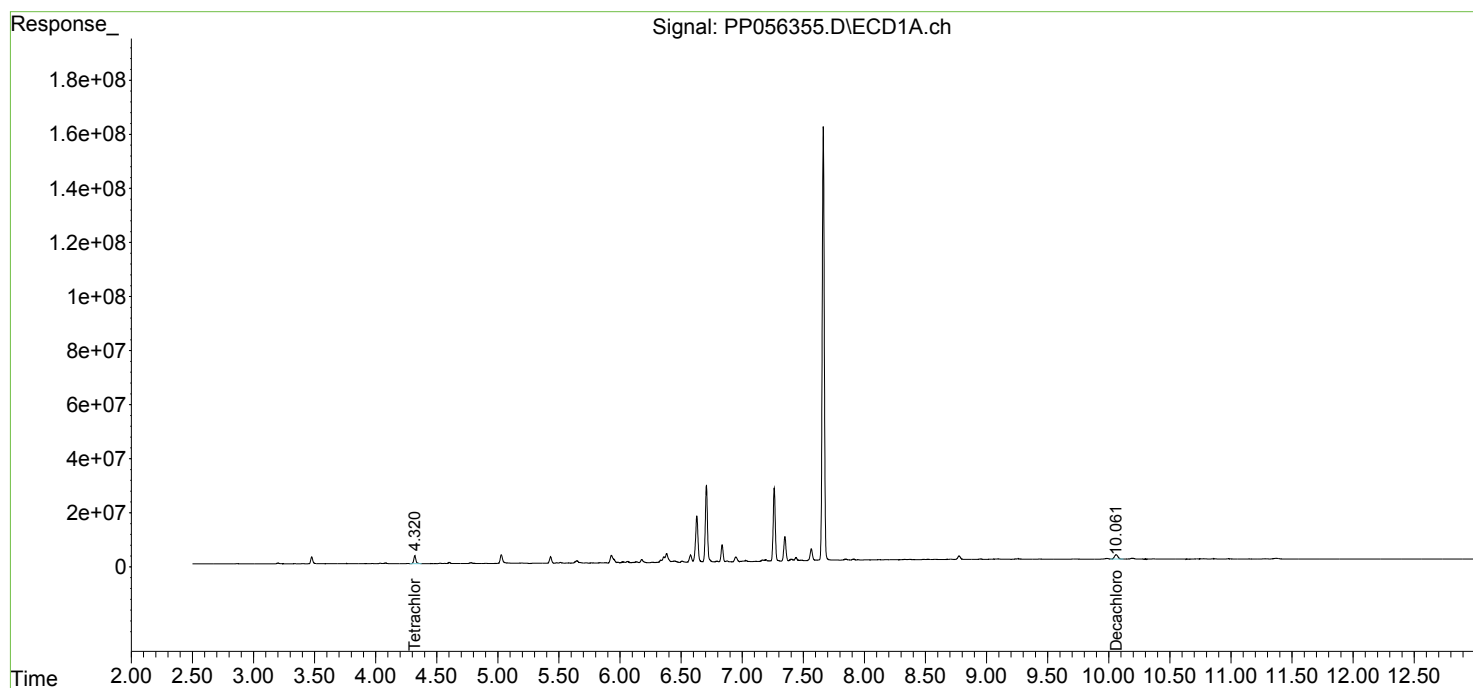

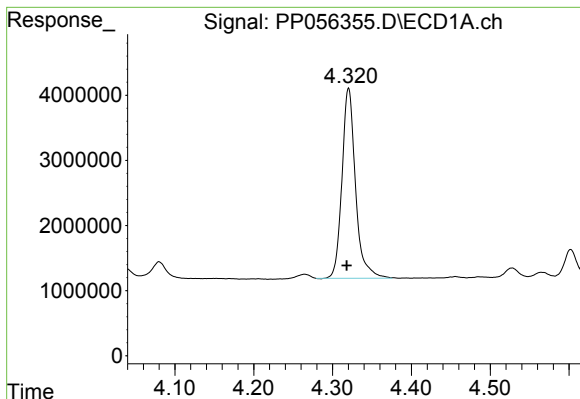


#1 Tetrachloro-m-xylene

R.T.: 4.320 min
Delta R.T.: 0.002 min
Response: 34861631
Conc: 22.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
VNJ-228


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 03/10/2023
Supervised By :Ankita Jodhani 03/10/2023

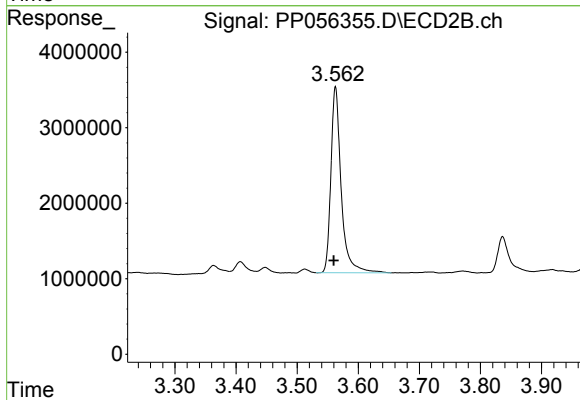


#1 Tetrachloro-m-xylene

R.T.: 3.563 min
Delta R.T.: 0.003 min
Response: 28882029
Conc: 20.47 ng/ml

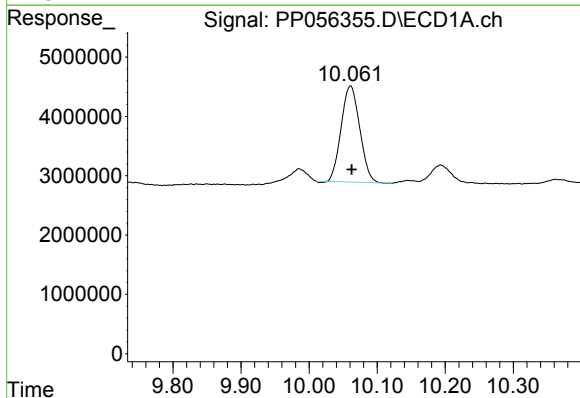

#2 Decachlorobiphenyl

R.T.: 10.061 min
Delta R.T.: -0.002 min
Response: 30697521
Conc: 15.45 ng/ml

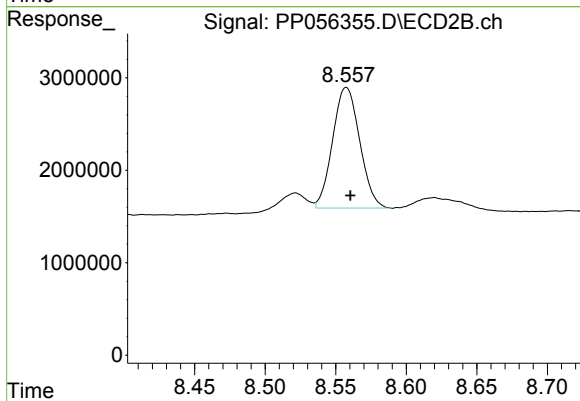

#2 Decachlorobiphenyl

R.T.: 8.557 min
Delta R.T.: -0.003 min
Response: 17413548
Conc: 15.58 ng/ml m