

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031023\
 Data File : PP056370.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Mar 2023 19:06
 Operator : YP\AJ
 Sample : 01852-03
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TT-051-IDWGW-20230308

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 09 20:41:30 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Mar 08 02:03:40 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.319	3.561	29854678	23300428	19.227	16.513
2) SA Decachlor...	10.059	8.557	18089845	11310664	9.107	10.118

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP031023\
Data File : PP056370.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Mar 2023 19:06
Operator : YP\AJ
Sample : 01852-03
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
TT-051-IDWGW-20230308

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 09 20:41:30 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP030823.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Mar 08 02:03:40 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

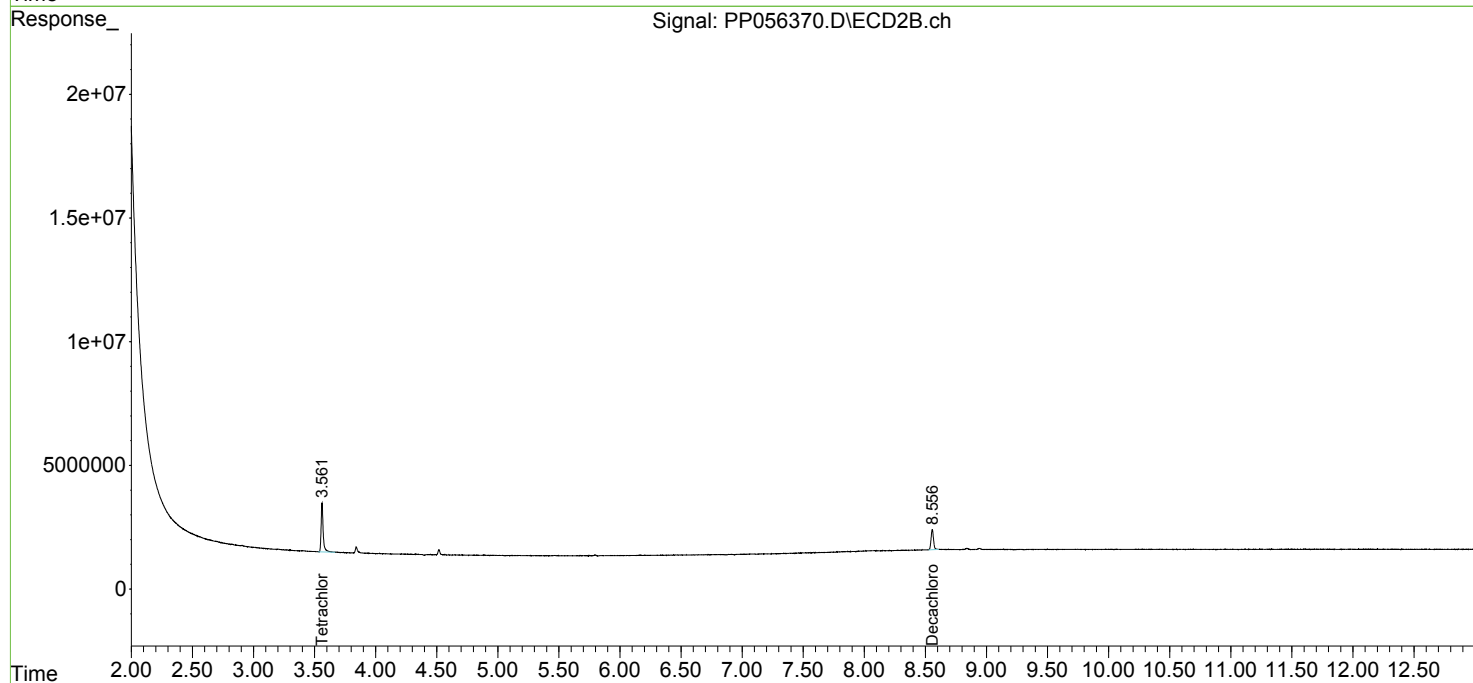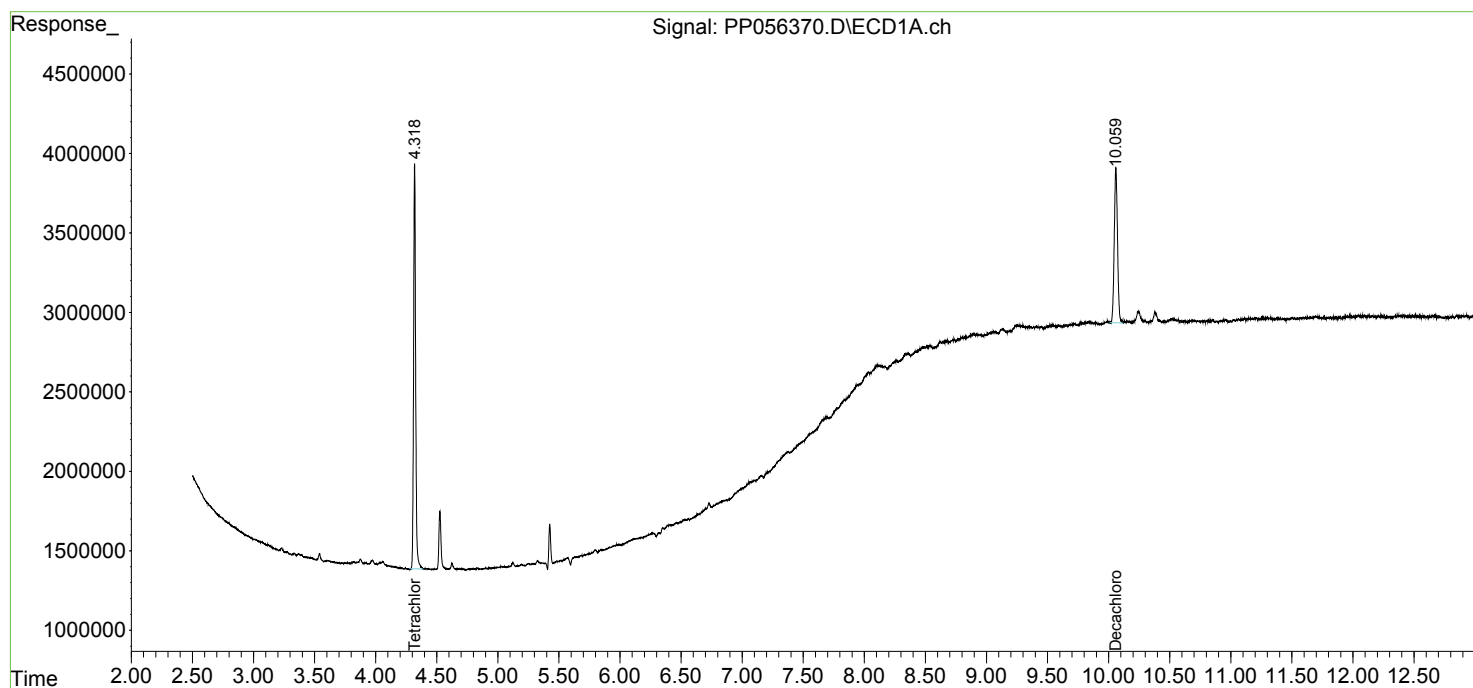


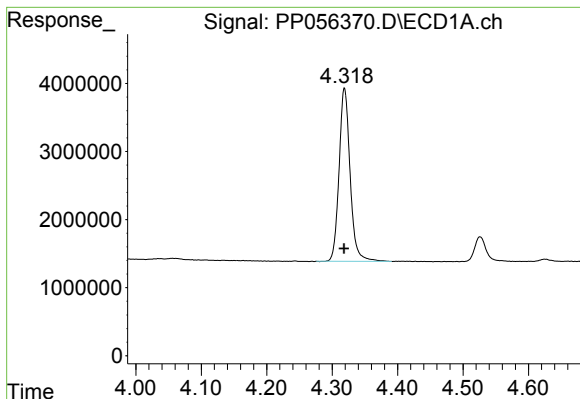

#1 Tetrachloro-m-xylene


R.T.: 4.319 min
Delta R.T.: 0.000 min
Response: 29854678
Conc: 19.23 ng/ml

Instrument :
ECD_P
ClientSampleId :
TT-051-IDWGW-20230308

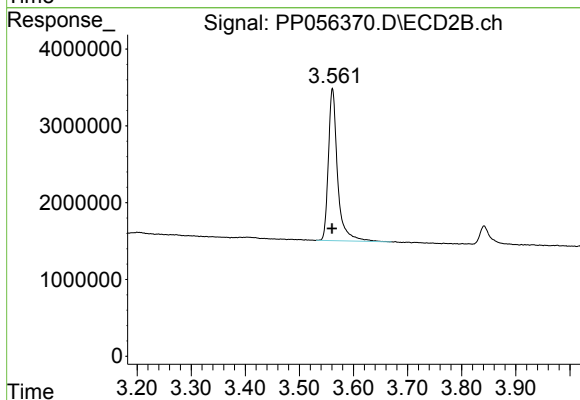


#1 Tetrachloro-m-xylene

R.T.: 3.561 min
Delta R.T.: 0.001 min
Response: 23300428
Conc: 16.51 ng/ml

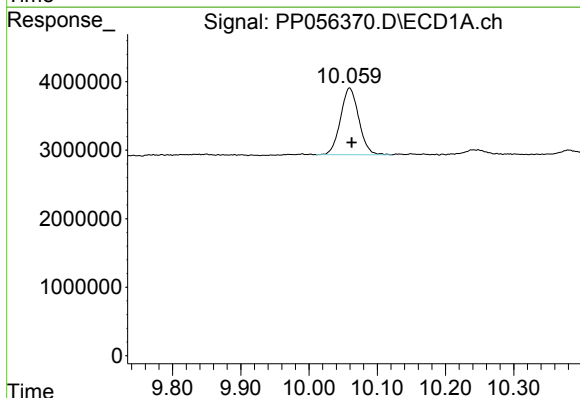

#2 Decachlorobiphenyl

R.T.: 10.059 min
Delta R.T.: -0.003 min
Response: 18089845
Conc: 9.11 ng/ml

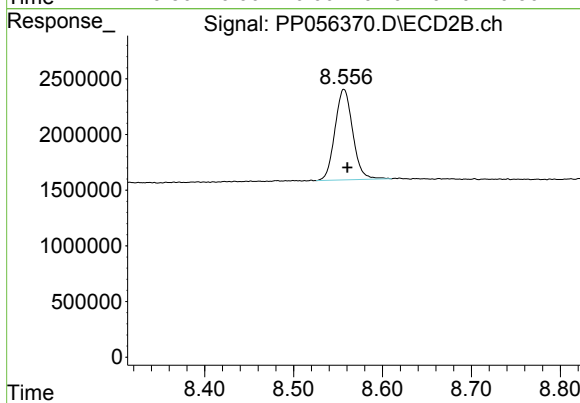

#2 Decachlorobiphenyl

R.T.: 8.557 min
Delta R.T.: -0.004 min
Response: 11310664
Conc: 10.12 ng/ml